

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013183.D
 Acq On : 21 Dec 2022 00:28
 Operator : CG/JU
 Sample : N5984-11
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COLD6

Quant Time: Dec 21 03:34:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 19 21:43:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	526440	20.000	ng/u1	0.00
20) Naphthalene-d8	10.763	136	2213186	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.593	164	1409412	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.351	188	2847334	20.000	ng/u1	0.00
79) Chrysene-d12	21.433	240	2075433	20.000	ng/u1	0.00
88) Perylene-d12	23.916	264	2485370	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	60998	4.954	ng/uL	0.00
4) Pyridine-d5	3.764	84	959219	27.425	ng/u1	0.00
7) Phenol-d5	7.111	99	1279640	29.842	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	795623	30.759	ng/u1	0.00
11) 2-Chlorophenol-d4	7.481	132	1031842	30.568	ng/u1	0.00
15) 4-Methylphenol-d8	8.664	113	1039717	29.592	ng/u1	0.00
21) Nitrobenzene-d5	9.122	128	513221	31.562	ng/u1	0.00
24) 2-Nitrophenol-d4	9.846	143	588913	32.169	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	1073211	30.182	ng/u1	0.00
31) 4-Chloroaniline-d4	10.905	131	1379768	27.486	ng/u1	0.00
46) Dimethylphthalate-d6	13.999	166	3245690	29.964	ng/u1	0.00
49) Acenaphthylene-d8	14.287	160	3700187	31.087	ng/u1	0.00
54) 4-Nitrophenol-d4	14.793	143	430852	22.113	ng/u1	0.00
60) Fluorene-d10	15.587	176	2809020	30.653	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	363336	19.829	ng/u1	0.00
73) Anthracene-d10	17.451	188	4046503	31.501	ng/u1	0.00
81) Pyrene-d10	19.681	212	4129454	34.664	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.757	264	3831017	30.925	ng/u1	0.00
Target Compounds						
71) Pentachlorophenol	16.998	266	69025	3.104	ng/u1	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013183.D
Acq On : 21 Dec 2022 00:28
Operator : CG/JU
Sample : N5984-11
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COLD6

Quant Time: Dec 21 03:34:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 19 21:43:11 2022
Response via : Initial Calibration

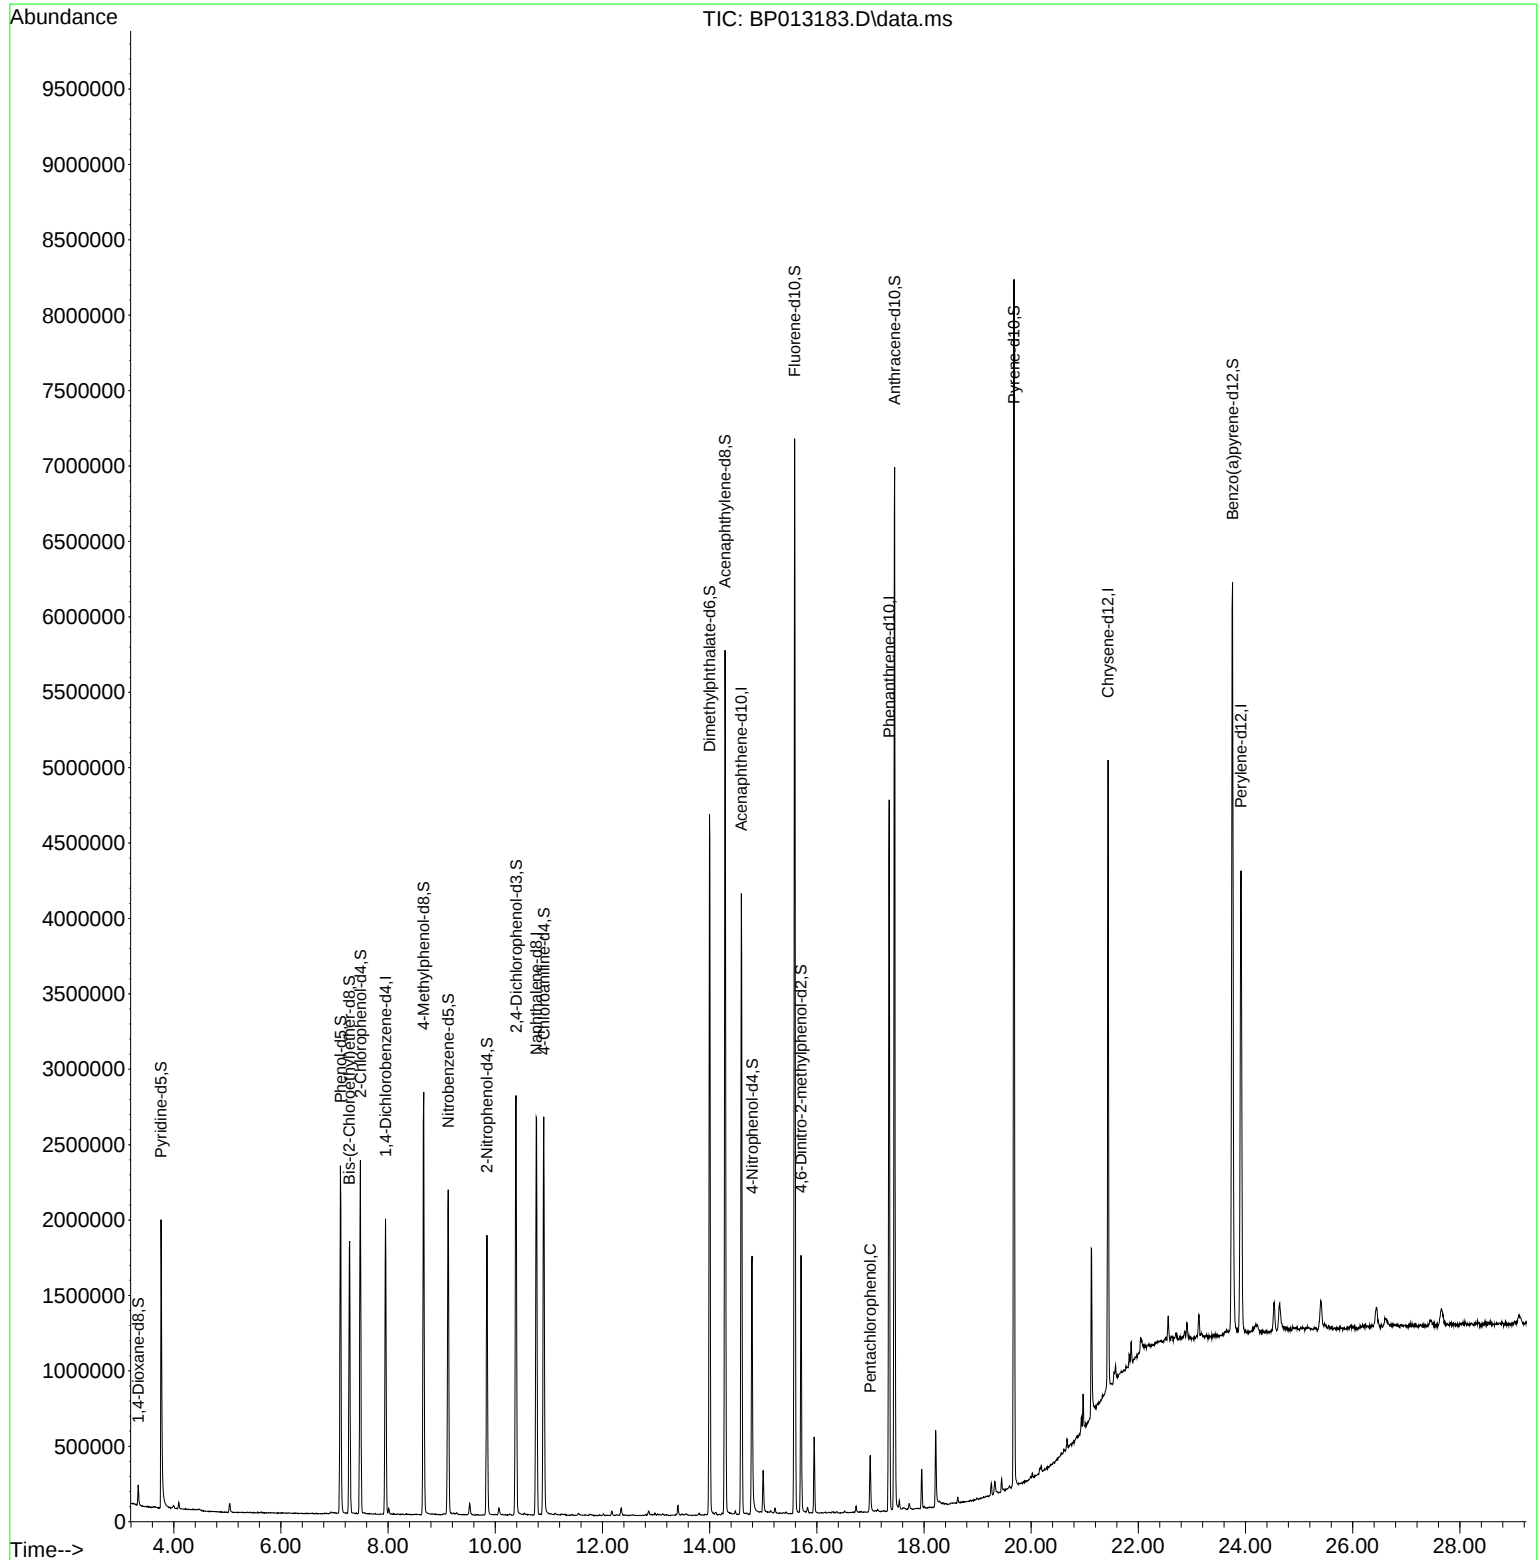

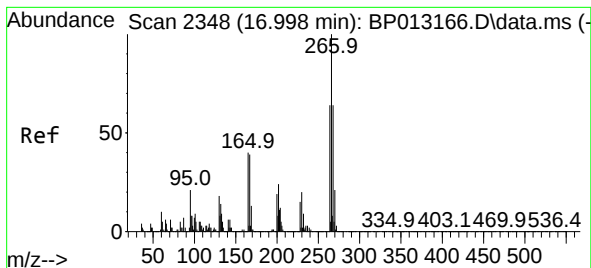

#71

Pentachlorophenol

Concen: 3.104 ng/ul

RT: 16.998 min Scan# 2348

Delta R.T. 0.000 min

Lab File: BP013183.D


Acq: 21 Dec 2022 00:28

Instrument :

BNA_P

ClientSampleId :

COLD6

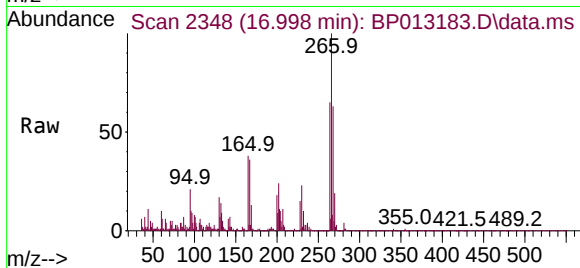

Tgt Ion:266 Resp: 69025

Ion Ratio Lower Upper

266 100

264 65.0 50.9 76.3

268 63.4 51.4 77.2

