

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013192.D
 Acq On : 21 Dec 2022 06:08
 Operator : CG/JU
 Sample : N5984-05
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0LC9

Quant Time: Dec 21 06:37:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 19 21:43:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	535444	20.000	ng/u1	0.00
20) Naphthalene-d8	10.763	136	2167495	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.592	164	1184886	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.351	188	2249642	20.000	ng/u1	0.00
79) Chrysene-d12	21.433	240	2082440	20.000	ng/u1	0.00
88) Perylene-d12	23.915	264	2536021	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	52974	4.230	ng/uL	0.00
4) Pyridine-d5	3.775	84	121816	3.424	ng/u1	0.01
7) Phenol-d5	7.110	99	1105027	25.337	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	708659	26.936	ng/u1	0.00
11) 2-Chlorophenol-d4	7.481	132	890287	25.931	ng/u1	0.00
15) 4-Methylphenol-d8	8.657	113	810969	22.694	ng/u1	-0.01
21) Nitrobenzene-d5	9.122	128	431972	27.125	ng/u1	0.00
24) 2-Nitrophenol-d4	9.845	143	493175	27.508	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	899889	25.841	ng/u1	0.00
31) 4-Chloroaniline-d4	10.904	131	760582	15.471	ng/u1	0.00
46) Dimethylphthalate-d6	13.998	166	2545570	27.954	ng/u1	0.00
49) Acenaphthylene-d8	14.286	160	2904659	29.028	ng/u1	0.00
54) 4-Nitrophenol-d4	14.792	143	324902	19.835	ng/u1	0.00
60) Fluorene-d10	15.586	176	2157328	28.003	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	333454	23.033	ng/u1	0.00
73) Anthracene-d10	17.451	188	3029822	29.853	ng/u1	0.00
81) Pyrene-d10	19.680	212	3480565	29.118	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.756	264	3792465	30.002	ng/u1	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	17.010	266	9468301	538.963	ng/u1	99
82) Pyrene	19.710	202	147329	1.053	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013192.D
Acq On : 21 Dec 2022 06:08
Operator : CG/JU
Sample : N5984-05
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0LC9

Quant Time: Dec 21 06:37:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 19 21:43:11 2022
Response via : Initial Calibration

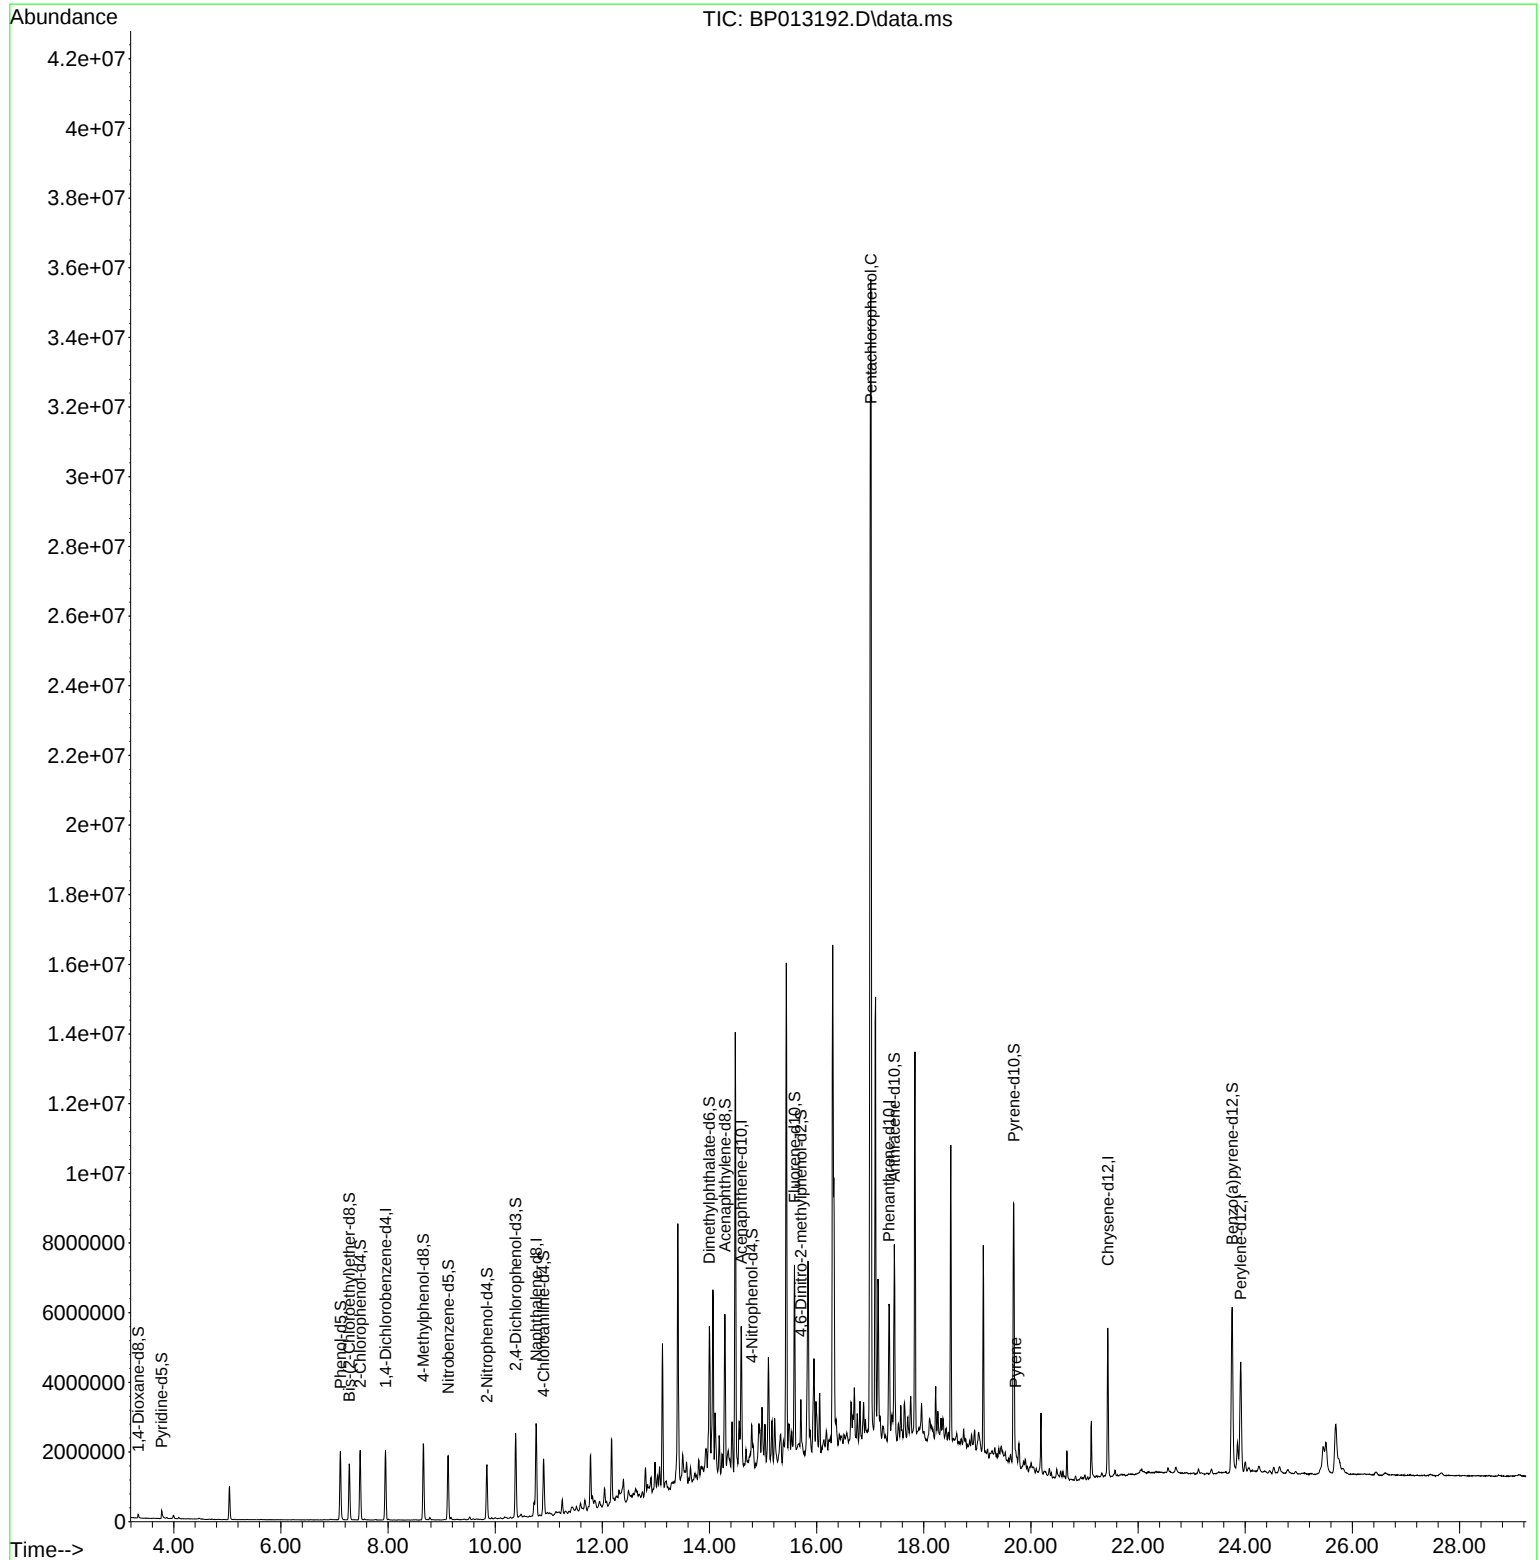

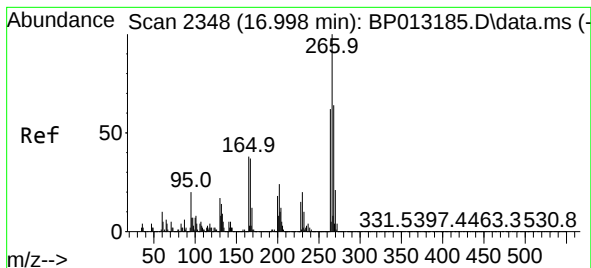

#71

Pentachlorophenol

Concen: 538.963 ng/ul

RT: 17.010 min Scan# 2348

Delta R.T. 0.012 min

Lab File: BP013192.D

Acq: 21 Dec 2022 06:08

Instrument :

BNA_P

ClientSampleId :

C0LC9





Tgt Ion:266 Resp: 9468301

Ion Ratio Lower Upper

266 100

264 64.4 50.9 76.3

268 65.0 51.4 77.2

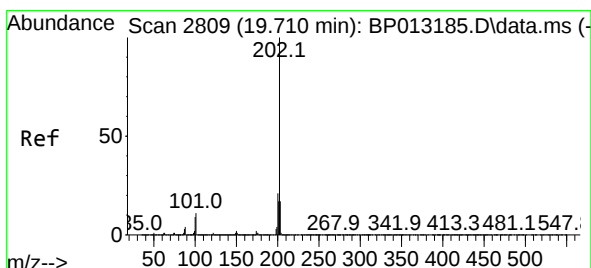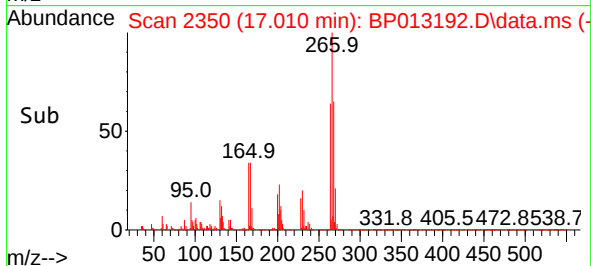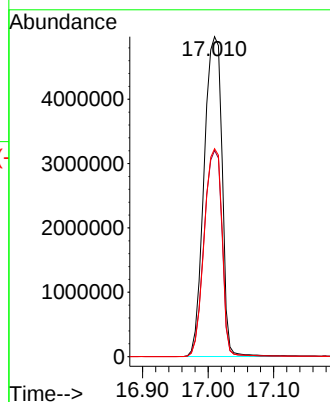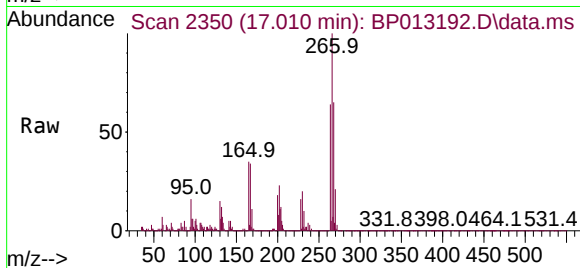

#82

Pyrene

Concen: 1.053 ng/ul

RT: 19.710 min Scan# 2809

Delta R.T. -0.006 min

Lab File: BP013192.D

Acq: 21 Dec 2022 06:08

Tgt Ion:202 Resp: 147329

Ion Ratio Lower Upper

202 100

101 12.5 9.4 14.2

100 9.1 7.8 11.8

