

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013197.D
 Acq On : 21 Dec 2022 08:58
 Operator : CG/JU
 Sample : N5984-14
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COLFO

Quant Time: Dec 21 21:50:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 19 21:43:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	553083	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136	2174443	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.592	164	1149456	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.351	188	2202196	20.000	ng/ul	0.00
79) Chrysene-d12	21.433	240	2283013	20.000	ng/ul	0.00
88) Perylene-d12	23.916	264	2702670	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	47305	3.657	ng/uL	0.00
4) Pyridine-d5	3.770	84	230991	6.286	ng/ul	0.00
7) Phenol-d5	7.111	99	924385	20.519	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	590421	21.726	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	754893	21.286	ng/ul	0.00
15) 4-Methylphenol-d8	8.658	113	668793	18.118	ng/ul	-0.01
21) Nitrobenzene-d5	9.116	128	356113	22.290	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.846	143	399861	22.232	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	739102	21.156	ng/ul	0.00
31) 4-Chloroaniline-d4	10.904	131	713164	14.460	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	2040788	23.101	ng/ul	0.00
49) Acenaphthylene-d8	14.287	160	2343794	24.145	ng/ul	0.00
54) 4-Nitrophenol-d4	14.787	143	253388	15.946	ng/ul	0.00
60) Fluorene-d10	15.587	176	1732781	23.185	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	253689	17.901	ng/ul	0.00
73) Anthracene-d10	17.451	188	2501104	25.174	ng/ul	0.00
81) Pyrene-d10	19.680	212	3098420	23.644	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.751	264	3415544	25.354	ng/ul	-0.01
Target Compounds						
					Qvalue	
71) Pentachlorophenol	17.010	266	8004551	465.459	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013197.D
Acq On : 21 Dec 2022 08:58
Operator : CG/JU
Sample : N5984-14
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COLFO

Quant Time: Dec 21 21:50:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 19 21:43:11 2022
Response via : Initial Calibration

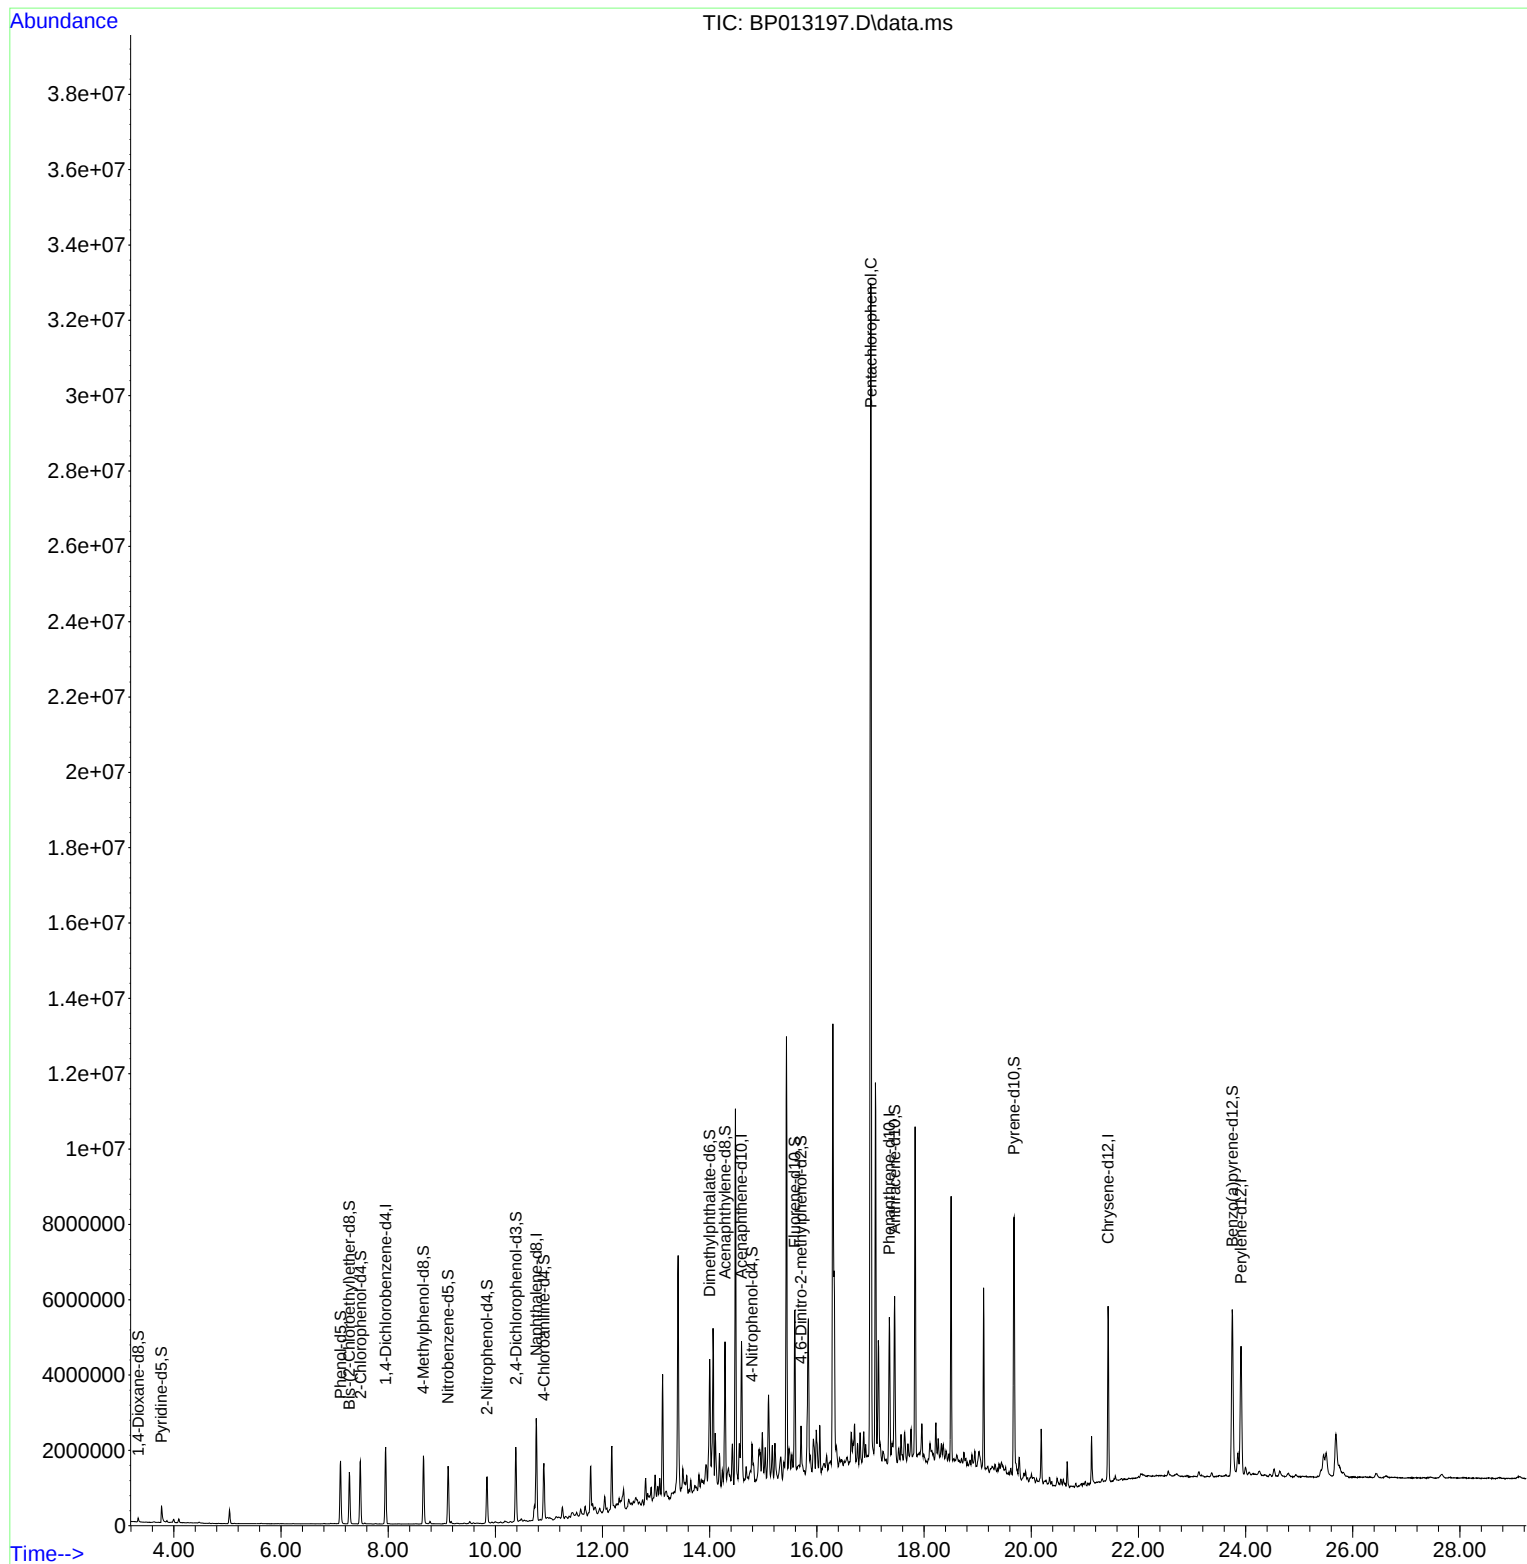

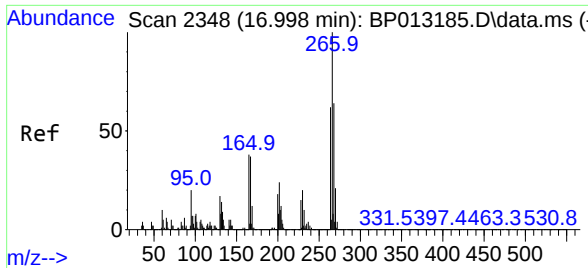

#71
 Pentachlorophenol
 Concen: 465.459 ng/ul
 RT: 17.010 min Scan# 21
 Delta R.T. 0.012 min
 Lab File: BP013197.D
 Acq: 21 Dec 2022 08:58

Instrument :
 BNA_P
 ClientSampleId :
 COLFO

Tgt Ion:266 Resp: 8004551

Ion	Ratio	Lower	Upper
266	100		
264	64.0	50.9	76.3
268	64.3	51.4	77.2

