

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013123.D
 Acq On : 19 Dec 2022 12:51
 Operator : CG/JU
 Sample : PB149588BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK588

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013123.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	22	26	33	rVB	128081	177861	1.41%	0.142%
2	3.764	95	98	120	rBV	1577657	2402774	19.09%	1.916%
3	4.099	151	155	162	rVB	90596	127051	1.01%	0.101%
4	7.111	660	667	680	rBV	1924281	2948240	23.42%	2.351%
5	7.281	688	696	707	rBV	1622667	2487561	19.76%	1.984%
6	7.481	723	730	743	rBV	1885336	3050484	24.23%	2.432%
7	7.958	803	811	821	rBV	1752989	2725072	21.65%	2.173%
8	8.663	923	931	943	rBV	2340513	3657003	29.05%	2.916%
9	8.769	948	949	960	rVB10	11033	23916	0.19%	0.019%
10	9.122	1000	1009	1021	rBV	1809961	2927930	23.26%	2.335%
11	9.852	1122	1133	1142	rBV	1467102	2408090	19.13%	1.920%
12	10.387	1217	1224	1242	rBV	2323265	3813775	30.29%	3.041%
13	10.769	1279	1289	1297	rBV	2390683	3994694	31.73%	3.185%
14	10.910	1305	1313	1328	rBV	2189711	3784095	30.06%	3.017%
15	11.105	1340	1346	1352	rVB	7160	13024	0.10%	0.010%
16	12.357	1553	1559	1565	rVB2	38054	66703	0.53%	0.053%
17	12.646	1603	1608	1613	rBV5	10170	16855	0.13%	0.013%
18	13.222	1700	1706	1712	rBV4	13002	22877	0.18%	0.018%
19	13.399	1730	1736	1739	rBV7	10453	19663	0.16%	0.016%
20	13.434	1739	1742	1746	rVV3	10033	14138	0.11%	0.011%
21	13.481	1746	1750	1754	rVB5	10572	15169	0.12%	0.012%
22	13.569	1761	1765	1770	rVB6	8650	12882	0.10%	0.010%
23	14.004	1832	1839	1851	rBV	4626790	6113928	48.56%	4.875%
24	14.110	1855	1857	1863	rVV7	7194	13055	0.10%	0.010%
25	14.293	1879	1888	1899	rBV	4822833	6967921	55.35%	5.556%
26	14.598	1933	1940	1947	rBV	3772489	5525693	43.89%	4.406%
27	14.663	1948	1951	1956	rVB3	13870	19505	0.15%	0.016%
28	14.787	1965	1972	1990	rBV	1658234	2614979	20.77%	2.085%
29	14.951	1998	2000	2005	rVV6	9835	14770	0.12%	0.012%
30	14.998	2005	2008	2014	rVB3	20041	33300	0.26%	0.027%
31	15.222	2042	2046	2051	rVB8	11335	17532	0.14%	0.014%
32	15.410	2072	2078	2082	rBV4	12254	19451	0.15%	0.016%
33	15.593	2101	2109	2116	rBV	6363777	9137582	72.58%	7.286%
34	15.640	2116	2117	2123	rVV4	39639	54473	0.43%	0.043%
35	15.710	2123	2129	2143	rVV	1972528	2724137	21.64%	2.172%
36	15.834	2146	2150	2160	rVB3	33406	73997	0.59%	0.059%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013123.D
 Acq On : 19 Dec 2022 12:51
 Operator : CG/JU
 Sample : PB149588BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK588

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

37	16.381	2237	2243	2247	rBV9	8964	16370	0.13%	0.013%
38	16.534	2266	2269	2278	rVB10	11068	16651	0.13%	0.013%
39	16.657	2286	2290	2293	rVB5	11221	15738	0.13%	0.013%
40	16.810	2313	2316	2321	rBV5	10859	20282	0.16%	0.016%
41	16.998	2343	2348	2351	rBV6	16878	26950	0.21%	0.021%
42	17.028	2351	2353	2359	rVB7	10716	14934	0.12%	0.012%
43	17.134	2370	2371	2380	rVB5	10916	16458	0.13%	0.013%
44	17.351	2401	2408	2419	rBV	4840707	7000313	55.60%	5.582%
45	17.451	2419	2425	2444	rVV	7331570	10207478	81.08%	8.139%
46	18.298	2566	2569	2574	rBV4	14201	20589	0.16%	0.016%
47	19.263	2729	2733	2738	rBV	85269	106491	0.85%	0.085%
48	19.328	2740	2744	2748	rBV	87409	124871	0.99%	0.100%
49	19.686	2799	2805	2818	rBV	9708987	12589813	100.00%	10.039%
50	21.439	3098	3103	3114	rBV	5673465	7713744	61.27%	6.151%
51	23.763	3491	3498	3515	rVV2	5742162	11851290	94.13%	9.450%
52	23.921	3518	3525	3542	rVB2	3562468	7627124	60.58%	6.082%




Sum of corrected areas: 125409276

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013123.D
Acq On : 19 Dec 2022 12:51
Operator : CG/JU
Sample : PB149588BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

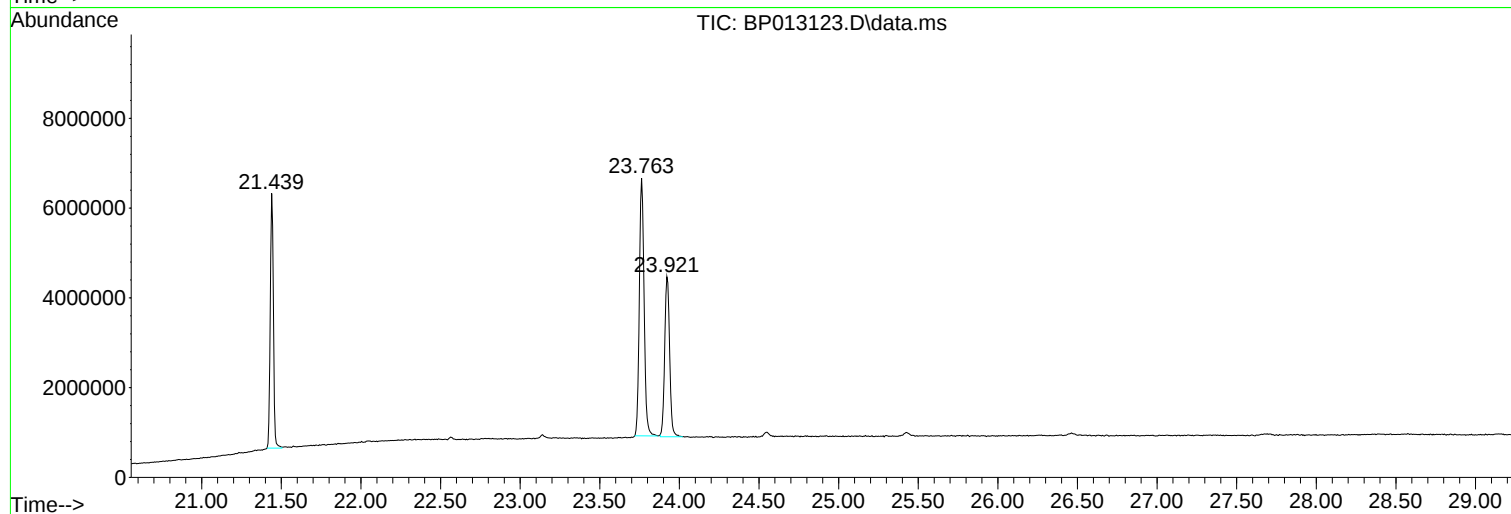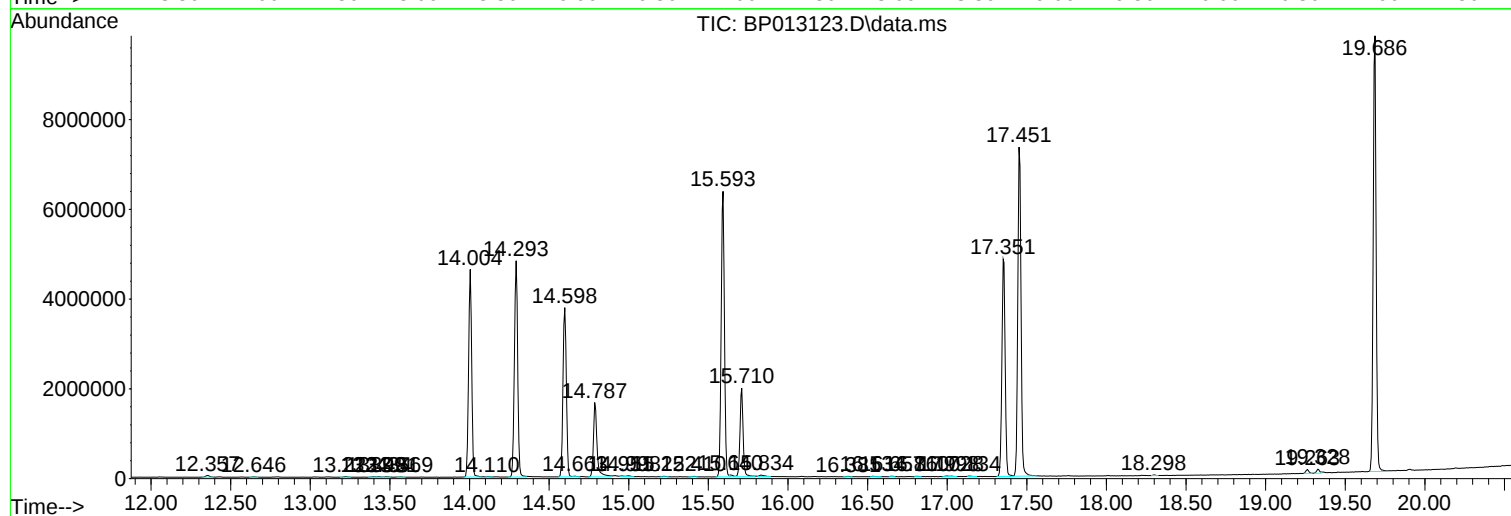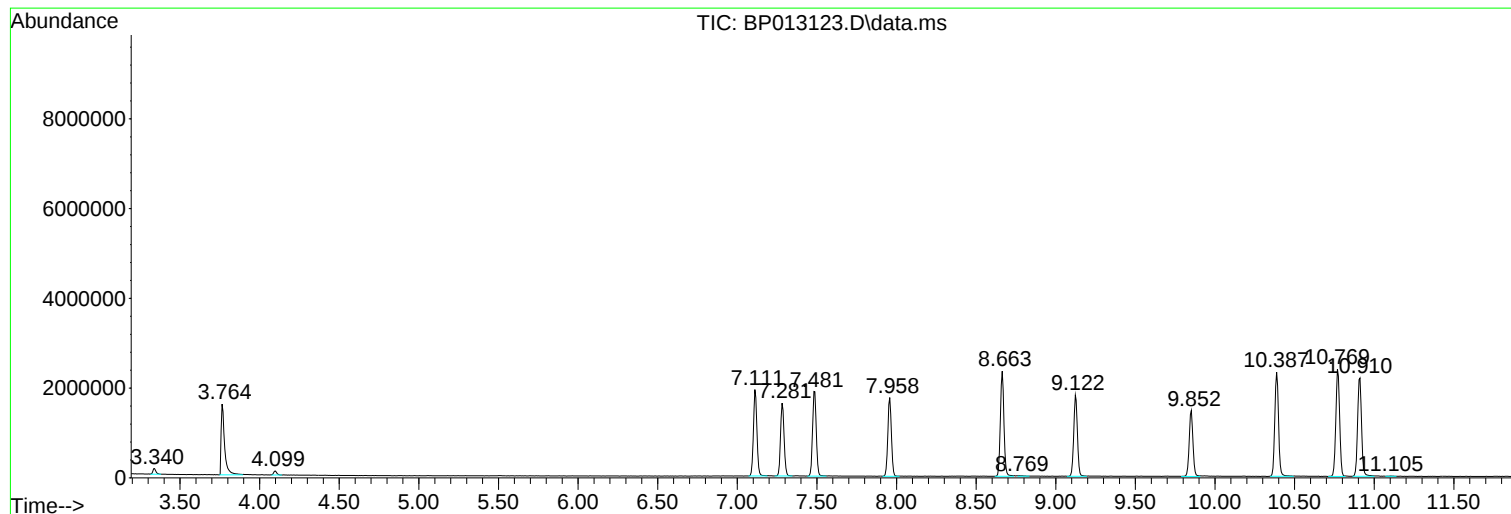

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013123.D
Acq On : 19 Dec 2022 12:51
Operator : CG/JU
Sample : PB149588BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013123.D
Acq On : 19 Dec 2022 12:51
Operator : CG/JU
Sample : PB149588BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------