

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013131.D
 Acq On : 19 Dec 2022 17:47
 Operator : CG/JU
 Sample : PB149638BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK638

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013131.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	22	26	37	rVB	152995	210250	2.09%	0.176%
2	3.764	95	98	115	rBV	1764674	2642712	26.26%	2.209%
3	4.099	150	155	163	rVB	115910	161094	1.60%	0.135%
4	7.116	660	668	678	rBV	2018760	3227410	32.07%	2.698%
5	7.281	690	696	707	rVB	1755468	2736112	27.19%	2.287%
6	7.487	724	731	739	rBV	2114148	3343804	33.23%	2.795%
7	7.958	804	811	819	rBV	2079670	3224164	32.04%	2.695%
8	8.663	924	931	945	rBV	2550443	4058956	40.34%	3.393%
9	9.128	1001	1010	1020	rBV	2004732	3268412	32.48%	2.732%
10	9.852	1124	1133	1146	rBV	1680130	2704393	26.87%	2.261%
11	10.387	1216	1224	1240	rBV	2540867	4215114	41.89%	3.524%
12	10.775	1280	1290	1297	rBV	2748290	4679217	46.50%	3.912%
13	10.910	1305	1313	1335	rBV	2491412	4180706	41.55%	3.495%
14	12.357	1552	1559	1566	rBV	48996	85230	0.85%	0.071%
15	12.575	1590	1596	1601	rVB10	4757	10964	0.11%	0.009%
16	13.398	1730	1736	1740	rBV9	7755	15209	0.15%	0.013%
17	13.487	1745	1751	1755	rVV8	12724	21484	0.21%	0.018%
18	13.575	1762	1766	1772	rVB6	8758	13626	0.14%	0.011%
19	14.004	1833	1839	1851	rBV	4674749	6381300	63.41%	5.334%
20	14.116	1855	1858	1864	rVB8	7266	12289	0.12%	0.010%
21	14.292	1881	1888	1902	rBV	5350519	7575334	75.28%	6.333%
22	14.598	1933	1940	1948	rBV	4354219	6379064	63.39%	5.333%
23	14.792	1966	1973	1990	rBV	1540727	2492548	24.77%	2.084%
24	15.004	2005	2009	2017	rVB6	16900	30728	0.31%	0.026%
25	15.222	2042	2046	2055	rVB6	6344	12861	0.13%	0.011%
26	15.592	2101	2109	2116	rBV	6780920	9478940	94.20%	7.924%
27	15.710	2123	2129	2144	rBV	1977720	2630445	26.14%	2.199%
28	15.834	2146	2150	2156	rVB3	30688	59160	0.59%	0.049%
29	16.381	2238	2243	2248	rVB9	7483	14073	0.14%	0.012%
30	16.657	2284	2290	2295	rBV10	7311	12023	0.12%	0.010%
31	17.139	2366	2372	2378	rBV5	12476	26067	0.26%	0.022%
32	17.357	2402	2409	2419	rBV	5065386	7087624	70.43%	5.925%
33	17.457	2419	2426	2446	rVV	6873177	9693723	96.33%	8.104%
34	18.298	2566	2569	2573	rBV4	12002	18812	0.19%	0.016%
35	19.263	2729	2733	2738	rBV	72866	96576	0.96%	0.081%
36	19.328	2741	2744	2748	rBV	62924	84317	0.84%	0.070%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013131.D
Acq On : 19 Dec 2022 17:47
Operator : CG/JU
Sample : PB149638BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK638

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION

37	19.686	2799	2805	2815	rBV	7884231	10062874	100.00%	8.412%
38	21.439	3098	3103	3115	rBV	4040318	5599587	55.65%	4.681%
39	23.763	3491	3498	3511	rBV	3967367	7683761	76.36%	6.423%
40	23.921	3519	3525	3539	rVB2	2599262	5392482	53.59%	4.508%




Sum of corrected areas: 119623445

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013131.D
Acq On : 19 Dec 2022 17:47
Operator : CG/JU
Sample : PB149638BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK638

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

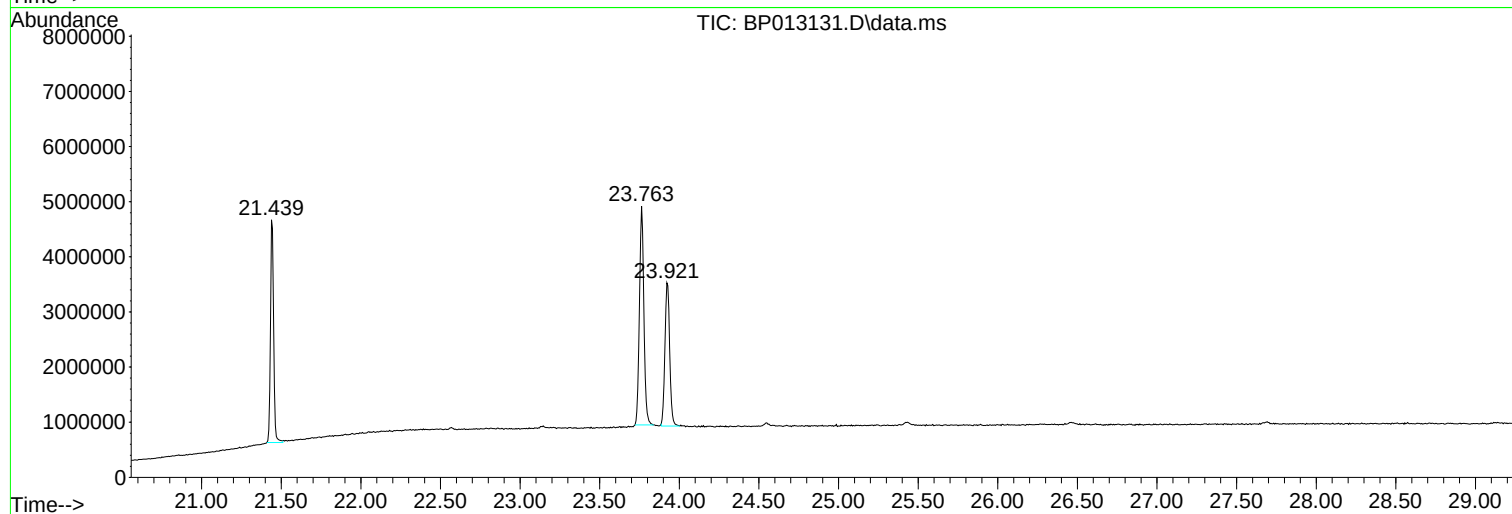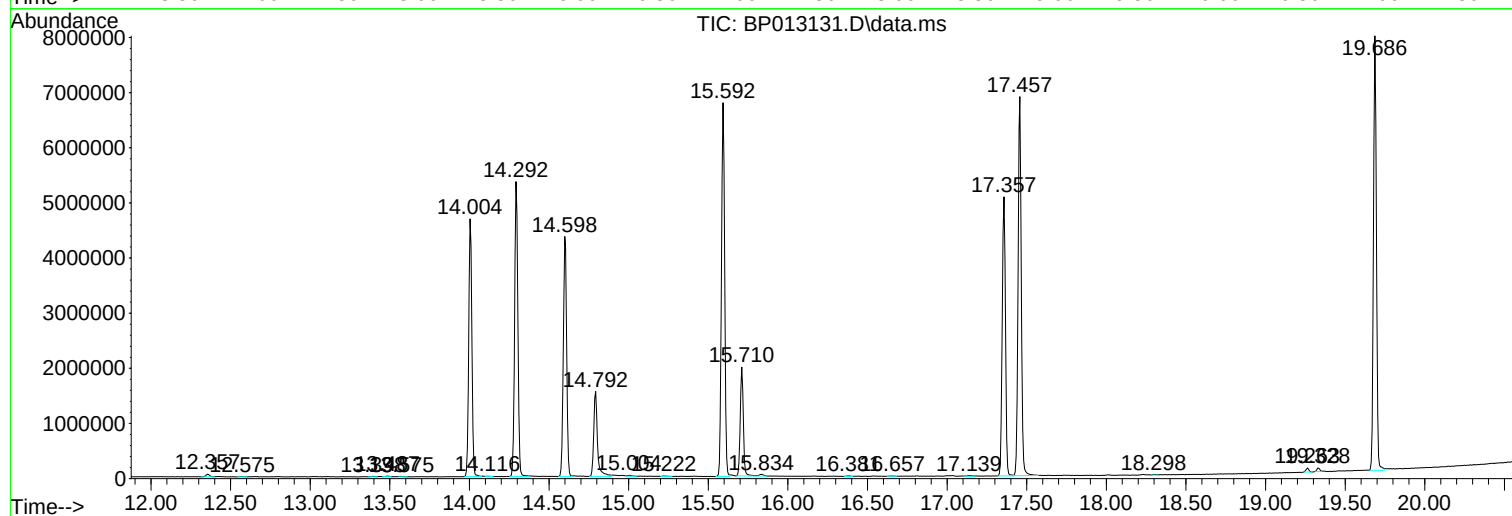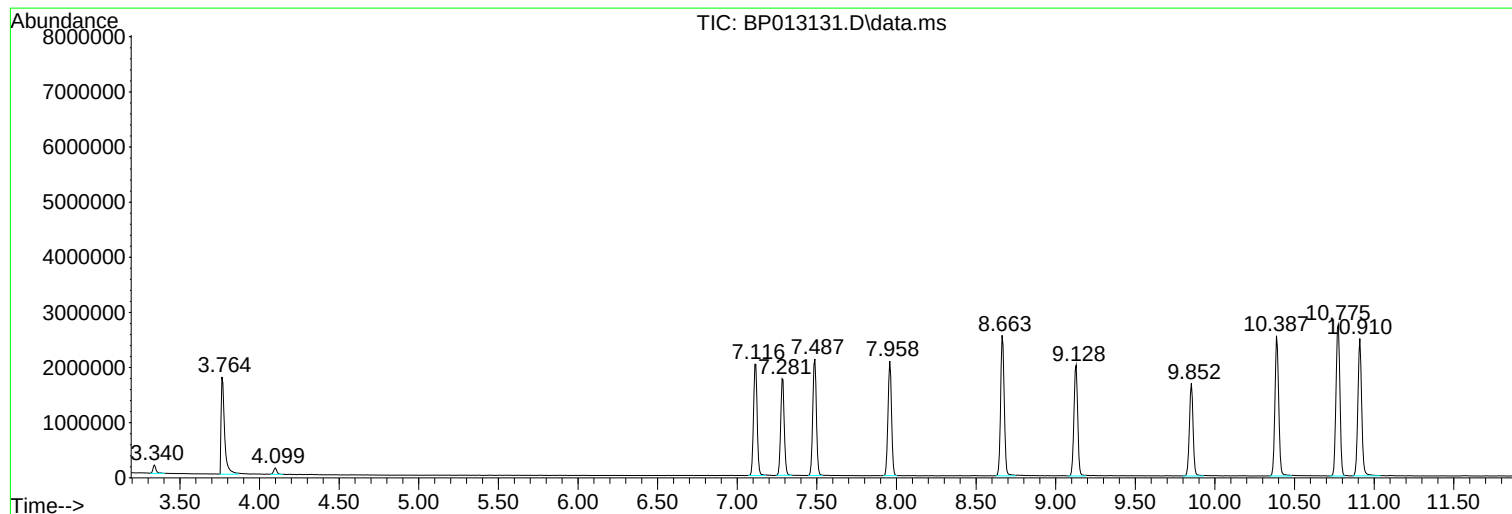

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013131.D
Acq On : 19 Dec 2022 17:47
Operator : CG/JU
Sample : PB149638BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK638

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013131.D
Acq On : 19 Dec 2022 17:47
Operator : CG/JU
Sample : PB149638BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK638

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc