

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013186.D
 Acq On : 21 Dec 2022 02:44
 Operator : CG/JU
 Sample : PB149579BL
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK579

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013186.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	22	25	35	rVB	154206	196952	1.64%	0.161%
2	3.763	94	98	119	rBV	2083662	3060226	25.51%	2.501%
3	4.093	150	154	163	rVB	108090	151842	1.27%	0.124%
4	7.110	659	667	683	rBV	2333923	3567596	29.74%	2.916%
5	7.281	689	696	707	rVB	1841339	2888373	24.08%	2.361%
6	7.481	723	730	740	rBV	2349296	3653482	30.46%	2.986%
7	7.951	801	810	821	rBV	1920166	2988309	24.91%	2.442%
8	8.663	923	931	945	rBV	2738649	4403309	36.71%	3.599%
9	9.122	1001	1009	1021	rBV	2127432	3511867	29.28%	2.870%
10	9.845	1123	1132	1143	rBV	1826798	2957724	24.66%	2.417%
11	10.381	1216	1223	1238	rBV	2711063	4520770	37.69%	3.695%
12	10.763	1278	1288	1300	rBV	2489337	4289726	35.76%	3.506%
13	10.904	1304	1312	1327	rBV	2553301	4339166	36.18%	3.547%
14	12.351	1550	1558	1565	rVB	48291	80404	0.67%	0.066%
15	13.569	1760	1765	1772	rBV7	9081	14467	0.12%	0.012%
16	13.998	1831	1838	1852	rBV	4274970	5926923	49.41%	4.844%
17	14.286	1880	1887	1898	rBV	5043202	7414455	61.82%	6.060%
18	14.592	1932	1939	1952	rBV	3657329	5326744	44.41%	4.354%
19	14.792	1966	1973	1990	rBV	1430266	2415359	20.14%	1.974%
20	15.586	2101	2108	2122	rBV	6274135	8870578	73.96%	7.250%
21	15.704	2122	2128	2140	rVV	1563615	2065136	17.22%	1.688%
22	15.828	2145	2149	2156	rVB2	29462	51456	0.43%	0.042%
23	17.133	2367	2371	2375	rBV3	8761	12255	0.10%	0.010%
24	17.351	2400	2408	2416	rBV	3913342	5538375	46.17%	4.527%
25	17.451	2418	2425	2440	rVV	5978375	8789678	73.28%	7.184%
26	19.257	2729	2732	2737	rVB3	74056	89109	0.74%	0.073%
27	19.327	2740	2744	2748	rBV	62479	90179	0.75%	0.074%
28	19.680	2798	2804	2816	rBV	7894597	10171084	84.80%	8.313%
29	21.433	3097	3102	3110	rBV	4599468	6081892	50.71%	4.971%
30	23.757	3490	3497	3512	rVB2	5802664	11994370	100.00%	9.803%
31	23.915	3517	3524	3535	rVB	3356488	6888152	57.43%	5.630%




Sum of corrected areas: 122349958

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013186.D
Acq On : 21 Dec 2022 02:44
Operator : CG/JU
Sample : PB149579BL
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK579

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

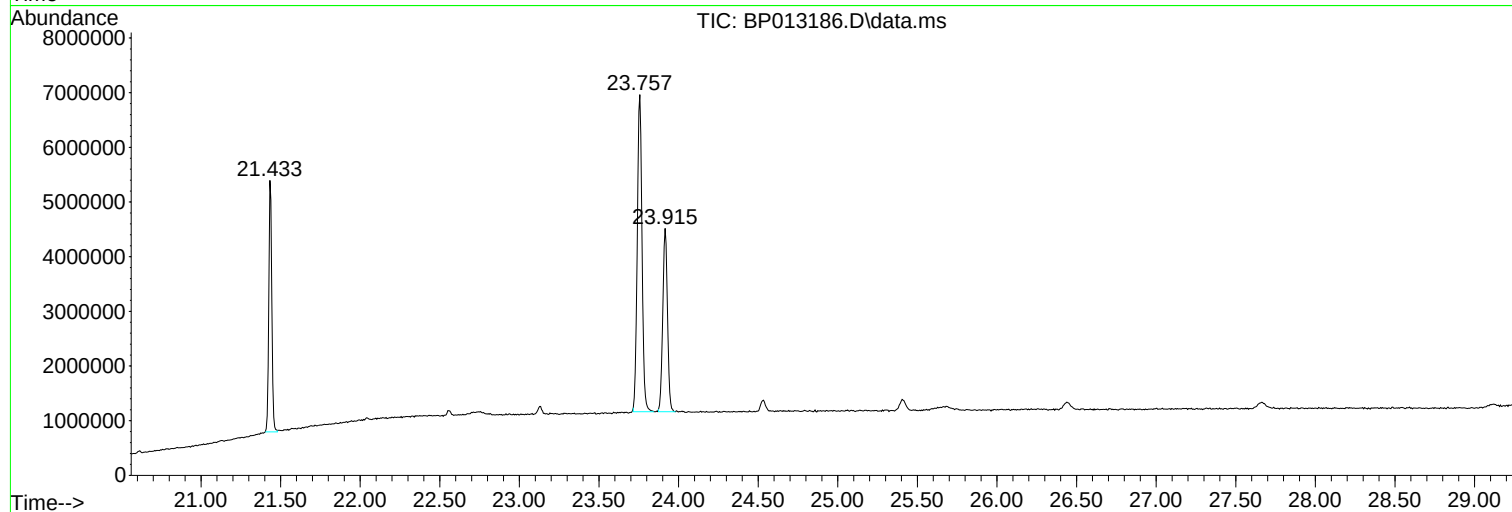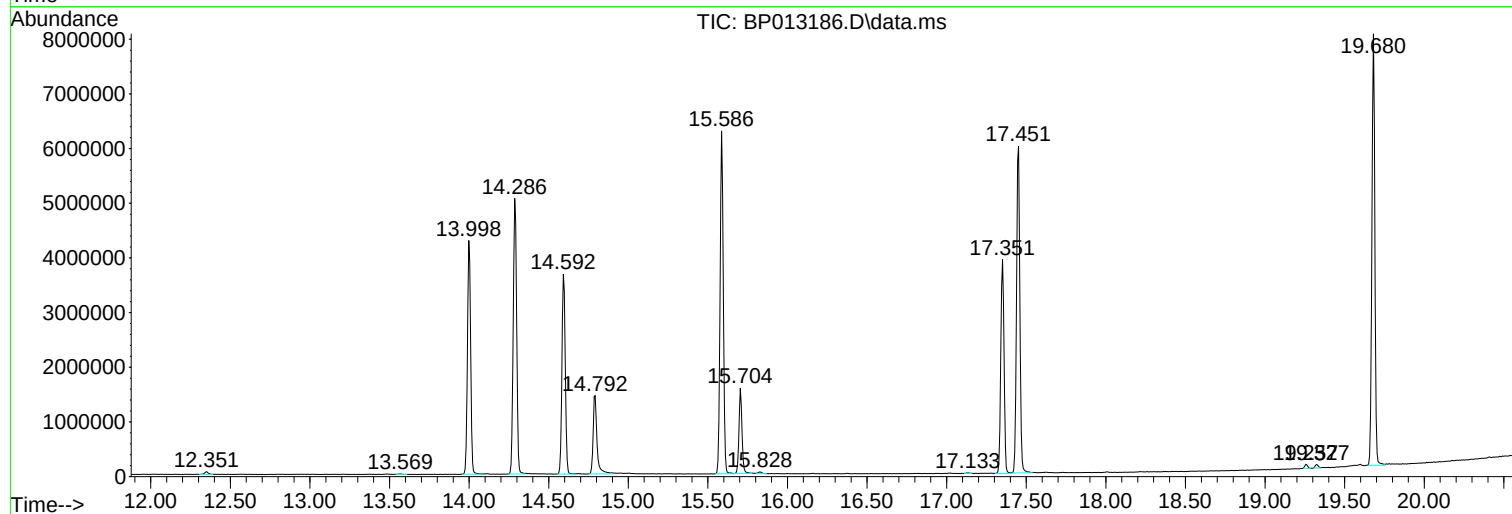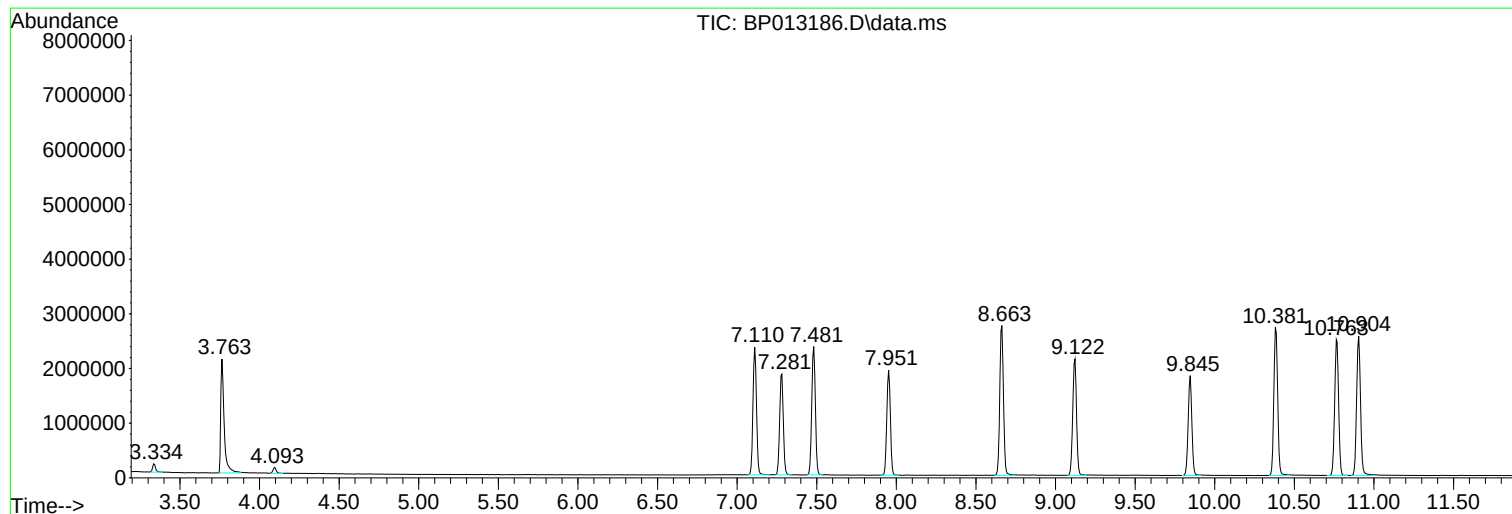

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013186.D
Acq On : 21 Dec 2022 02:44
Operator : CG/JU
Sample : PB149579BL
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK579

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013186.D
Acq On : 21 Dec 2022 02:44
Operator : CG/JU
Sample : PB149579BL
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK579

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc