

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013217.D
 Acq On : 21 Dec 2022 20:20
 Operator : CG/JU
 Sample : N6032-04
 Misc :
 ALS Vial : 99 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COLA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013217.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	17	20	23	rBV2	32289	37707	0.27%	0.028%
2	3.340	23	26	31	rVB	119609	147231	1.04%	0.109%
3	3.781	99	101	115	rBV	98011	165475	1.17%	0.123%
4	3.999	133	138	143	rVB	35320	58687	0.42%	0.044%
5	4.093	150	154	159	rVB	42187	62999	0.45%	0.047%
6	5.040	310	315	320	rVB2	51178	77831	0.55%	0.058%
7	5.852	450	453	460	rVB	11767	20433	0.14%	0.015%
8	7.111	659	667	673	rBV	507332	832470	5.90%	0.618%
9	7.275	688	695	705	rBV	1980797	3017428	21.38%	2.239%
10	7.475	722	729	737	rBV	1547810	2461153	17.44%	1.826%
11	7.952	802	810	817	rBV	2251184	3563329	25.24%	2.644%
12	8.011	817	820	828	rVB5	21482	35518	0.25%	0.026%
13	8.552	906	912	918	rVB8	10710	19923	0.14%	0.015%
14	8.658	921	930	943	rBV	1312723	2081289	14.74%	1.544%
15	8.781	947	951	957	rVB	22134	35073	0.25%	0.026%
16	9.052	991	997	1001	rBV4	23693	38429	0.27%	0.029%
17	9.116	1001	1008	1016	rBV	2422263	3940415	27.92%	2.924%
18	9.275	1030	1035	1042	rVB3	45342	75640	0.54%	0.056%
19	9.522	1072	1077	1081	rVB3	14062	23088	0.16%	0.017%
20	9.840	1122	1131	1142	rBV	1391499	2323994	16.46%	1.725%
21	10.381	1214	1223	1237	rBV	2432550	4006029	28.38%	2.973%
22	10.669	1266	1272	1278	rBV6	19554	39503	0.28%	0.029%
23	10.763	1280	1288	1296	rBV	3203178	5380096	38.12%	3.992%
24	10.899	1304	1311	1323	rBV	1023403	1802300	12.77%	1.337%
25	11.422	1396	1400	1408	rBV3	18216	38797	0.27%	0.029%
26	11.493	1408	1412	1417	rBV4	12258	20109	0.14%	0.015%
27	11.557	1417	1423	1432	rVB10	15725	38663	0.27%	0.029%
28	12.046	1503	1506	1510	rVB3	15448	21867	0.15%	0.016%
29	12.346	1552	1557	1564	rBV	54670	88819	0.63%	0.066%
30	12.869	1641	1646	1655	rBV2	41356	77890	0.55%	0.058%
31	12.951	1655	1660	1667	rVB7	8787	17647	0.13%	0.013%
32	13.199	1697	1702	1707	rBV7	13124	25150	0.18%	0.019%
33	13.516	1751	1756	1760	rBV	30008	51404	0.36%	0.038%
34	13.563	1760	1764	1768	rVB6	13454	25710	0.18%	0.019%
35	13.910	1818	1823	1827	rBV8	15986	28092	0.20%	0.021%
36	13.999	1831	1838	1849	rVV	6145806	8294284	58.76%	6.155%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013217.D
 Acq On : 21 Dec 2022 20:20
 Operator : CG/JU
 Sample : N6032-04
 Misc :
 ALS Vial : 99 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COLA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

37	14.116	1854	1858	1861	rVB6	9856	14945	0.11%	0.011%
38	14.287	1880	1887	1907	rVB	7013636	10056585	71.25%	7.463%
39	14.593	1932	1939	1948	rBV	5405774	7744949	54.87%	5.747%
40	14.669	1948	1952	1964	rVB2	60880	96173	0.68%	0.071%
41	14.793	1967	1973	1991	rBV	185685	395910	2.80%	0.294%
42	15.010	2004	2010	2015	rBV6	53551	94393	0.67%	0.070%
43	15.263	2046	2053	2058	rBV	67894	106372	0.75%	0.079%
44	15.387	2070	2074	2075	rBV3	18794	23744	0.17%	0.018%
45	15.587	2100	2108	2120	rBV	9243265	13052717	92.47%	9.686%
46	15.704	2122	2128	2139	rVV	1335190	1823950	12.92%	1.353%
47	15.828	2144	2149	2154	rVB	36978	60464	0.43%	0.045%
48	15.951	2165	2170	2178	rVB2	54881	84277	0.60%	0.063%
49	16.292	2221	2228	2232	rBV9	14123	28462	0.20%	0.021%
50	16.934	2332	2337	2342	rBV3	31953	50707	0.36%	0.038%
51	17.092	2361	2364	2368	rBV6	13821	21138	0.15%	0.016%
52	17.134	2368	2371	2377	rVB3	14583	24588	0.17%	0.018%
53	17.298	2395	2399	2401	rBV2	19959	24394	0.17%	0.018%
54	17.345	2401	2407	2417	rVV	5879511	8348508	59.14%	6.195%
55	17.445	2418	2424	2436	rVV2	9834212	14115360	100.00%	10.475%
56	17.539	2437	2440	2444	rVB5	39047	54816	0.39%	0.041%
57	17.628	2452	2455	2461	rVB3	21997	31580	0.22%	0.023%
58	17.722	2468	2471	2477	rVB7	12002	18413	0.13%	0.014%
59	18.004	2514	2519	2529	rBV	726449	899522	6.37%	0.668%
60	18.216	2551	2555	2563	rBV3	62681	91099	0.65%	0.068%
61	18.292	2564	2568	2570	rBV	35568	44312	0.31%	0.033%
62	18.322	2570	2573	2582	rVB7	26723	51170	0.36%	0.038%
63	18.786	2649	2652	2658	rVB5	56298	64656	0.46%	0.048%
64	19.257	2727	2732	2737	rBV	112643	165190	1.17%	0.123%
65	19.328	2739	2744	2748	rBV	127539	219459	1.55%	0.163%
66	19.445	2762	2764	2769	rBV5	39051	44920	0.32%	0.033%
67	19.681	2798	2804	2815	rBV	10328779	13399810	94.93%	9.944%
68	21.433	3097	3102	3108	rBV	4527306	5803614	41.12%	4.307%
69	23.751	3489	3496	3507	rVB2	5953931	12043936	85.33%	8.937%
70	23.910	3517	3523	3535	rVB2	3257311	6684490	47.36%	4.960%




Sum of corrected areas: 134759095

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013217.D
Acq On : 21 Dec 2022 20:20
Operator : CG/JU
Sample : N6032-04
Misc :
ALS Vial : 99 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COLA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

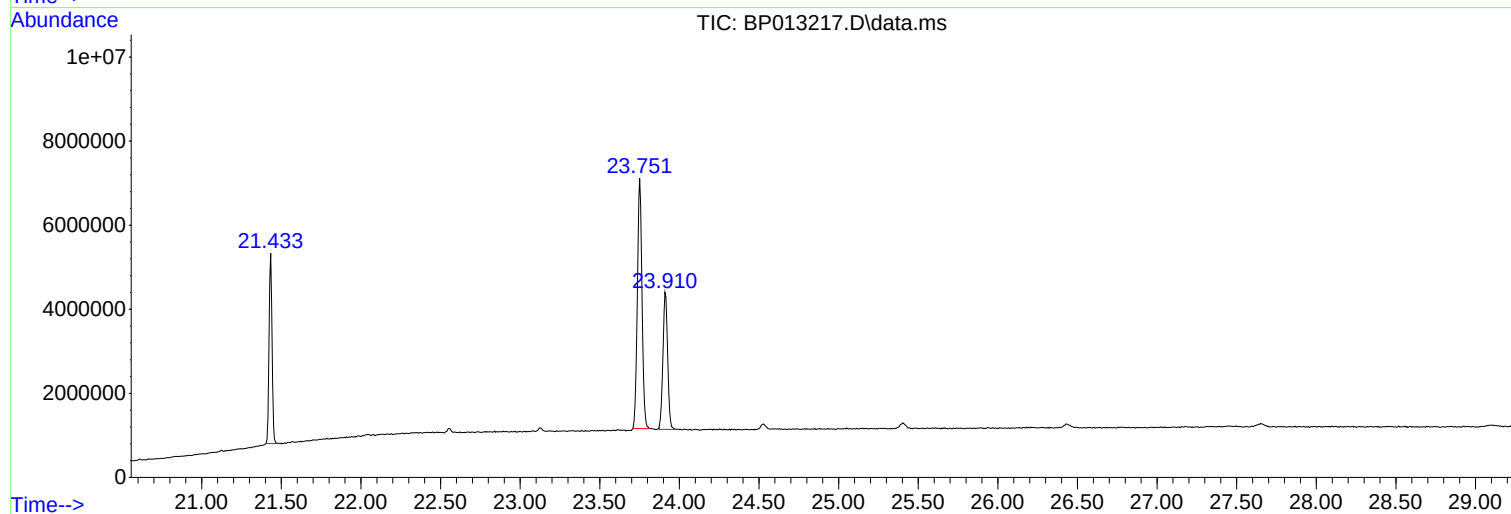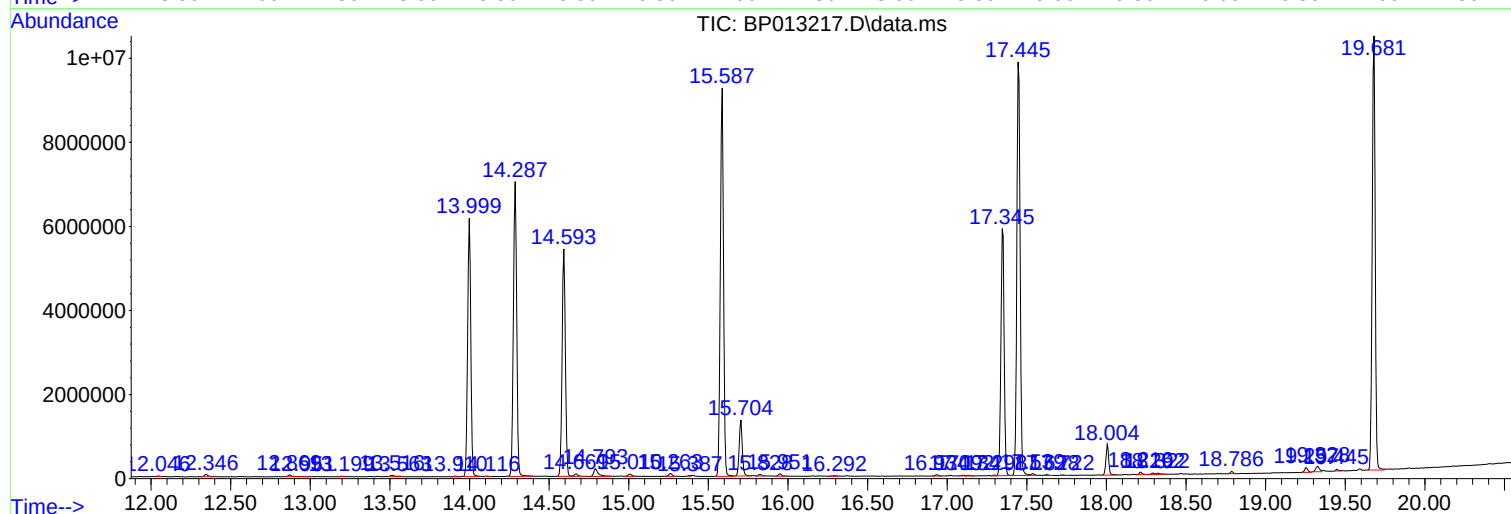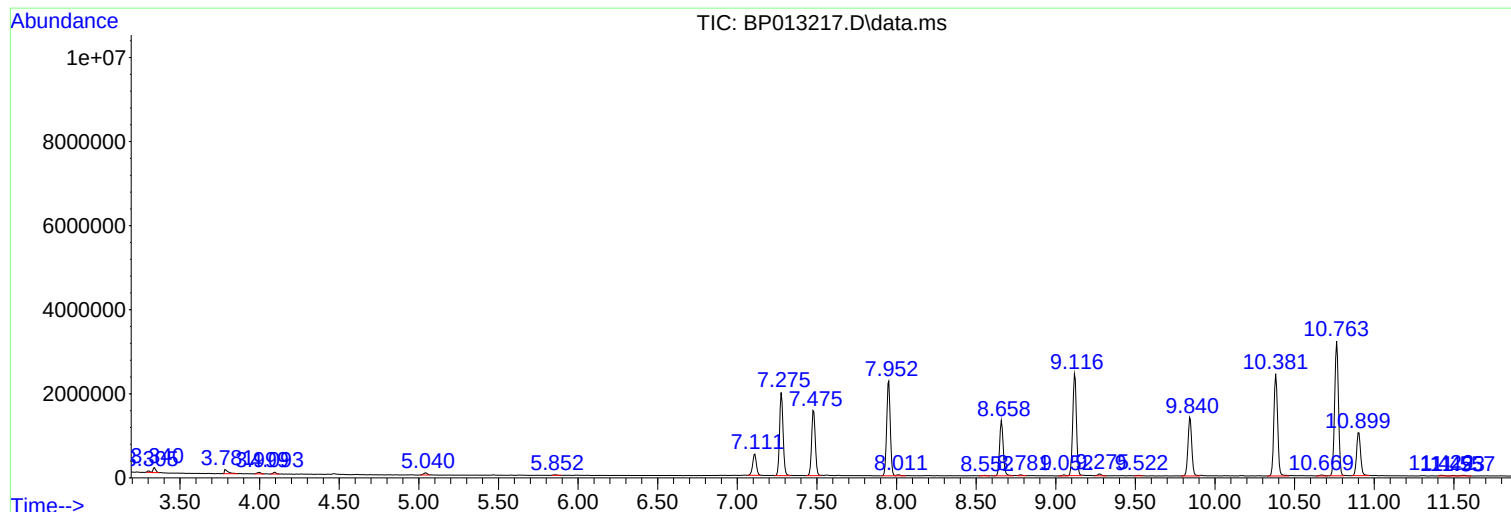

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013217.D
Acq On : 21 Dec 2022 20:20
Operator : CG/JU
Sample : N6032-04
Misc :
ALS Vial : 99 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COLA6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 7,9-Di-tert-butyl-1-oxaspiro... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
18.004	2.15 ng/ul	899522	Phenanthrene-d10	17.345

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	95		
2	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	70		
3	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	50		
4	1-(3-Amino-4,6-dimethylthieno[2,...	220	C11H12N2OS	052505-42-7	45		
5	2,5-di-tert-Butyl-1,4-benzoquinone	220	C14H20O2	002460-77-7	44		

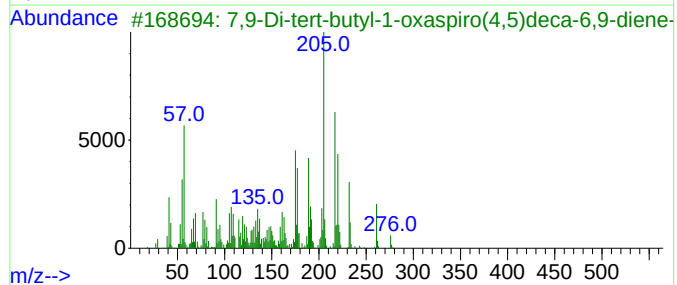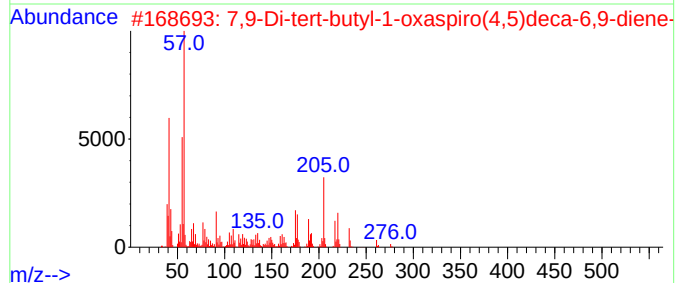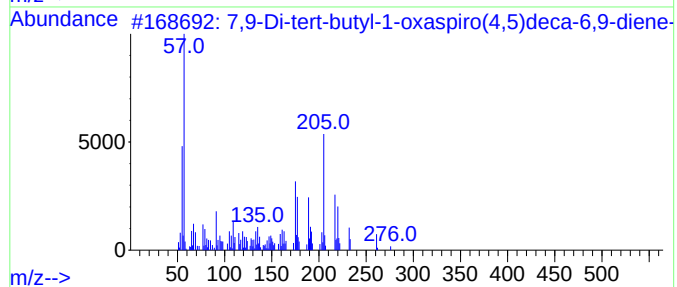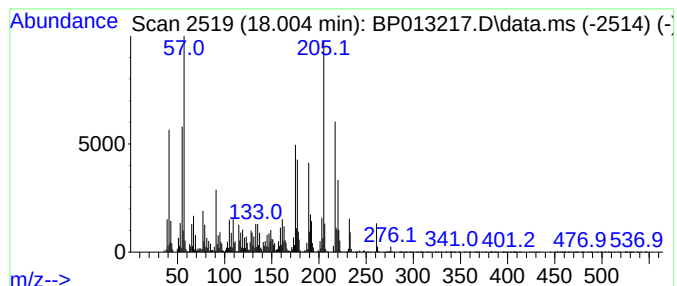

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013217.D
Acq On : 21 Dec 2022 20:20
Operator : CG/JU
Sample : N6032-04
Misc :
ALS Vial : 99 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0LA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
7,9-Di-tert-but...	18.004	2.1	ng/ul	899522	4	17.345	8348510	20.0