

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013218.D
 Acq On : 21 Dec 2022 20:54
 Operator : CG/JU
 Sample : N6032-05
 Misc :
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COL87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013218.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	15	20	23	rBV	601072	795779	6.46%	0.742%
2	3.334	23	25	30	rVB	127918	149737	1.22%	0.140%
3	3.775	98	100	120	rBV	238566	387767	3.15%	0.362%
4	3.993	133	137	142	rVB	39563	59761	0.49%	0.056%
5	4.093	151	154	160	rVB	36932	50989	0.41%	0.048%
6	4.628	242	245	251	rVB7	18466	27190	0.22%	0.025%
7	5.040	310	315	320	rBV2	49098	83482	0.68%	0.078%
8	7.111	660	667	675	rVB	395935	641679	5.21%	0.599%
9	7.275	688	695	707	rBV	1782827	2681670	21.78%	2.502%
10	7.475	723	729	740	rBV	1180134	1876952	15.25%	1.751%
11	7.564	740	744	749	rVB5	12330	18858	0.15%	0.018%
12	7.952	801	810	818	rBV	1905447	3047037	24.75%	2.843%
13	8.658	924	930	942	rBV	930162	1461028	11.87%	1.363%
14	9.116	1001	1008	1017	rBV	2186837	3549609	28.83%	3.311%
15	9.516	1071	1076	1083	rVB3	19945	32125	0.26%	0.030%
16	9.840	1124	1131	1142	rBV	1420464	2324632	18.88%	2.169%
17	10.381	1216	1223	1233	rBV	1831399	2961725	24.06%	2.763%
18	10.763	1278	1288	1295	rBV	2621138	4314267	35.04%	4.025%
19	10.899	1304	1311	1320	rBV	916737	1623151	13.18%	1.514%
20	12.016	1496	1501	1507	rBV10	7610	16946	0.14%	0.016%
21	12.346	1551	1557	1563	rBV	46951	78787	0.64%	0.073%
22	13.199	1696	1702	1711	rVB	7214	16959	0.14%	0.016%
23	13.404	1730	1737	1746	rVB6	19423	34117	0.28%	0.032%
24	13.546	1754	1761	1769	rVB6	16190	34049	0.28%	0.032%
25	13.922	1819	1825	1829	rBV9	6547	12671	0.10%	0.012%
26	13.998	1829	1838	1853	rBV	4325578	5935345	48.21%	5.537%
27	14.287	1880	1887	1904	rBV	5346315	7816711	63.49%	7.292%
28	14.481	1915	1920	1923	rVB6	9370	16451	0.13%	0.015%
29	14.540	1926	1930	1932	rBV2	11426	15995	0.13%	0.015%
30	14.593	1932	1939	1949	rVB	3631492	5169806	41.99%	4.823%
31	14.793	1967	1973	1986	rBV	126272	279327	2.27%	0.261%
32	15.004	2003	2009	2016	rVB	20001	43332	0.35%	0.040%
33	15.587	2101	2108	2121	rBV	6446138	9449265	76.75%	8.815%
34	15.704	2122	2128	2137	rVV	1198837	1577826	12.82%	1.472%
35	15.822	2144	2148	2153	rVB4	30677	49977	0.41%	0.047%
36	15.951	2166	2170	2173	rBV3	16409	19384	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013218.D
 Acq On : 21 Dec 2022 20:54
 Operator : CG/JU
 Sample : N6032-05
 Misc :
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COL87

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

37	17.028	2348	2353	2356	rVB7	10468	15473	0.13%	0.014%
38	17.345	2401	2407	2417	rBV	3776122	5266947	42.78%	4.913%
39	17.445	2418	2424	2436	rBV	6638799	9280418	75.38%	8.658%
40	18.004	2516	2519	2523	rBV6	18952	23488	0.19%	0.022%
41	18.216	2550	2555	2560	rBV2	109498	154511	1.25%	0.144%
42	19.257	2728	2732	2736	rVB	80345	94845	0.77%	0.088%
43	19.322	2739	2743	2748	rBV	77058	118094	0.96%	0.110%
44	19.445	2761	2764	2767	rBV4	57016	69733	0.57%	0.065%
45	19.681	2798	2804	2814	rBV	8238305	10835005	88.00%	10.108%
46	21.433	3097	3102	3113	rBV	4533931	5821847	47.29%	5.431%
47	23.751	3489	3496	3507	rVB	6194390	12311899	100.00%	11.486%
48	23.910	3517	3523	3534	rVB2	3203477	6548388	53.19%	6.109%




Sum of corrected areas: 107195034

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013218.D
Acq On : 21 Dec 2022 20:54
Operator : CG/JU
Sample : N6032-05
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COL87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

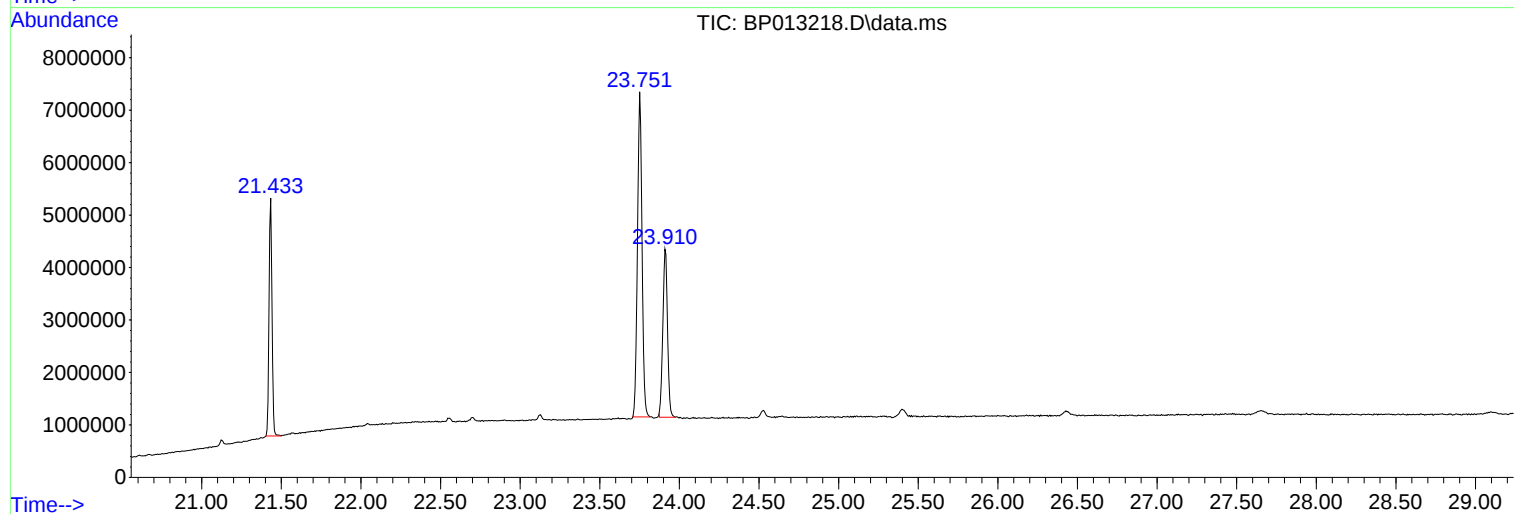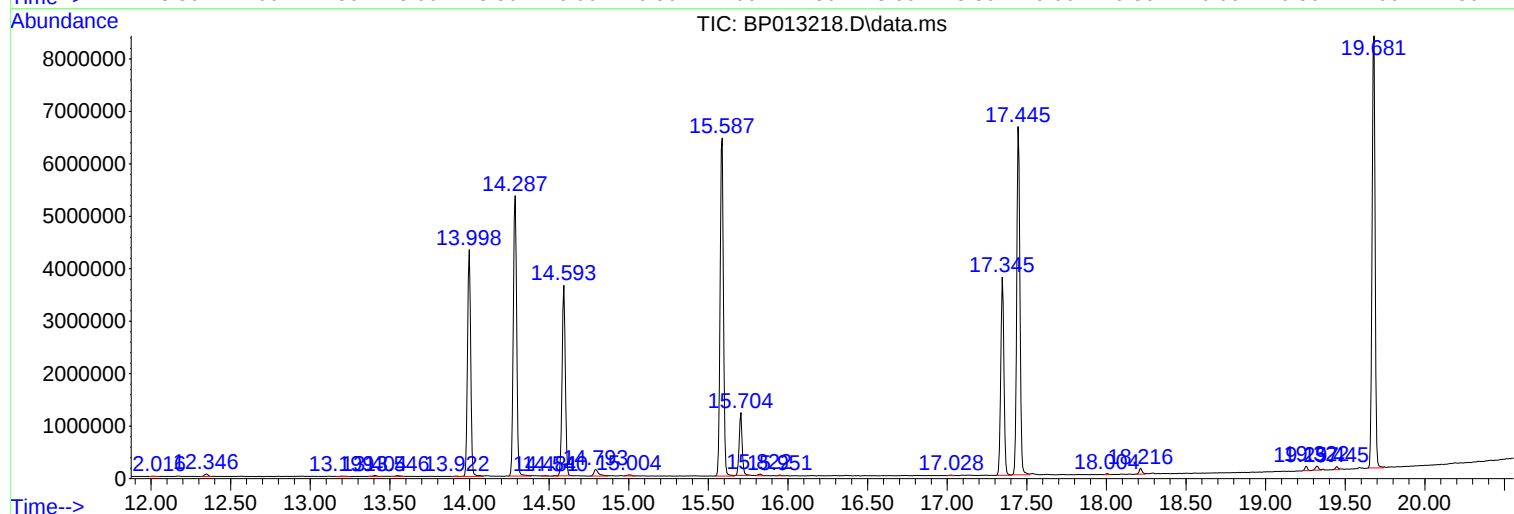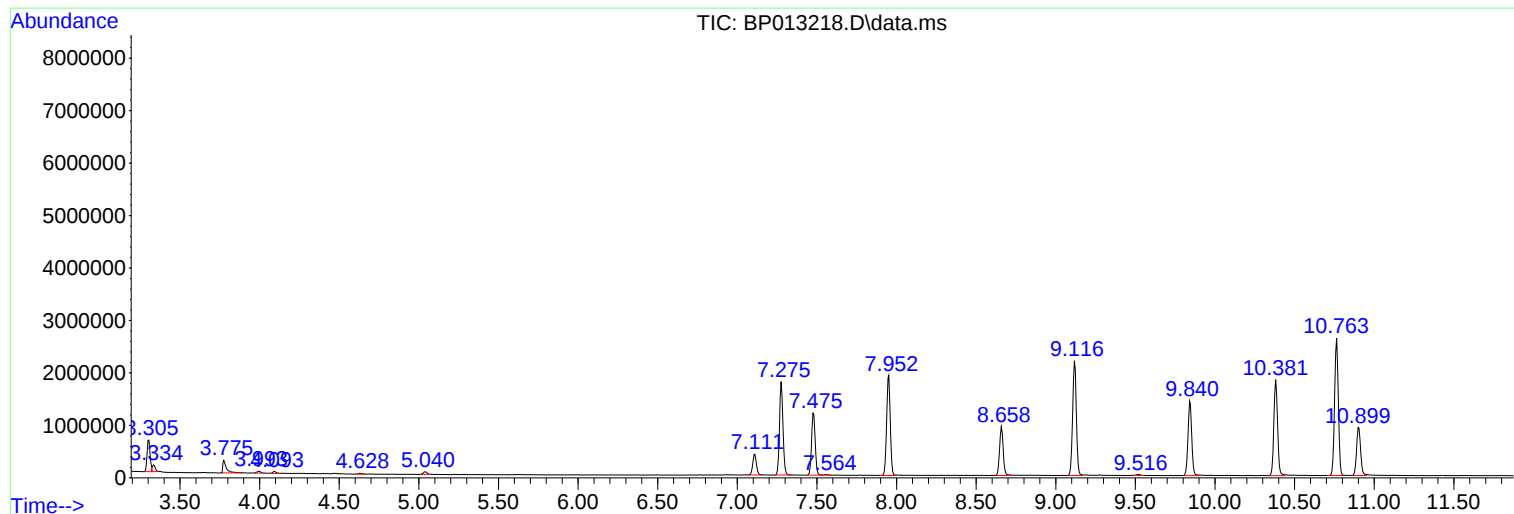

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013218.D
Acq On : 21 Dec 2022 20:54
Operator : CG/JU
Sample : N6032-05
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0L87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013218.D
Acq On : 21 Dec 2022 20:54
Operator : CG/JU
Sample : N6032-05
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0L87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc