

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013219.D
 Acq On : 21 Dec 2022 21:28
 Operator : CG/JU
 Sample : N6032-06
 Misc :
 ALS Vial : 101 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0L89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013219.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	15	19	23	rBV	457916	637253	5.75%	0.546%
2	3.334	23	25	30	rVB	129290	153114	1.38%	0.131%
3	3.623	71	74	83	rBV	75264	112378	1.01%	0.096%
4	3.781	98	101	114	rBV	140576	244152	2.20%	0.209%
5	3.993	134	137	145	rVB2	35074	56700	0.51%	0.049%
6	4.093	150	154	164	rVB	40838	59805	0.54%	0.051%
7	4.628	242	245	249	rVB5	11008	15905	0.14%	0.014%
8	5.040	307	315	324	rVB2	76636	123378	1.11%	0.106%
9	7.111	660	667	674	rBV	496083	786676	7.09%	0.674%
10	7.275	688	695	710	rBV	1799765	2743408	24.74%	2.352%
11	7.475	720	729	738	rBV	1461825	2306601	20.80%	1.977%
12	7.558	741	743	750	rVB5	11797	15525	0.14%	0.013%
13	7.952	802	810	818	rBV	2015842	3235049	29.18%	2.773%
14	8.287	862	867	871	rBV8	8313	15181	0.14%	0.013%
15	8.658	924	930	943	rBV	1217290	1979478	17.85%	1.697%
16	8.981	979	985	995	rBV	13555	41880	0.38%	0.036%
17	9.116	1000	1008	1022	rVV	2195414	3600934	32.48%	3.087%
18	9.516	1072	1076	1080	rBV7	9653	16041	0.14%	0.014%
19	9.840	1122	1131	1140	rBV	1614335	2639694	23.81%	2.263%
20	10.381	1215	1223	1241	rBV	2331872	3800846	34.28%	3.258%
21	10.763	1280	1288	1296	rBV	2909400	4821787	43.49%	4.134%
22	10.899	1304	1311	1327	rBV	989213	1738747	15.68%	1.491%
23	11.546	1417	1421	1427	rVB9	6157	11241	0.10%	0.010%
24	11.940	1483	1488	1494	rBV9	6520	12742	0.11%	0.011%
25	12.346	1550	1557	1565	rBV	48517	78209	0.71%	0.067%
26	13.404	1734	1737	1742	rVB5	11822	14735	0.13%	0.013%
27	13.557	1759	1763	1767	rVB7	8696	14206	0.13%	0.012%
28	13.999	1831	1838	1851	rBV	5375950	7183542	64.79%	6.158%
29	14.110	1853	1857	1863	rVB9	9582	19519	0.18%	0.017%
30	14.287	1879	1887	1899	rBV	6036750	8730478	78.74%	7.485%
31	14.481	1915	1920	1924	rVB7	10079	16706	0.15%	0.014%
32	14.593	1927	1939	1946	rBV	4431527	6528411	58.88%	5.597%
33	14.793	1966	1973	1984	rBV	223835	434128	3.92%	0.372%
34	15.004	2005	2009	2017	rVB7	34197	68121	0.61%	0.058%
35	15.222	2042	2046	2050	rBV7	6495	12593	0.11%	0.011%
36	15.587	2100	2108	2120	rBV	7840865	11088253	100.00%	9.506%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013219.D
 Acq On : 21 Dec 2022 21:28
 Operator : CG/JU
 Sample : N6032-06
 Misc :
 ALS Vial : 101 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COL89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

37	15.704	2122	2128	2142	rVV	1700157	2366082	21.34%	2.028%
38	15.822	2144	2148	2155	rVB2	33118	56107	0.51%	0.048%
39	15.945	2164	2169	2173	rBV7	10683	19053	0.17%	0.016%
40	16.151	2202	2204	2210	rBV7	7502	12759	0.12%	0.011%
41	16.293	2223	2228	2231	rBV7	14309	23034	0.21%	0.020%
42	17.022	2349	2352	2356	rVB5	12706	16106	0.15%	0.014%
43	17.092	2361	2364	2368	rVV5	16331	23525	0.21%	0.020%
44	17.140	2368	2372	2377	rVB5	17334	32218	0.29%	0.028%
45	17.345	2400	2407	2417	rBV	4795868	6717143	60.58%	5.759%
46	17.445	2418	2424	2441	rVV	7778068	10845704	97.81%	9.298%
47	17.828	2487	2489	2493	rVB4	14081	13587	0.12%	0.012%
48	18.004	2516	2519	2523	rVB5	17636	18516	0.17%	0.016%
49	18.216	2551	2555	2560	rBV5	46356	66643	0.60%	0.057%
50	19.251	2727	2731	2737	rBV2	90984	153756	1.39%	0.132%
51	19.322	2740	2743	2747	rVB	75724	102346	0.92%	0.088%
52	19.681	2798	2804	2815	rBV	7614820	10410257	93.89%	8.925%
53	21.433	3097	3102	3110	rVB	3985880	5335158	48.12%	4.574%
54	23.751	3489	3496	3509	rVB	5384983	10857268	97.92%	9.308%
55	23.910	3517	3523	3534	rVB2	3101267	6219284	56.09%	5.332%


Sum of corrected areas: 116645962

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013219.D
Acq On : 21 Dec 2022 21:28
Operator : CG/JU
Sample : N6032-06
Misc :
ALS Vial : 101 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COL89

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

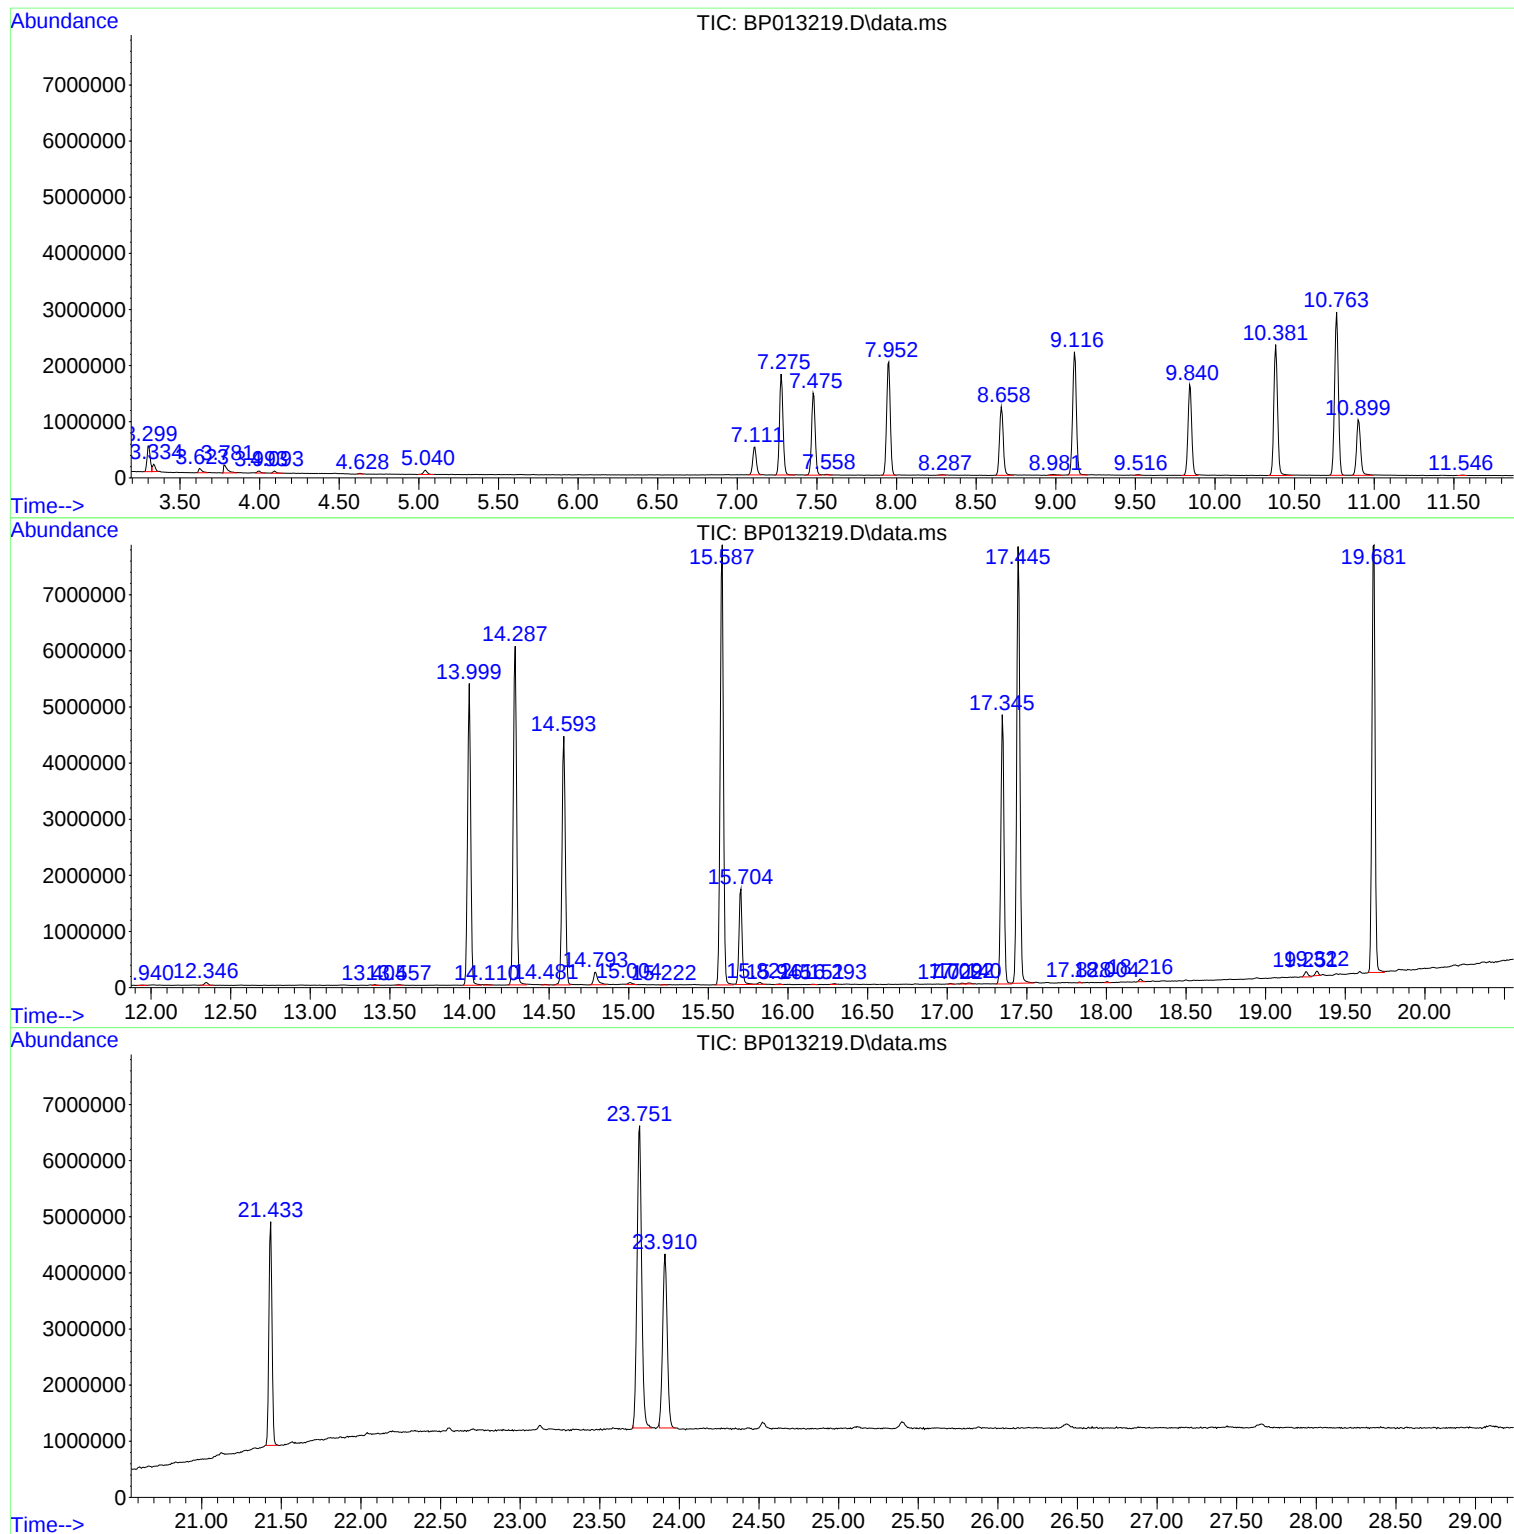

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013219.D
Acq On : 21 Dec 2022 21:28
Operator : CG/JU
Sample : N6032-06
Misc :
ALS Vial : 101 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0L89

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013219.D
Acq On : 21 Dec 2022 21:28
Operator : CG/JU
Sample : N6032-06
Misc :
ALS Vial : 101 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0L89

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc