

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013222.D
 Acq On : 21 Dec 2022 23:45
 Operator : CG/JU
 Sample : PB149681BL
 Misc :
 ALS Vial : 105 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK681

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013222.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	21	25	32	rVB	154206	197202	1.98%	0.185%
2	3.763	95	98	118	rBV	1894436	2783241	28.01%	2.608%
3	4.093	150	154	160	rVB	42352	58326	0.59%	0.055%
4	7.104	657	666	684	rBV	2008653	3198267	32.19%	2.997%
5	7.275	687	695	707	rVB	1706640	2604782	26.22%	2.441%
6	7.475	722	729	741	rBV	2081666	3270623	32.92%	3.065%
7	7.951	803	810	819	rVB	1780214	2864127	28.83%	2.684%
8	8.657	922	930	942	rBV	2472064	3898768	39.24%	3.654%
9	9.116	1001	1008	1021	rBV	1934878	3095058	31.15%	2.901%
10	9.840	1124	1131	1141	rBV	1554385	2560123	25.77%	2.399%
11	10.381	1214	1223	1239	rBV	2424727	4004375	40.31%	3.753%
12	10.763	1280	1288	1297	rBV	2472533	4080816	41.07%	3.825%
13	10.898	1304	1311	1324	rBV	2269167	3991894	40.18%	3.741%
14	12.345	1552	1557	1564	rVB	42958	65297	0.66%	0.061%
15	13.375	1728	1732	1737	rBV8	5748	11481	0.12%	0.011%
16	13.557	1759	1763	1768	rVB7	6829	11222	0.11%	0.011%
17	13.998	1831	1838	1852	rBV	3769287	5168699	52.02%	4.844%
18	14.286	1879	1887	1899	rBV	4255725	6391933	64.34%	5.991%
19	14.592	1930	1939	1948	rBV	3266885	4961605	49.94%	4.650%
20	14.786	1965	1972	1993	rBV	1134299	1944066	19.57%	1.822%
21	14.992	2005	2007	2014	rVB8	10458	19918	0.20%	0.019%
22	15.586	2101	2108	2122	rBV	5182538	7535887	75.85%	7.063%
23	15.704	2122	2128	2139	rBV	1162964	1657194	16.68%	1.553%
24	15.822	2144	2148	2156	rVB5	29056	50791	0.51%	0.048%
25	16.157	2202	2205	2210	rVB7	7209	10005	0.10%	0.009%
26	16.369	2237	2241	2245	rBV7	8363	11621	0.12%	0.011%
27	17.022	2349	2352	2356	rBV6	7121	10408	0.10%	0.010%
28	17.098	2361	2365	2367	rBV5	7493	12011	0.12%	0.011%
29	17.345	2400	2407	2417	rBV	3601018	4905006	49.37%	4.597%
30	17.445	2418	2424	2441	rVV	5211458	7316210	73.64%	6.857%
31	19.257	2728	2732	2738	rVB2	56081	72682	0.73%	0.068%
32	19.321	2739	2743	2747	rBV	57945	83152	0.84%	0.078%
33	19.674	2798	2803	2812	rBV	6466128	8479977	85.35%	7.947%
34	21.433	3097	3102	3110	rVB	4043844	5311760	53.46%	4.978%
35	23.751	3489	3496	3507	rVB2	4925305	9935099	100.00%	9.311%
36	23.909	3517	3523	3537	rVB2	2933072	6126686	61.67%	5.742%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013222.D
Acq On : 21 Dec 2022 23:45
Operator : CG/JU
Sample : PB149681BL
Misc :
ALS Vial : 105 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK681

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION




Sum of corrected areas: 106700312

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013222.D
Acq On : 21 Dec 2022 23:45
Operator : CG/JU
Sample : PB149681BL
Misc :
ALS Vial : 105 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK681

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

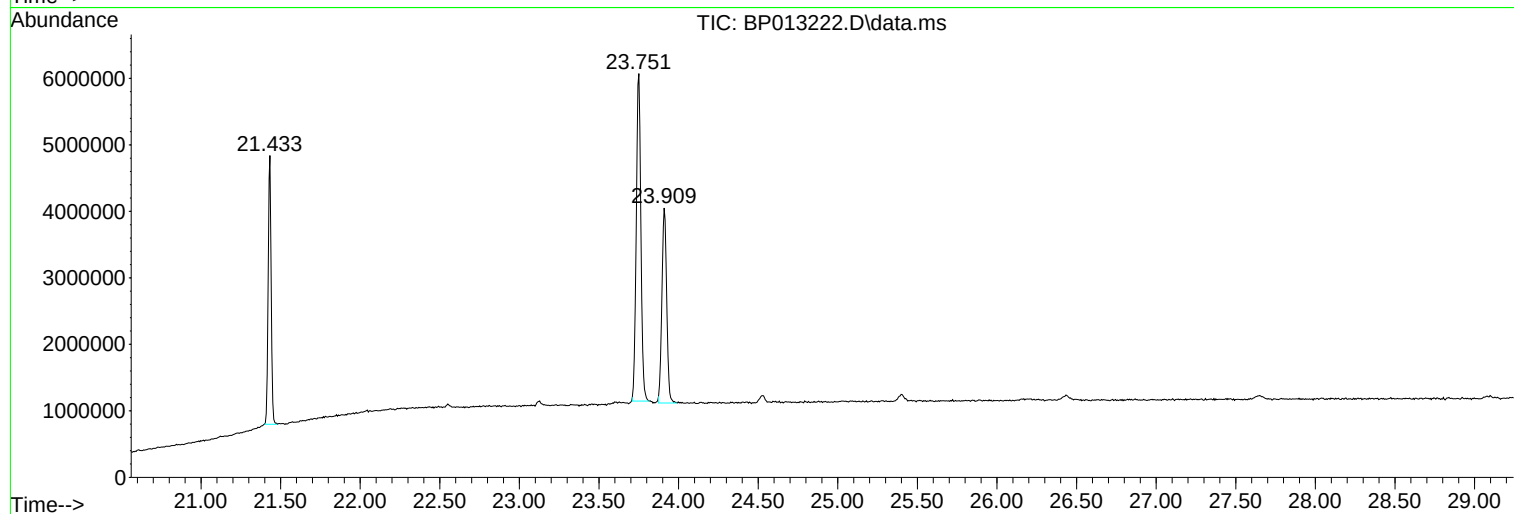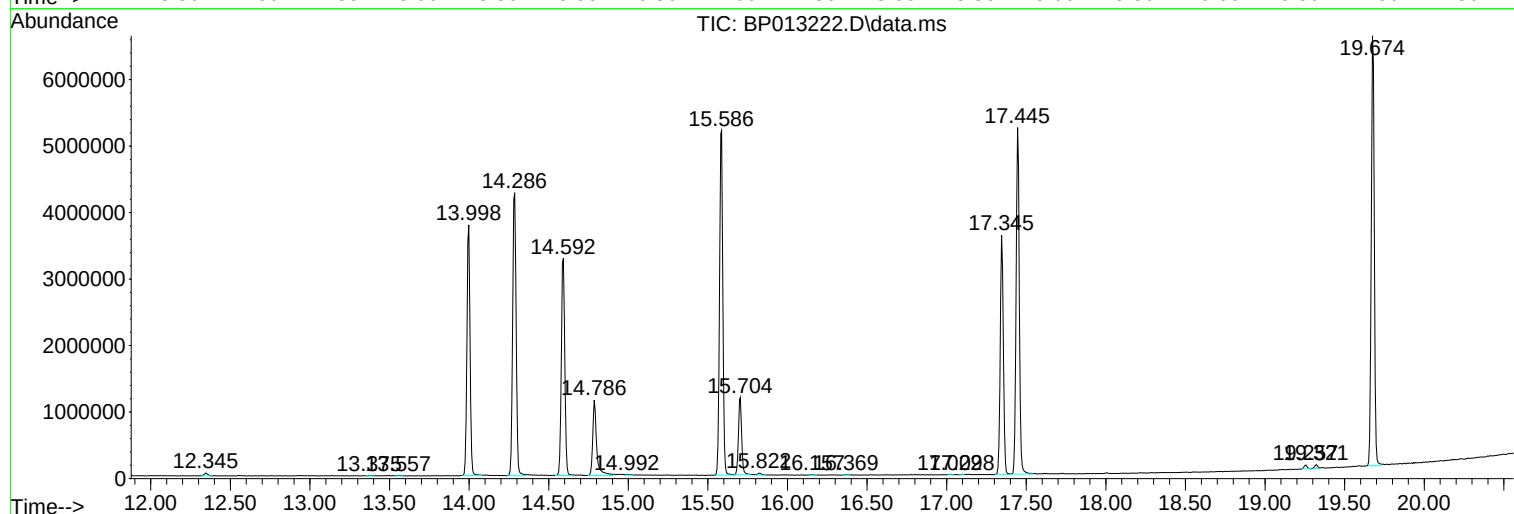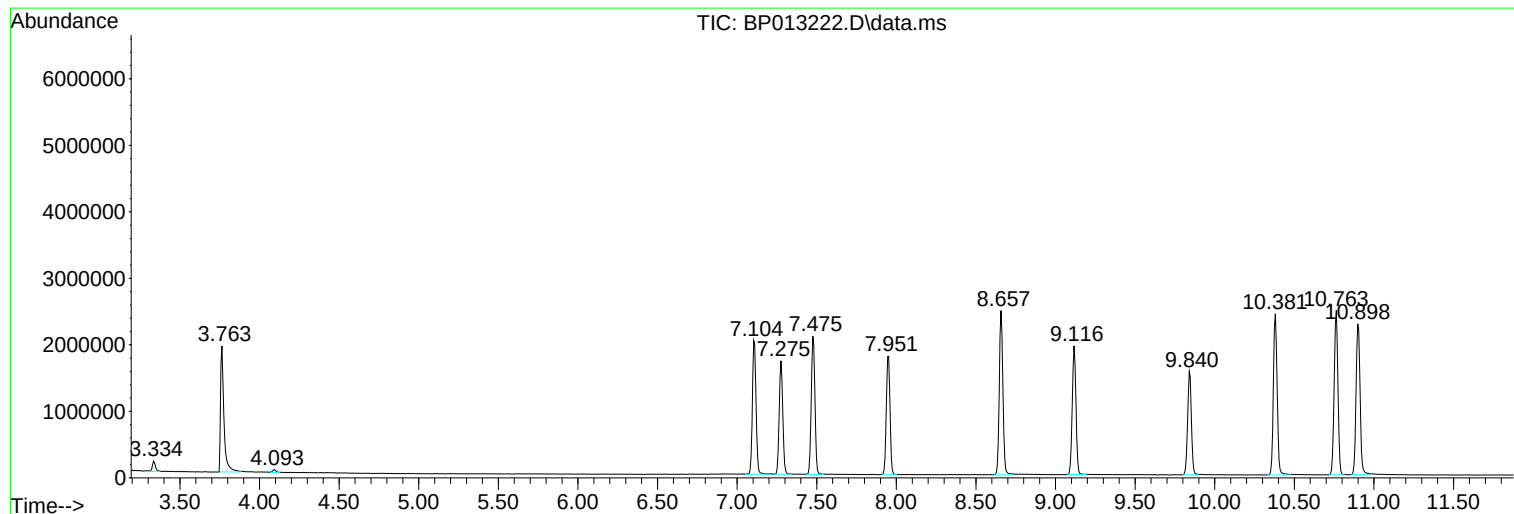

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013222.D
Acq On : 21 Dec 2022 23:45
Operator : CG/JU
Sample : PB149681BL
Misc :
ALS Vial : 105 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK681

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013222.D
Acq On : 21 Dec 2022 23:45
Operator : CG/JU
Sample : PB149681BL
Misc :
ALS Vial : 105 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK681

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc