

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013223.D
 Acq On : 22 Dec 2022 00:19
 Operator : CG/JU
 Sample : PB149797BL
 Misc :
 ALS Vial : 106 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK797

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013223.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	21	25	32	rVB	163130	204140	1.99%	0.168%
2	3.764	95	98	117	rBV	2051820	3074088	30.04%	2.529%
3	4.093	150	154	160	rVB	48864	65132	0.64%	0.054%
4	7.105	659	666	678	rBV	2274840	3605107	35.22%	2.966%
5	7.275	688	695	706	rVB	1933380	2952478	28.85%	2.429%
6	7.475	720	729	740	rBV	2381974	3703275	36.18%	3.047%
7	7.946	802	809	816	rBV	2026123	3259072	31.84%	2.682%
8	8.657	921	930	943	rBV	2873088	4493682	43.91%	3.697%
9	9.116	1000	1008	1020	rBV	2250110	3601465	35.19%	2.963%
10	9.840	1123	1131	1145	rBV	1891664	3013187	29.44%	2.479%
11	10.381	1215	1223	1238	rBV	2856126	4657731	45.51%	3.832%
12	10.763	1277	1288	1296	rBV	2900314	4763389	46.54%	3.919%
13	10.898	1302	1311	1324	rBV	2773402	4689037	45.81%	3.858%
14	12.345	1552	1557	1564	rBV	46369	78938	0.77%	0.065%
15	12.551	1585	1592	1596	rBV10	4766	10762	0.11%	0.009%
16	13.563	1760	1764	1770	rVB9	8896	14709	0.14%	0.012%
17	13.998	1827	1838	1850	rBV	4564177	6349417	62.04%	5.224%
18	14.110	1854	1857	1862	rVB7	7471	11646	0.11%	0.010%
19	14.287	1879	1887	1905	rBV	5213380	7768865	75.91%	6.392%
20	14.592	1931	1939	1949	rBV	3922358	6023440	58.85%	4.956%
21	14.787	1965	1972	1990	rBV	1373482	2233799	21.83%	1.838%
22	15.004	2004	2009	2016	rVB	11401	22953	0.22%	0.019%
23	15.586	2100	2108	2121	rBV	6362721	9275220	90.62%	7.632%
24	15.704	2121	2128	2143	rVV	1415112	1955006	19.10%	1.609%
25	15.822	2143	2148	2154	rVB3	30253	53792	0.53%	0.044%
26	16.151	2201	2204	2210	rBV8	5544	11185	0.11%	0.009%
27	16.369	2236	2241	2245	rBV8	8790	14500	0.14%	0.012%
28	17.104	2361	2366	2367	rBV5	8127	11883	0.12%	0.010%
29	17.345	2400	2407	2417	rBV	4179459	5815515	56.82%	4.785%
30	17.445	2417	2424	2442	rVV	6309811	8502428	83.07%	6.996%
31	19.251	2728	2731	2736	rBV2	59685	81263	0.79%	0.067%
32	19.322	2740	2743	2751	rVB	56299	80896	0.79%	0.067%
33	19.674	2798	2803	2814	rBV	6635375	8790060	85.88%	7.233%
34	21.433	3097	3102	3110	rBV	4370192	5588958	54.61%	4.599%
35	23.751	3489	3496	3508	rVB2	4918350	10234914	100.00%	8.421%
36	23.910	3517	3523	3537	rVB2	3121859	6521855	63.72%	5.366%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013223.D
Acq On : 22 Dec 2022 00:19
Operator : CG/JU
Sample : PB149797BL
Misc :
ALS Vial : 106 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK797

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION


Sum of corrected areas: 121533787

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013223.D
Acq On : 22 Dec 2022 00:19
Operator : CG/JU
Sample : PB149797BL
Misc :
ALS Vial : 106 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK797

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

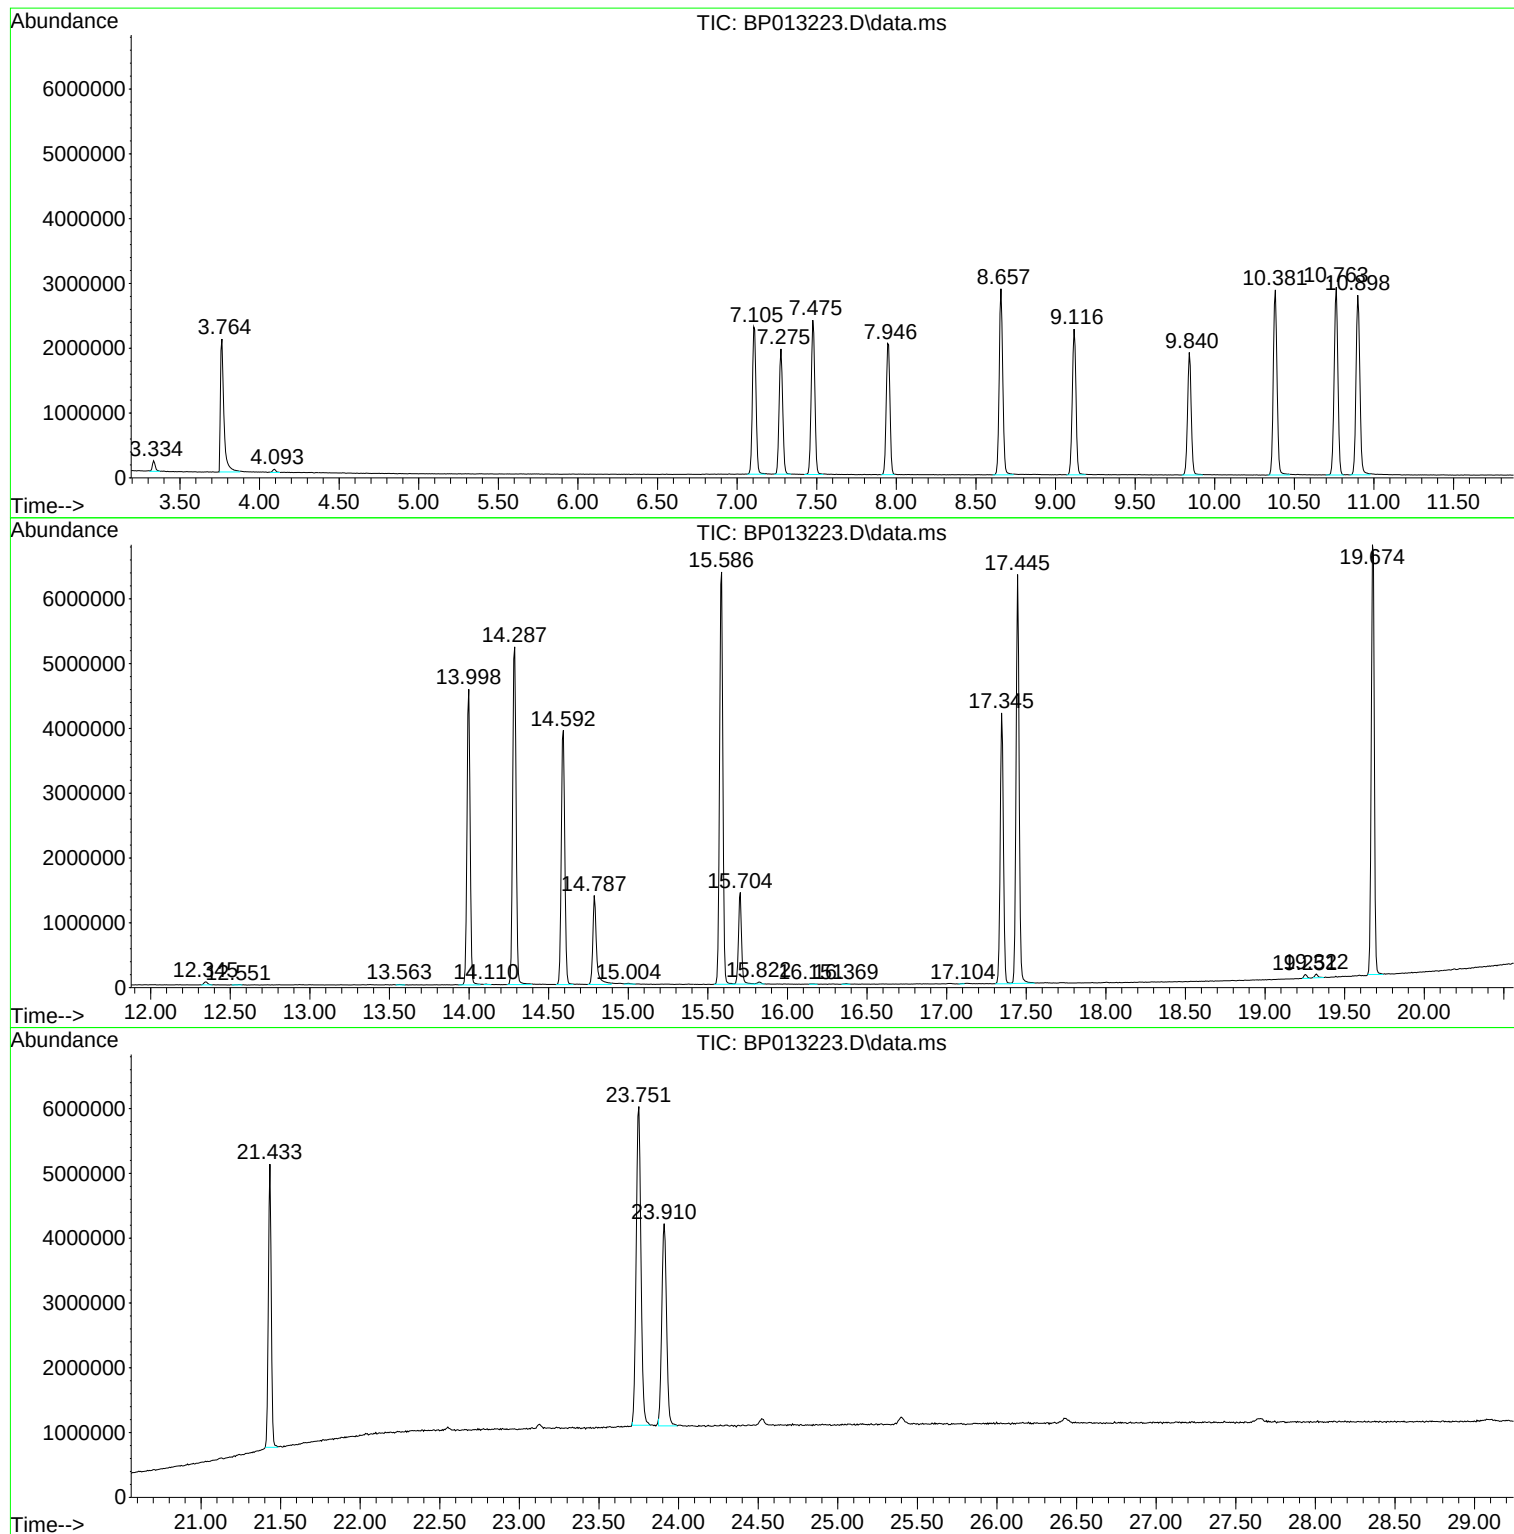

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013223.D
Acq On : 22 Dec 2022 00:19
Operator : CG/JU
Sample : PB149797BL
Misc :
ALS Vial : 106 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK797

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013223.D
Acq On : 22 Dec 2022 00:19
Operator : CG/JU
Sample : PB149797BL
Misc :
ALS Vial : 106 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK797

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc