

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013227.D
 Acq On : 22 Dec 2022 02:35
 Operator : CG/JU
 Sample : N6032-15
 Misc :
 ALS Vial : 110 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COLC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013227.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	16	19	22	rBV	98673	121702	0.83%	0.107%
2	3.334	22	25	31	rVB	113312	146316	0.99%	0.129%
3	3.775	97	100	111	rBV	195757	312460	2.12%	0.276%
4	3.999	133	138	142	rBV	33063	42922	0.29%	0.038%
5	4.093	150	154	160	rVB	40442	56093	0.38%	0.049%
6	5.040	309	315	323	rVB2	66571	102755	0.70%	0.091%
7	7.104	660	666	677	rBV	545654	862073	5.85%	0.761%
8	7.275	688	695	703	rBV	1638253	2494460	16.94%	2.201%
9	7.475	722	729	740	rBV	1322553	2051849	13.93%	1.810%
10	7.945	800	809	817	rBV	1966968	3150129	21.39%	2.779%
11	8.010	817	820	827	rVB5	14703	23546	0.16%	0.021%
12	8.657	923	930	941	rBV	1053563	1657594	11.26%	1.462%
13	9.116	1000	1008	1020	rBV	1983609	3158732	21.45%	2.787%
14	9.516	1069	1076	1084	rVB	8197	21786	0.15%	0.019%
15	9.839	1123	1131	1145	rBV	1305092	2140950	14.54%	1.889%
16	10.381	1214	1223	1236	rBV	1749192	2977858	20.22%	2.627%
17	10.763	1279	1288	1298	rBV	2566481	4311072	29.27%	3.804%
18	10.904	1305	1312	1322	rBV	376756	677236	4.60%	0.598%
19	12.163	1520	1526	1532	rVB	42448	74089	0.50%	0.065%
20	12.345	1550	1557	1562	rBV2	39497	70284	0.48%	0.062%
21	12.551	1587	1592	1601	rBV2	7493	18144	0.12%	0.016%
22	12.780	1627	1631	1638	rVB8	11157	18571	0.13%	0.016%
23	13.210	1699	1704	1710	rVB4	13269	23424	0.16%	0.021%
24	13.545	1755	1761	1768	rBV9	9532	22401	0.15%	0.020%
25	13.998	1831	1838	1854	rBV	3910684	5524410	37.51%	4.874%
26	14.286	1879	1887	1902	rBV	4526988	6782355	46.05%	5.984%
27	14.592	1932	1939	1951	rBV	3527766	5230323	35.52%	4.615%
28	14.786	1967	1972	1982	rBV	235114	461963	3.14%	0.408%
29	14.869	1983	1986	1994	rVB4	31845	61050	0.41%	0.054%
30	14.998	2004	2008	2013	rVB7	17000	30212	0.21%	0.027%
31	15.580	2100	2107	2122	rBV	6181281	8838942	60.02%	7.799%
32	15.698	2122	2127	2141	rVV	1366897	1936605	13.15%	1.709%
33	15.822	2145	2148	2154	rVB3	28809	48087	0.33%	0.042%
34	15.945	2167	2169	2175	rVB3	13968	15013	0.10%	0.013%
35	17.098	2360	2365	2367	rBV6	10775	15840	0.11%	0.014%
36	17.127	2368	2370	2378	rVB6	11654	21638	0.15%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013227.D
 Acq On : 22 Dec 2022 02:35
 Operator : CG/JU
 Sample : N6032-15
 Misc :
 ALS Vial : 110 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0LC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

37	17.345	2400	2407	2417	rBV	4397002	6115453	41.53%	5.396%
38	17.445	2418	2424	2438	rVV	7011908	9787626	66.46%	8.636%
39	18.004	2515	2519	2523	rBV7	17948	27695	0.19%	0.024%
40	18.210	2550	2554	2562	rBV4	64470	107952	0.73%	0.095%
41	19.251	2728	2731	2736	rVB2	90530	118458	0.80%	0.105%
42	19.321	2739	2743	2747	rBV	84447	111331	0.76%	0.098%
43	19.445	2761	2764	2768	rVB4	42572	44957	0.31%	0.040%
44	19.674	2797	2803	2816	rBV	9697168	12746599	86.55%	11.246%
45	21.433	3096	3102	3109	rBV	5659416	7598469	51.60%	6.704%
46	23.751	3488	3496	3507	rBV2	7217698	14726820	100.00%	12.993%
47	23.909	3516	3523	3533	rVB2	4071898	8452467	57.40%	7.458%




Sum of corrected areas: 113340711

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013227.D
Acq On : 22 Dec 2022 02:35
Operator : CG/JU
Sample : N6032-15
Misc :
ALS Vial : 110 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COLC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

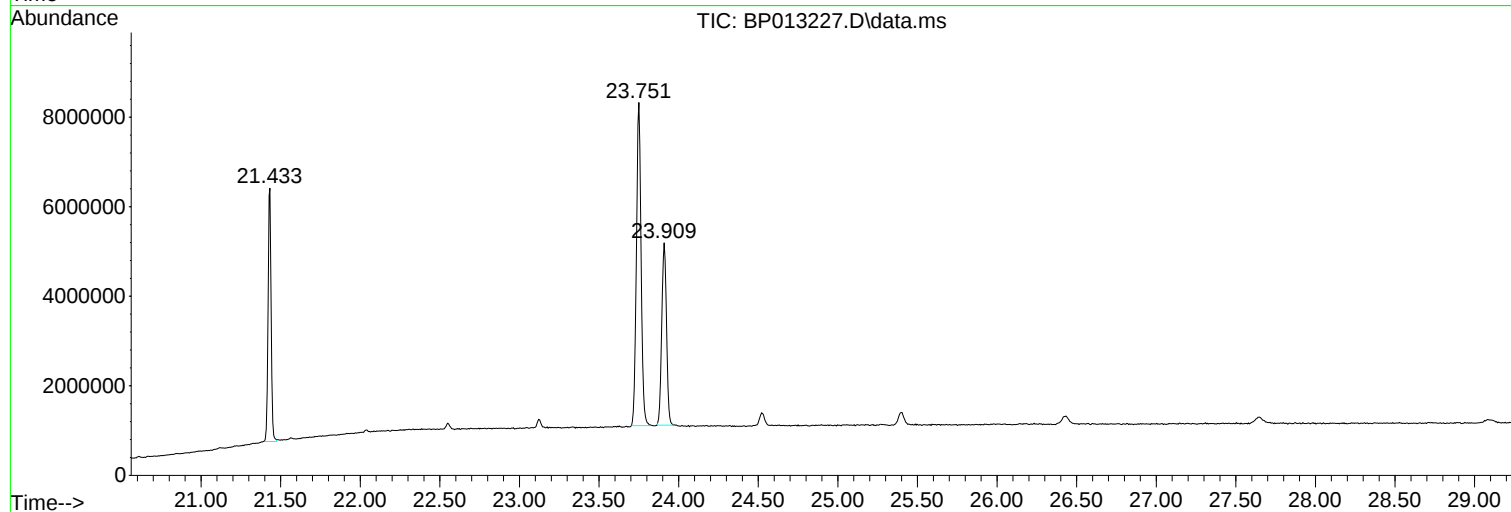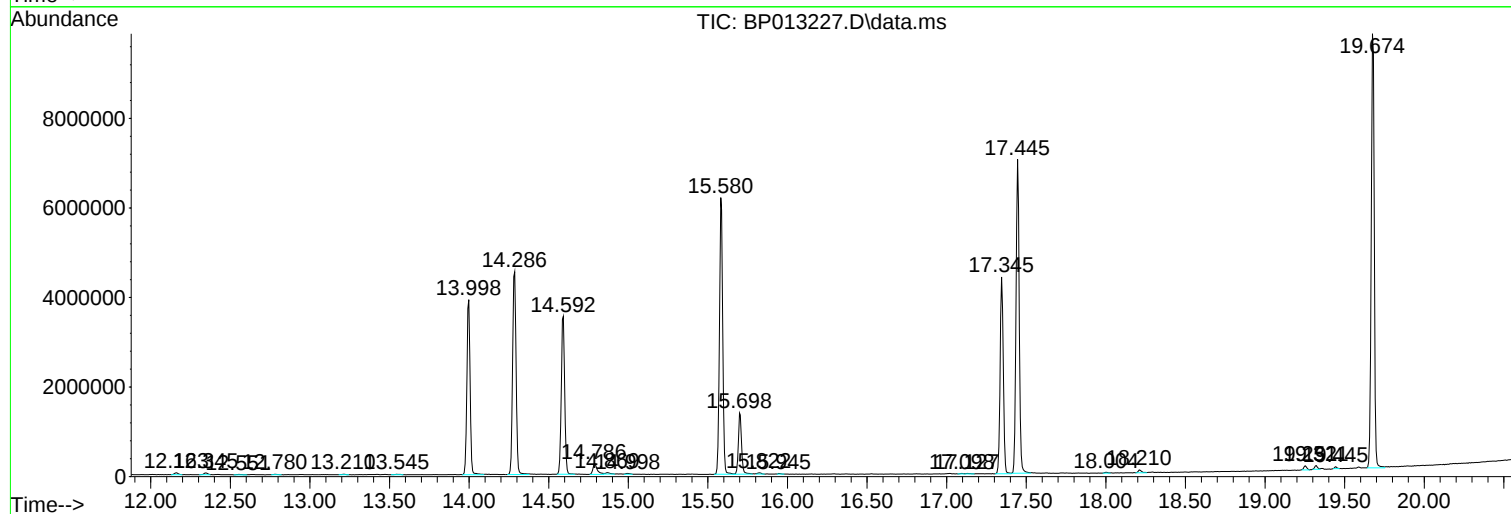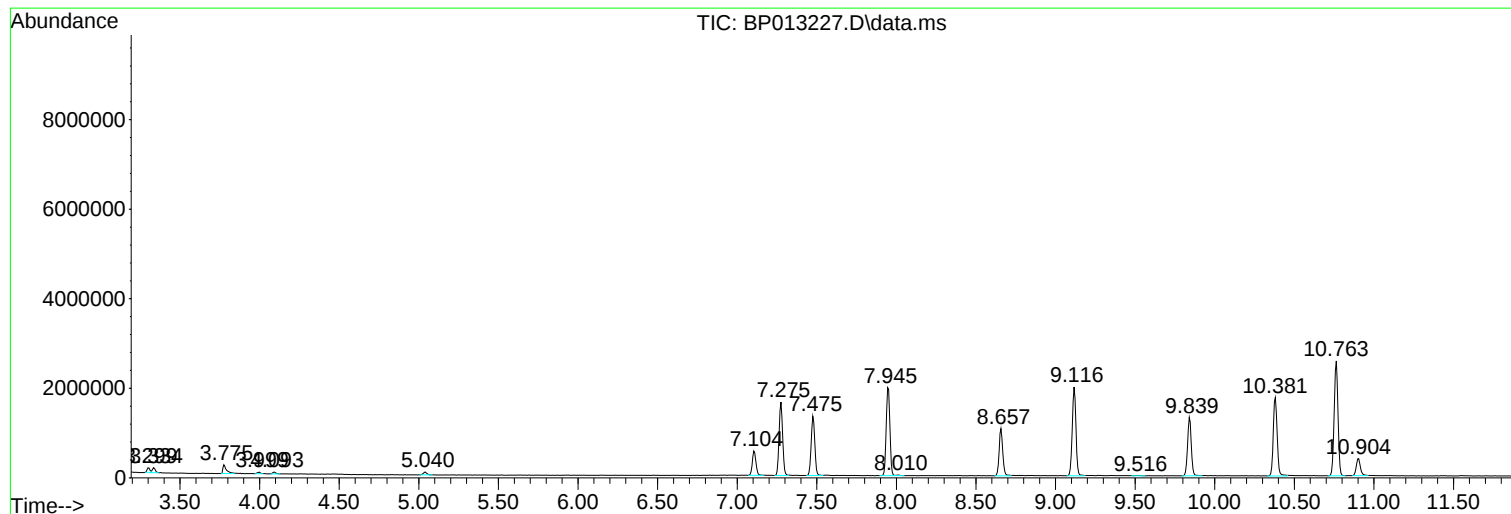

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013227.D
Acq On : 22 Dec 2022 02:35
Operator : CG/JU
Sample : N6032-15
Misc :
ALS Vial : 110 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0LC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013227.D
Acq On : 22 Dec 2022 02:35
Operator : CG/JU
Sample : N6032-15
Misc :
ALS Vial : 110 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0LC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
