

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013232.D
 Acq On : 22 Dec 2022 05:25
 Operator : CG/JU
 Sample : PB149716BL
 Misc :
 ALS Vial : 115 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK716

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	21	25	32	rVB	163246	198943	1.56%	0.173%
2	3.758	94	97	118	rBV	1930244	2959666	23.20%	2.570%
3	4.093	150	154	166	rVB	39829	64324	0.50%	0.056%
4	7.105	659	666	678	rBV	2180657	3343990	26.21%	2.904%
5	7.275	688	695	706	rBV	1758651	2720676	21.32%	2.363%
6	7.475	722	729	741	rBV	2208083	3449393	27.03%	2.996%
7	7.946	802	809	819	rVB	1577438	2443434	19.15%	2.122%
8	8.658	922	930	941	rBV	2450429	4007219	31.41%	3.480%
9	9.116	1000	1008	1023	rBV	1987655	3228751	25.31%	2.804%
10	9.840	1123	1131	1141	rBV	1661683	2655940	20.82%	2.307%
11	10.381	1215	1223	1240	rBV	2444306	4136576	32.42%	3.592%
12	10.757	1279	1287	1298	rBV	1970685	3348380	26.24%	2.908%
13	10.899	1302	1311	1328	rBV	2399660	4104528	32.17%	3.565%
14	12.346	1549	1557	1563	rBV	39185	71112	0.56%	0.062%
15	13.563	1758	1764	1769	rVB9	8698	17502	0.14%	0.015%
16	13.993	1829	1837	1852	rBV	3702258	5329533	41.77%	4.628%
17	14.281	1878	1886	1897	rBV	4468909	6595805	51.69%	5.728%
18	14.587	1932	1938	1952	rBV	2700006	4078754	31.97%	3.542%
19	14.787	1965	1972	1996	rBV	1478424	2493837	19.55%	2.166%
20	15.581	2100	2107	2121	rBV	5603231	8116284	63.61%	7.049%
21	15.698	2121	2127	2140	rVV	1510861	2113520	16.56%	1.835%
22	15.822	2144	2148	2154	rVB3	26294	43341	0.34%	0.038%
23	17.345	2401	2407	2417	rBV	3360320	4649157	36.44%	4.038%
24	17.445	2417	2424	2438	rBV	6357514	8851753	69.38%	7.687%
25	17.722	2469	2471	2477	rBV7	8770	12798	0.10%	0.011%
26	19.257	2727	2732	2736	rBV2	76793	116464	0.91%	0.101%
27	19.322	2739	2743	2747	rVV	71751	99820	0.78%	0.087%
28	19.675	2797	2803	2813	rBV	8630754	11423361	89.53%	9.921%
29	21.433	3097	3102	3109	rBV	4249146	5517835	43.25%	4.792%
30	23.751	3489	3496	3509	rVB2	6275834	12759141	100.00%	11.081%
31	23.910	3516	3523	3535	rVB2	2931735	6195938	48.56%	5.381%




Sum of corrected areas: 115147775

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013232.D
Acq On : 22 Dec 2022 05:25
Operator : CG/JU
Sample : PB149716BL
Misc :
ALS Vial : 115 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK716

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

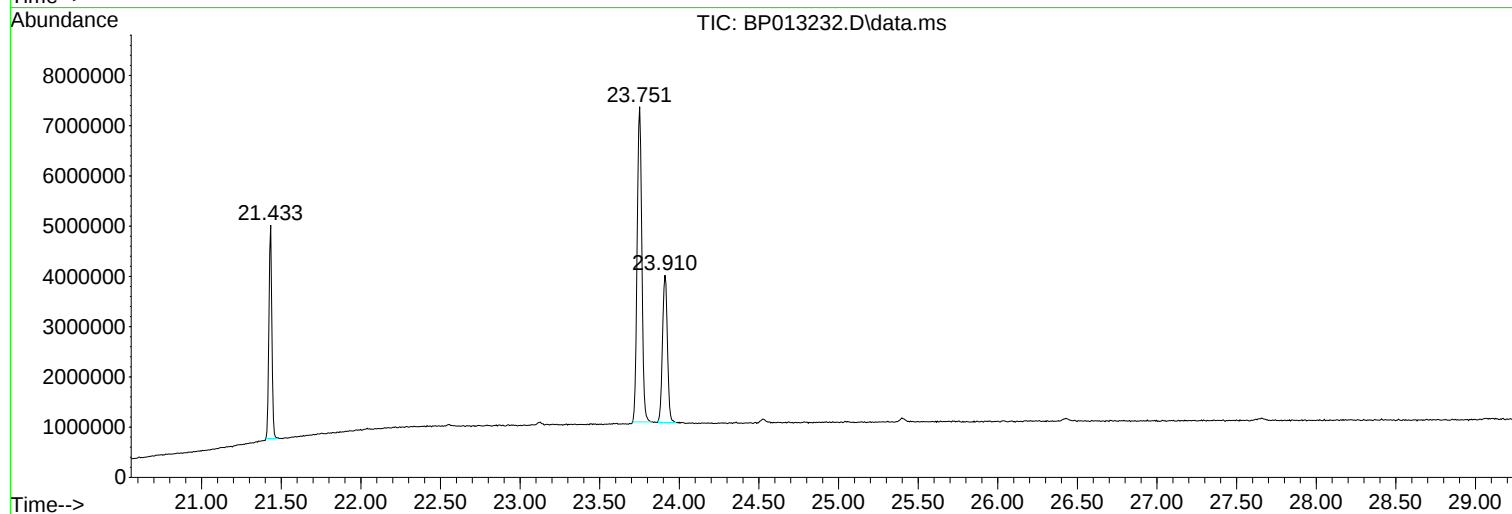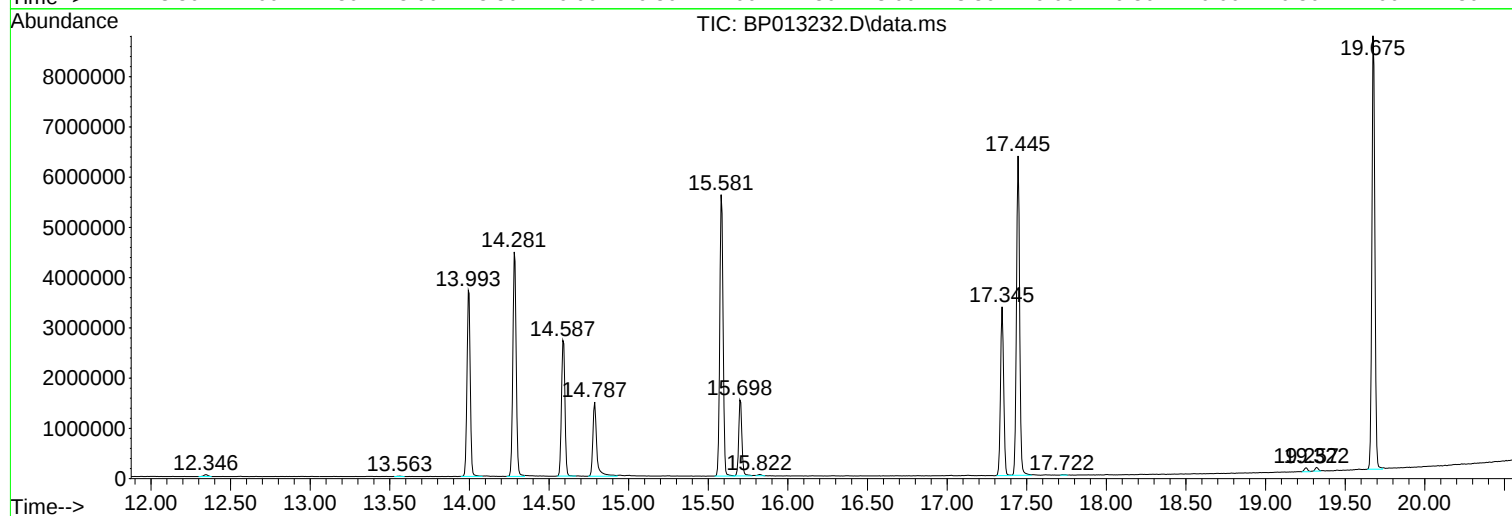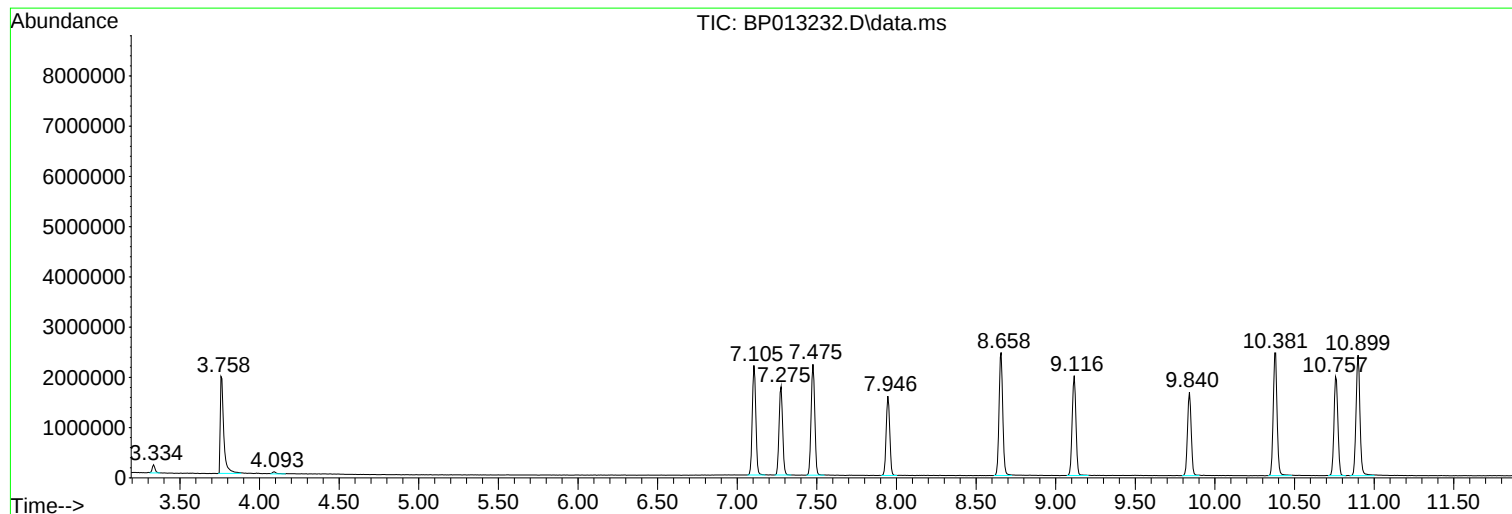

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013232.D
Acq On : 22 Dec 2022 05:25
Operator : CG/JU
Sample : PB149716BL
Misc :
ALS Vial : 115 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK716

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013232.D
Acq On : 22 Dec 2022 05:25
Operator : CG/JU
Sample : PB149716BL
Misc :
ALS Vial : 115 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK716

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc