
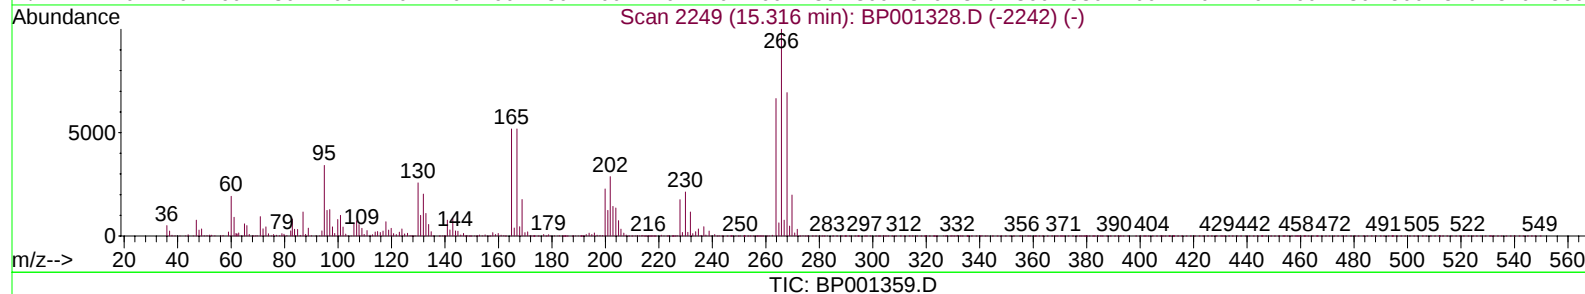
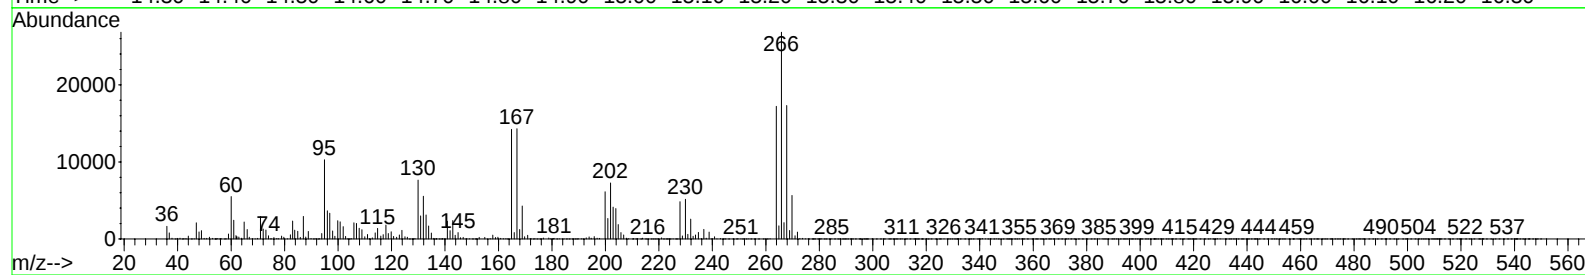


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP122319\
Data File : BP001359.D
Acq On : 23 Dec 2019 10:33
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 18:18:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP121919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 03:20:39 2019
Response via : Initial Calibration

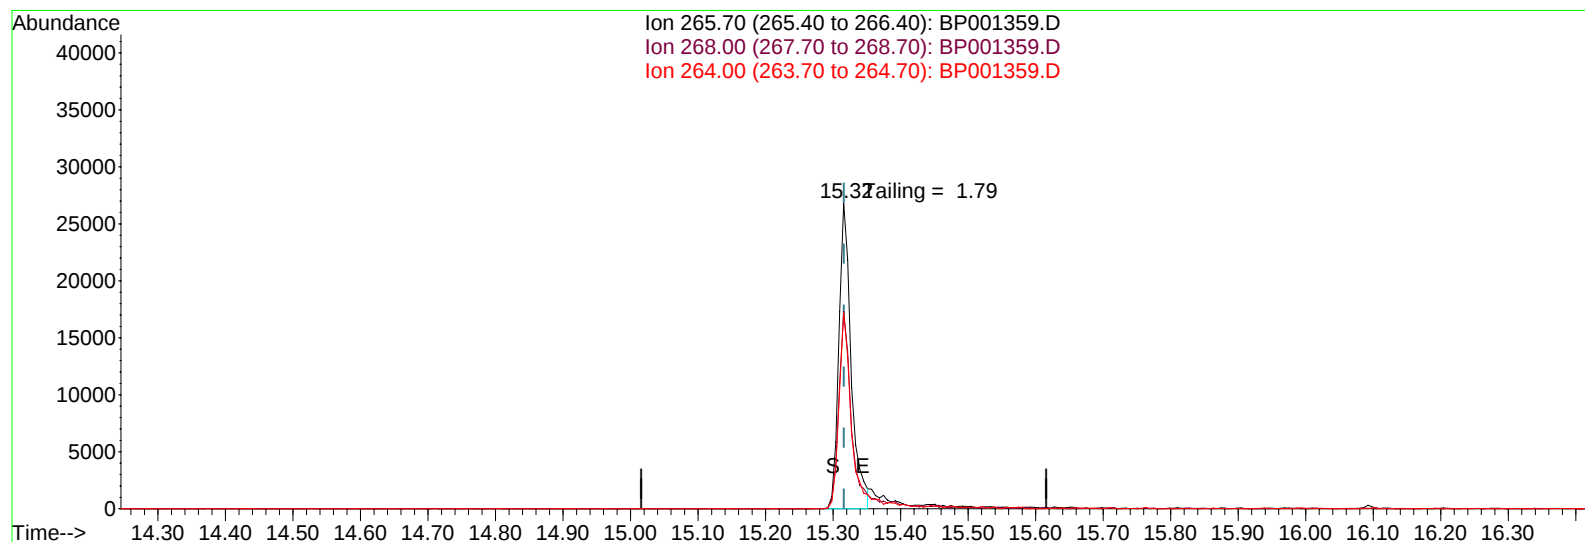

(70) Pentachlorophenol (C)




15.316min (-0.000) 415093.75ng

response 37247

Ion	Exp%	Act%
265.70	100	100
268.00	69.30	64.52
264.00	66.50	64.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP122319\
 Data File : BP001359.D
 Acq On : 23 Dec 2019 10:33
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 18:18:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP121919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 20 03:20:39 2019
 Response via : Initial Calibration

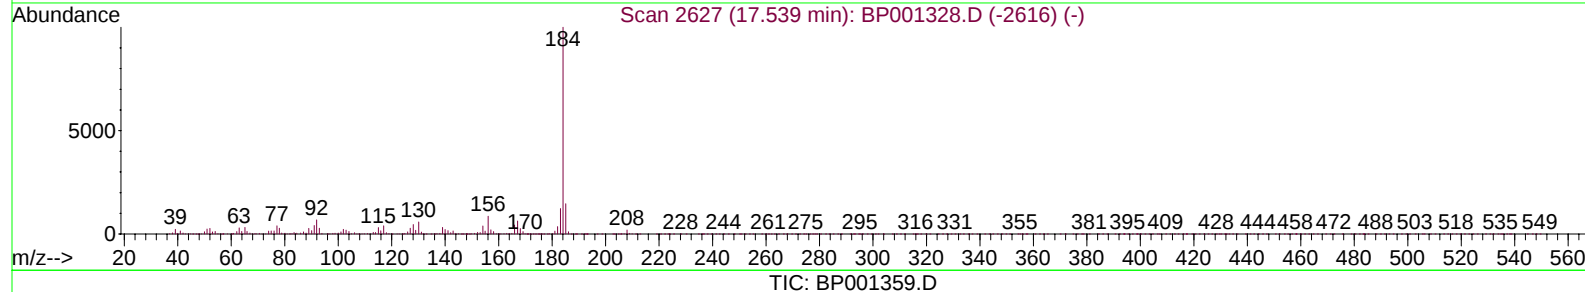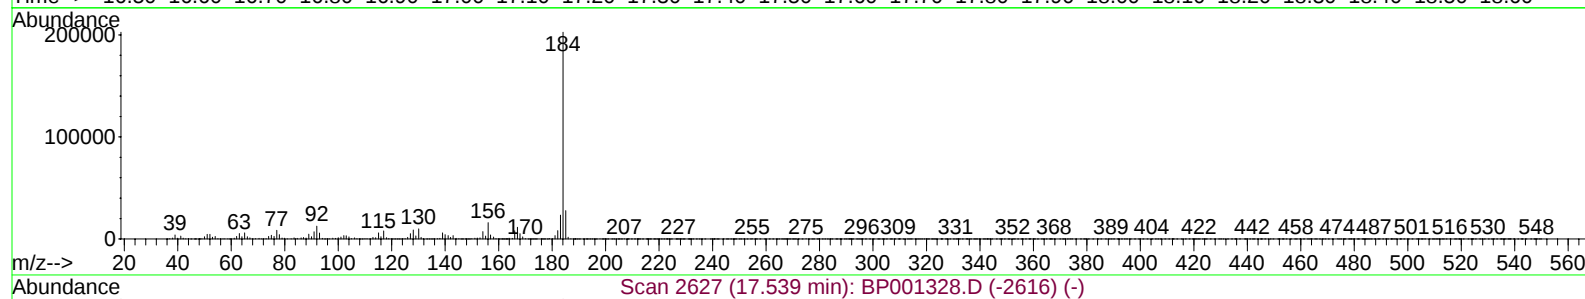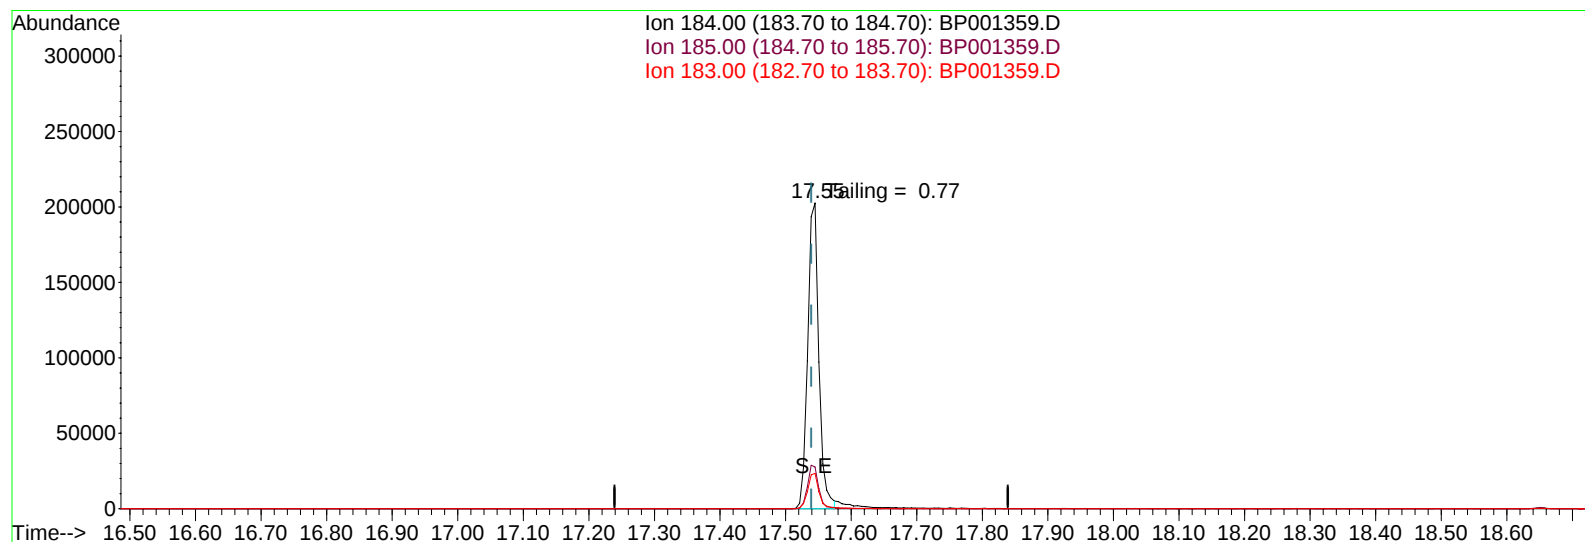

(77) Benzidine

17.545min (+0.006) 330482.07ng

response 250173

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	13.69
183.00	12.30	11.56
0.00	0.00	0.00