


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_P\DATA\BP122319\  
 Data File : BP001359.D  
 Acq On : 23 Dec 2019 10:33  
 Operator : JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP121919.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Dec 24 16:04:49 2019

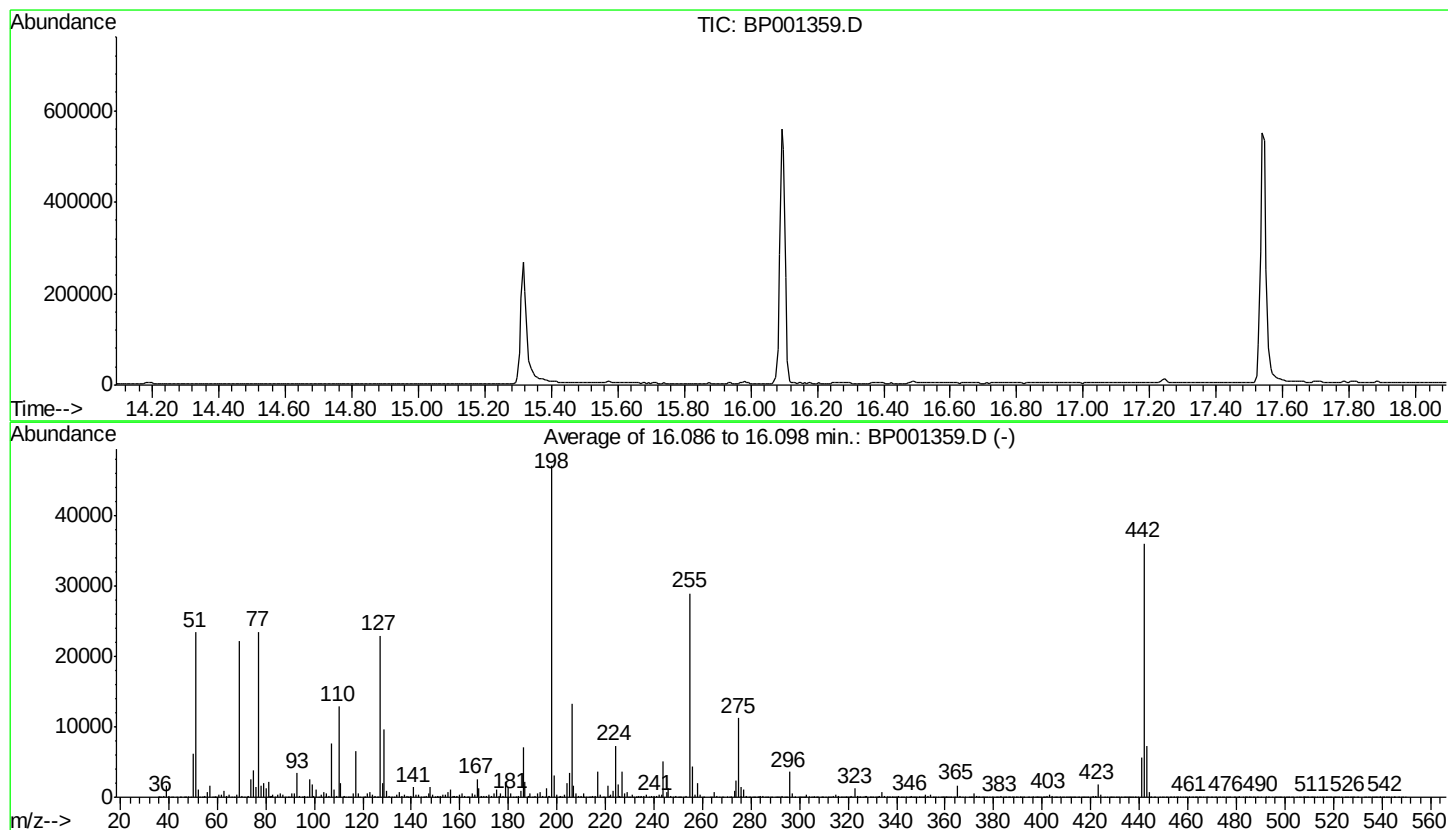

AutoFind: Scans 2380, 2381, 2382; Background Corrected with Scan 2373

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 49.8      | 23426   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.9       | 425     | PASS             |
| 69          | 198          | 0.00         | 100          | 47.1      | 22184   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 124     | PASS             |
| 127         | 198          | 10           | 80           | 48.6      | 22897   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.3       | 155     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 47072   | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 3129    | PASS             |
| 275         | 198          | 10           | 60           | 23.8      | 11224   | PASS             |
| 365         | 198          | 1            | 100          | 3.7       | 1730    | PASS             |
| 441         | 198          | 0.01         | 100          | 11.9      | 5581    | PASS             |
| 442         | 198          | 50           | 100          | 76.5      | 36033   | PASS             |
| 443         | 442          | 15           | 24           | 20.2      | 7268    | PASS             |