




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
 Data File : BP008543.D
 Acq On : 24 Dec 2021 01:35
 Operator : CG/JU
 Sample : M5126-19
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J28

Manual IntegrationsAPPROVED

Quant Time: Dec 24 04:16:06 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 23 14:48:11 2021
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/27/2021
 Supervised By :mohammad ahmed 12/31/2021

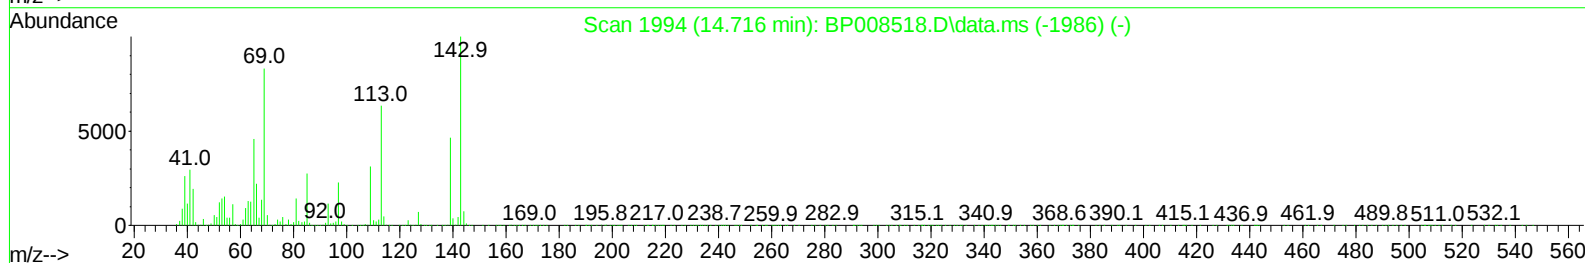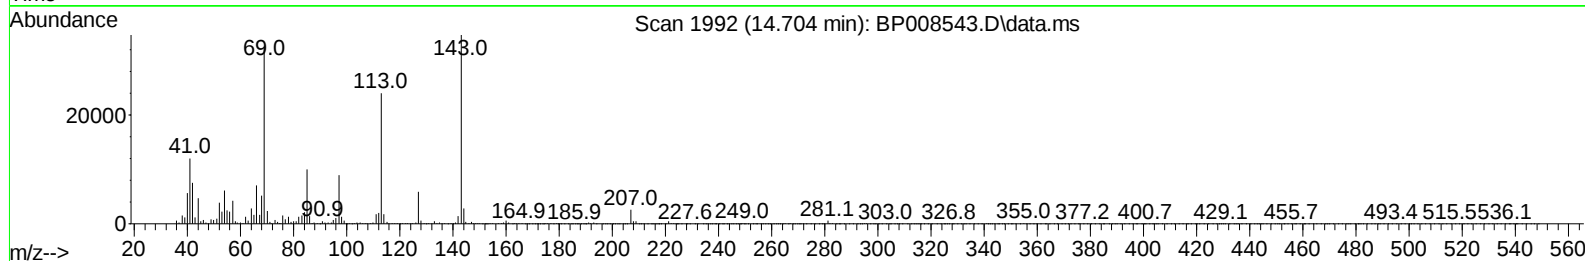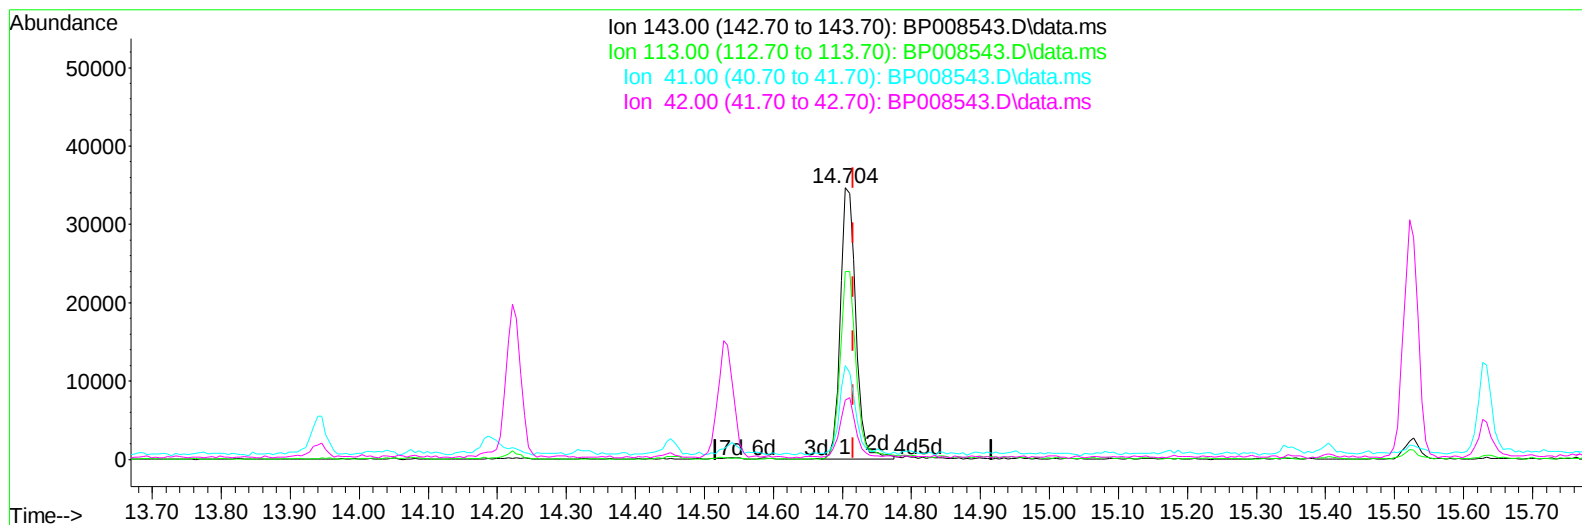

TIC: BP008543.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.704min (-0.012) 4.40 ng/ul m

response 54034

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	64.30	69.30
41.00	32.30	34.63
42.00	21.80	21.85




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
 Data File : BP008543.D
 Acq On : 24 Dec 2021 01:35
 Operator : CG/JU
 Sample : M5126-19
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J28

Manual IntegrationsAPPROVED

Quant Time: Jan 02 03:42:10 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 23 14:48:11 2021
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/27/2021
 Supervised By :mohammad ahmed 12/31/2021

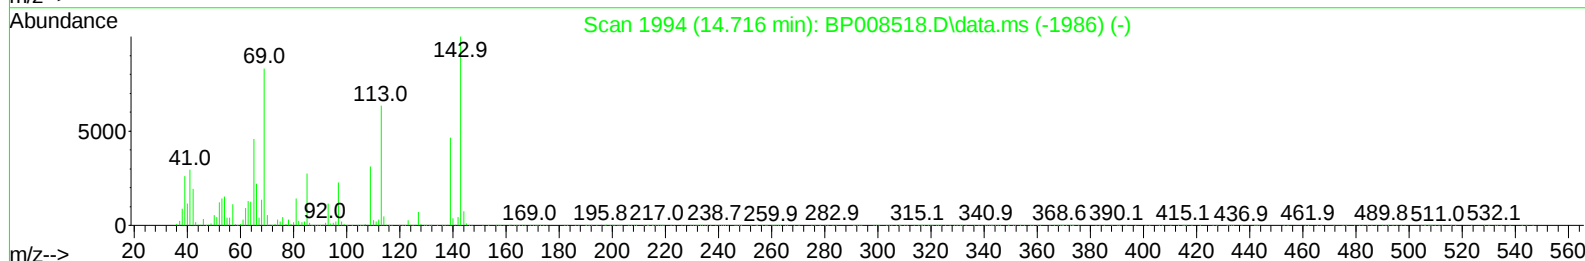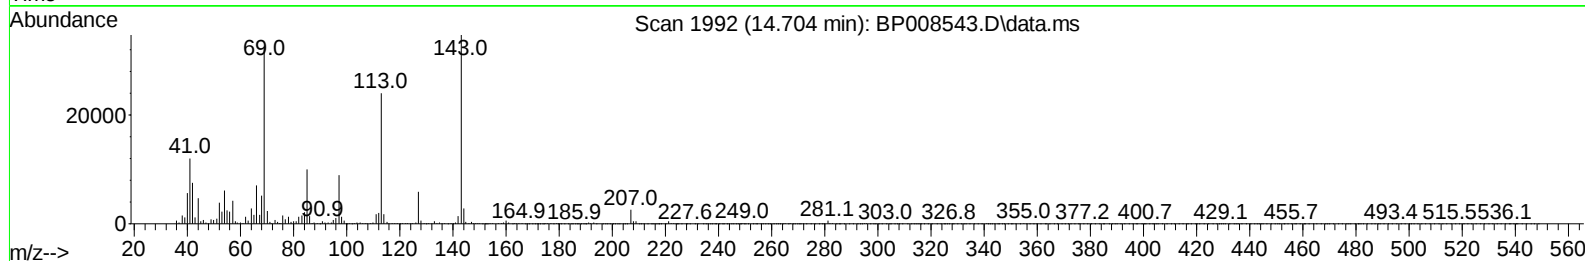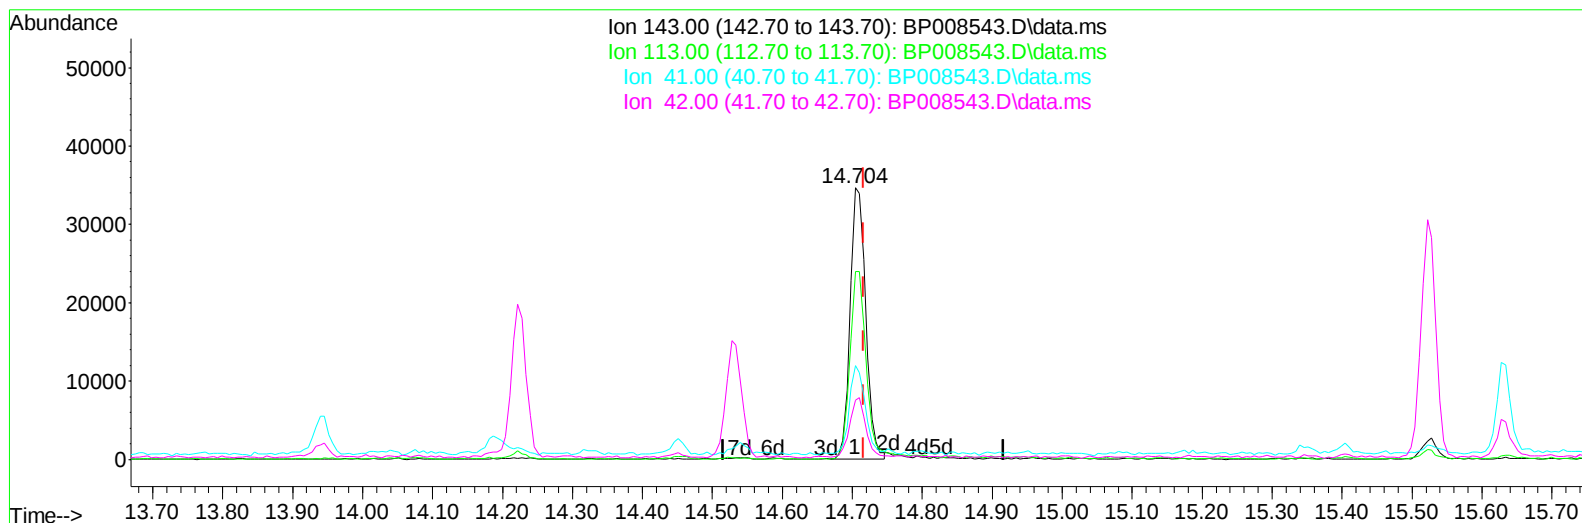

TIC: BP008543.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.704min (-0.012) 4.32 ng/u1

response 52969

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	64.30	69.30
41.00	32.30	34.63
42.00	21.80	21.85

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
 Data File : BP008543.D
 Acq On : 24 Dec 2021 01:35
 Operator : CG/JU
 Sample : M5126-19
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J28

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/27/2021
 Supervised By :mohammad ahmed 12/31/2021

Quant Time: Dec 24 04:16:06 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 23 14:48:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	441097	20.000	ng/ul	0.00
20) Naphthalene-d8	10.704	136	1717049	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.534	164	1047720	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	2002966	20.000	ng/ul	0.00
79) Chrysene-d12	21.357	240	1779621	20.000	ng/ul	0.00
88) Perylene-d12	23.792	264	1980689	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	44841	4.582	ng/uL	0.00
4) Pyridine-d5	3.764	84	136413	4.981	ng/ul	0.00
7) Phenol-d5	7.058	99	185230	5.264	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	626935	31.368	ng/ul	0.00
11) 2-Chlorophenol-d4	7.434	132	679979	24.291	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	367309	13.012	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	432485	35.595	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	397610	35.691	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	785182	28.712	ng/ul	0.00
31) 4-Chloroaniline-d4	10.834	131	879014	23.286	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	2751754	35.547	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	3484007	35.994	ng/ul	0.00
54) 4-Nitrophenol-d4	14.704	143	54034m	4.403	ng/ul	-0.01
60) Fluorene-d10	15.522	176	2541663	37.816	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200	257004	29.148	ng/ul	0.00
73) Anthracene-d10	17.381	188	4306833	45.375	ng/ul	0.00
81) Pyrene-d10	19.610	212	4579237	42.942	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.633	264	4596372	45.088	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
Data File : BP008543.D
Acq On : 24 Dec 2021 01:35
Operator : CG/JU
Sample : M5126-19
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J28

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/27/2021
Supervised By :mohammad ahmed 12/31/2021

Quant Time: Dec 24 04:16:06 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 23 14:48:11 2021
Response via : Initial Calibration

