

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
 Data File : BP008525.D
 Acq On : 23 Dec 2021 15:27
 Operator : CG/JU
 Sample : M5153-05ME
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGL70ME

Quant Time: Dec 24 04:10:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 23 14:48:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	418811	20.000	ng/ul	0.00
20) Naphthalene-d8	10.704	136	1625348	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.534	164	983282	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	1818237	20.000	ng/ul	0.00
79) Chrysene-d12	21.363	240	1627866	20.000	ng/ul	0.00
88) Perylene-d12	23.798	264	1822098	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	19813	2.132	ng/uL	0.00
4) Pyridine-d5	3.764	84	96571	3.714	ng/ul	0.00
7) Phenol-d5	7.058	99	303511	9.084	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	205985	10.855	ng/ul	0.00
11) 2-Chlorophenol-d4	7.434	132	261851	9.852	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	240796	8.984	ng/ul	0.00
21) Nitrobenzene-d5	9.058	128	122044	10.611	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	104958	9.953	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	231688	8.950	ng/ul	0.00
31) 4-Chloroaniline-d4	10.834	131	316503	8.857	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	864429	11.898	ng/ul	0.00
49) Acenaphthylene-d8	14.228	160	914903	10.071	ng/ul	0.00
54) 4-Nitrophenol-d4	14.710	143	68748	5.970	ng/ul	0.00
60) Fluorene-d10	15.528	176	695150	11.021	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.628	200	48810	6.098	ng/ul	-0.01
73) Anthracene-d10	17.381	188	1007760	11.696	ng/ul	0.00
81) Pyrene-d10	19.610	212	1072198	10.992	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.639	264	1020015	10.877	ng/ul	0.00
Target Compounds						
					Qvalue	
83) Butylbenzylphthalate	20.522	149	105939	2.675	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.292	149	4827074	80.290	ng/ul	99
89) Di-n-octyl phthalate	22.239	149	2470939	21.296	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
Data File : BP008525.D
Acq On : 23 Dec 2021 15:27
Operator : CG/JU
Sample : M5153-05ME
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGL70ME

Quant Time: Dec 24 04:10:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 23 14:48:11 2021
Response via : Initial Calibration




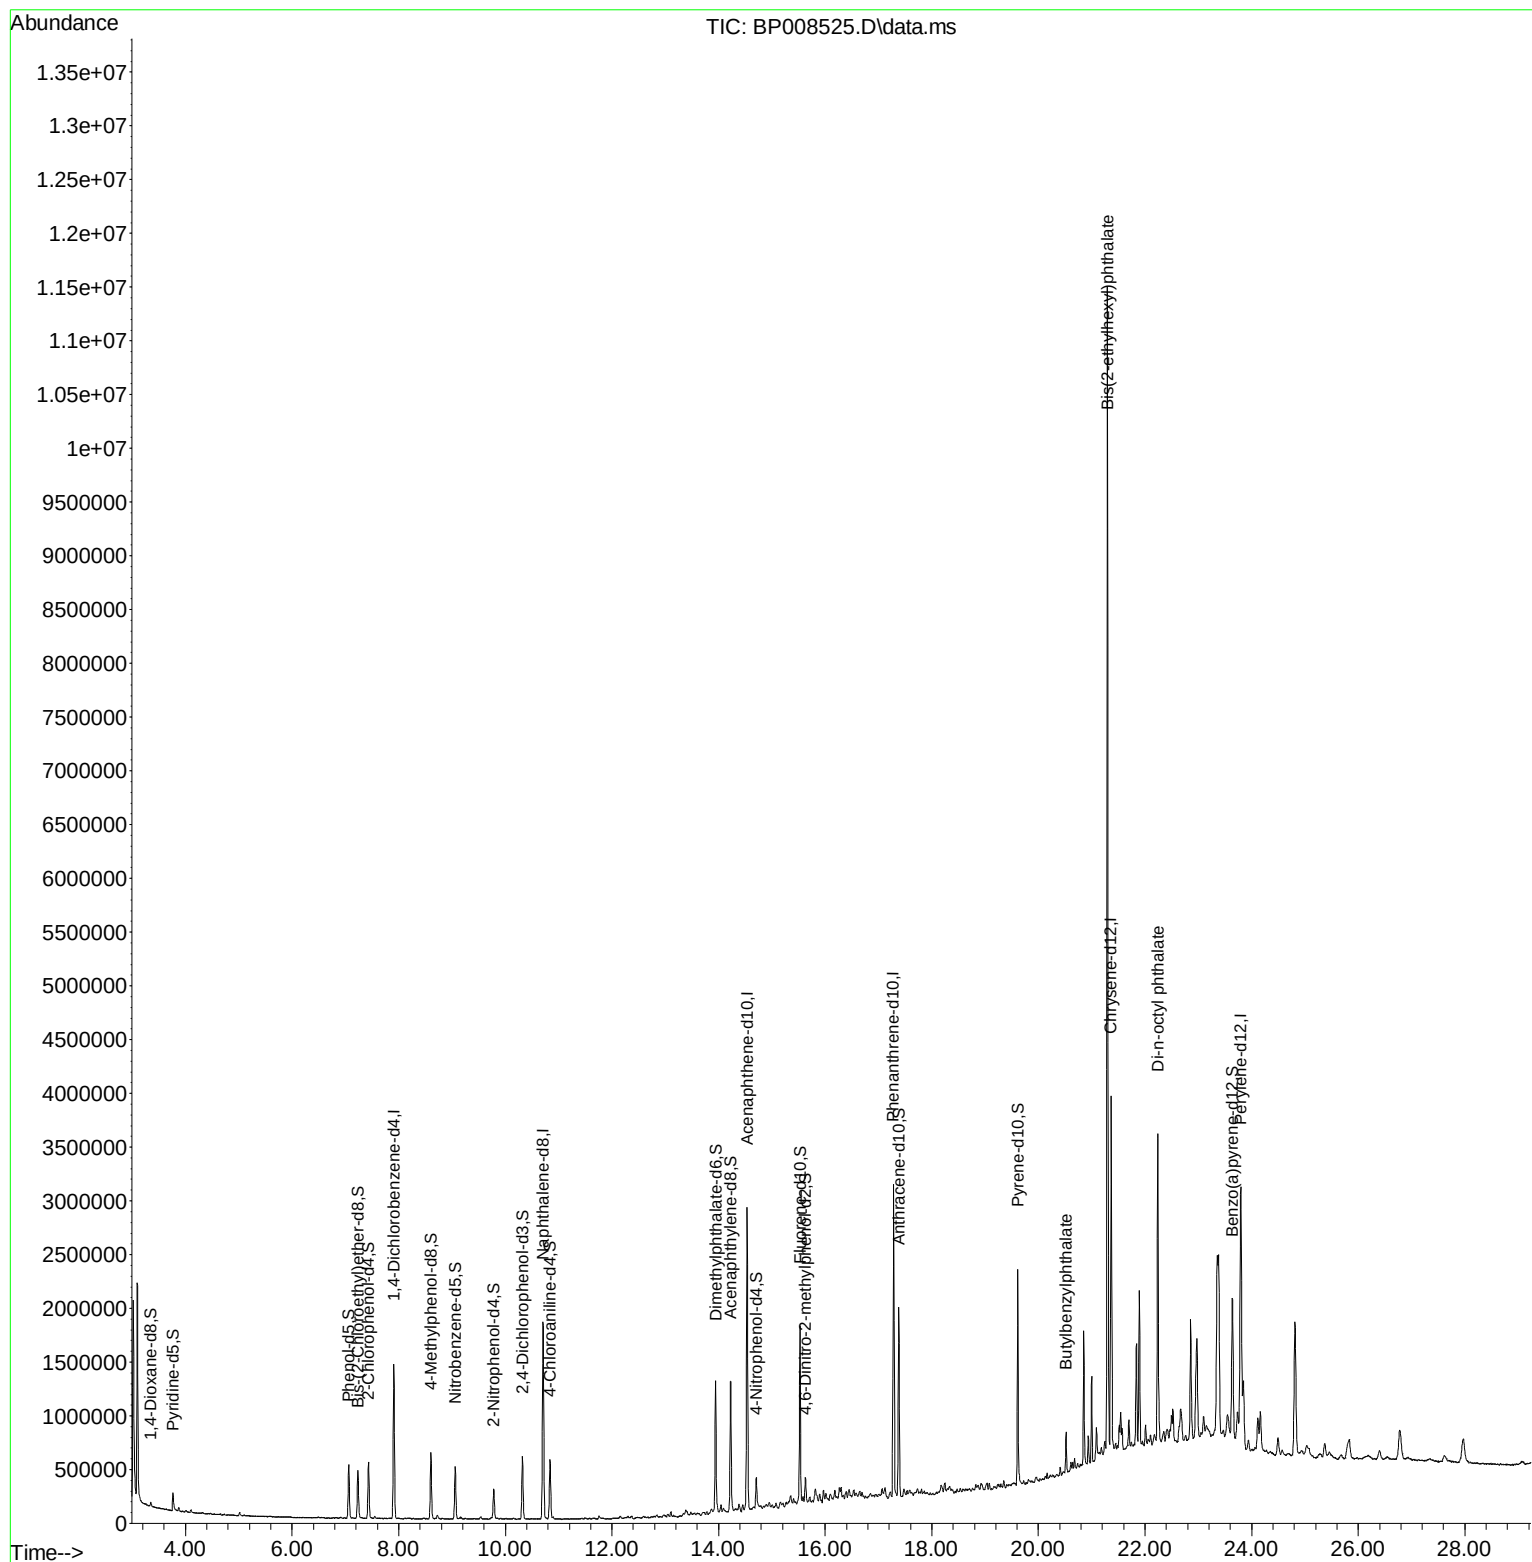


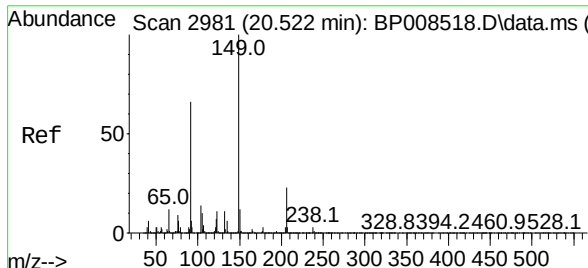

Butylbenzylphthalate
 Concen: 2.675 ng/ul
 RT: 20.522 min Scan# 2981
 Delta R.T. 0.000 min
 Lab File: BP008525.D
 Acq: 23 Dec 2021 15:27




Instrument :
 BNA_P
 ClientSampleId :
 BGL70ME

Tgt Ion:	149	Resp:	105939
Ion	Ratio	Lower	Upper
149	100		
91	67.0	53.4	80.2
206	23.4	18.2	27.2

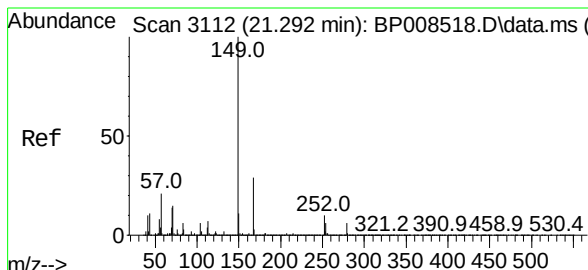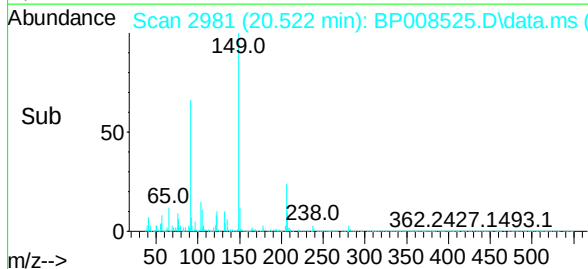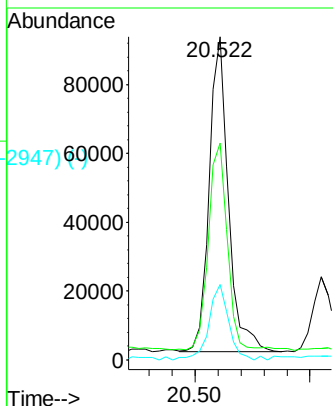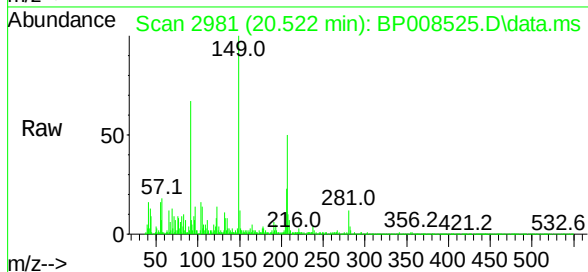


Bis(2-ethylhexyl)phthalate
 Concen: 80.290 ng/ul
 RT: 21.292 min Scan# 3112
 Delta R.T. 0.000 min
 Lab File: BP008525.D
 Acq: 23 Dec 2021 15:27

Tgt Ion:	149	Resp:	4827074
Ion	Ratio	Lower	Upper
149	100		
167	28.1	23.0	34.4
279	5.2	3.7	5.5

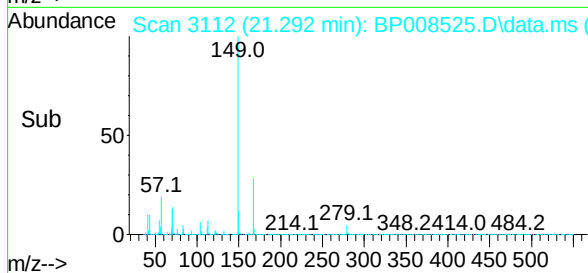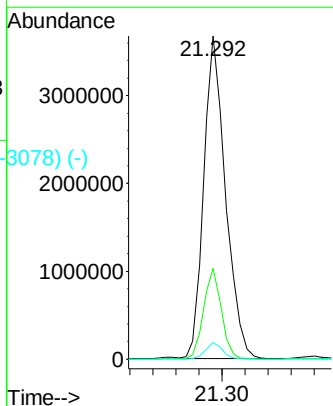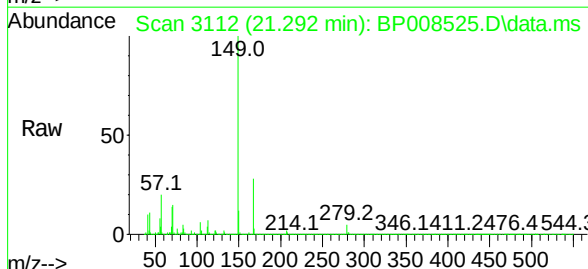

Abundance Scan 3271 (22.227 min): BP008518.D\data.ms (-3289)

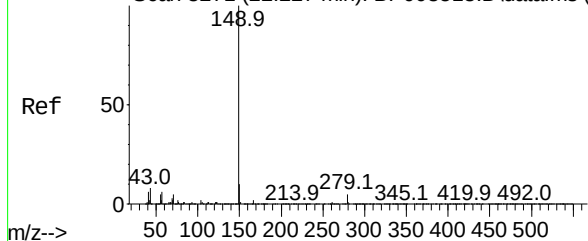


Di-n-octyl phthalate
Concen: 21.296 ng/ul
RT: 22.239 min Scan# 3273
Delta R.T. 0.012 min
Lab File: BP008525.D
Acq: 23 Dec 2021 15:27

Instrument :
BNA_P
ClientSampleId :
BGL70ME

Tgt Ion:149 Resp: 2470939

Abundance Scan 3273 (22.239 min): BP008525.D\data.ms

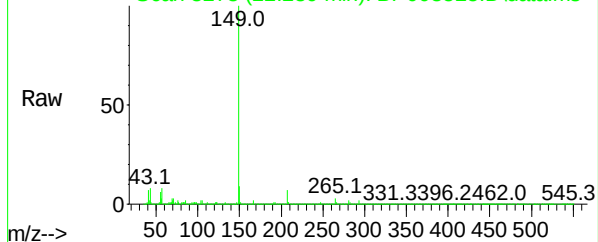

Abundance Scan 3273 (22.239 min): BP008525.D\data.ms (-32310)

