

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
 Data File : BP008535.D
 Acq On : 23 Dec 2021 21:05
 Operator : CG/JU
 Sample : M5090-16
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BG3C8

Quant Time: Dec 24 04:13:47 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 23 14:48:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	603981	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	2526311	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.545	164	1615562	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.280	188	3459892	20.000	ng/ul	0.00
79) Chrysene-d12	21.363	240	3272067	20.000	ng/ul	0.00
88) Perylene-d12	23.792	264	2628835	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	55222	4.121	ng/uL	0.00
4) Pyridine-d5	3.758	84	211714	5.646	ng/ul	0.00
7) Phenol-d5	7.057	99	306409	6.359	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	889848	32.515	ng/ul	0.00
11) 2-Chlorophenol-d4	7.434	132	973492	25.398	ng/ul	0.00
15) 4-Methylphenol-d8	8.604	113	602471	15.587	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	649082	36.309	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	617481	37.672	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	1192558	29.640	ng/ul	0.00
31) 4-Chloroaniline-d4	10.834	131	1805389	32.506	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	4022218	33.696	ng/ul	0.00
49) Acenaphthylene-d8	14.245	160	5191980	34.786	ng/ul	0.02
54) 4-Nitrophenol-d4	14.710	143	108373	5.727	ng/ul	0.00
60) Fluorene-d10	15.528	176	3750607	36.190	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.639	200	431082	28.304	ng/ul	0.00
73) Anthracene-d10	17.380	188	6012140	36.669	ng/ul	0.00
81) Pyrene-d10	19.616	212	6889423	35.138	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.639	264	5076321	37.519	ng/ul	0.00


Target Compounds					Qvalue
8) Phenol	7.087	94	402888	8.138 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
Data File : BP008535.D
Acq On : 23 Dec 2021 21:05
Operator : CG/JU
Sample : M5090-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3C8


Quant Time: Dec 24 04:13:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 23 14:48:11 2021
Response via : Initial Calibration

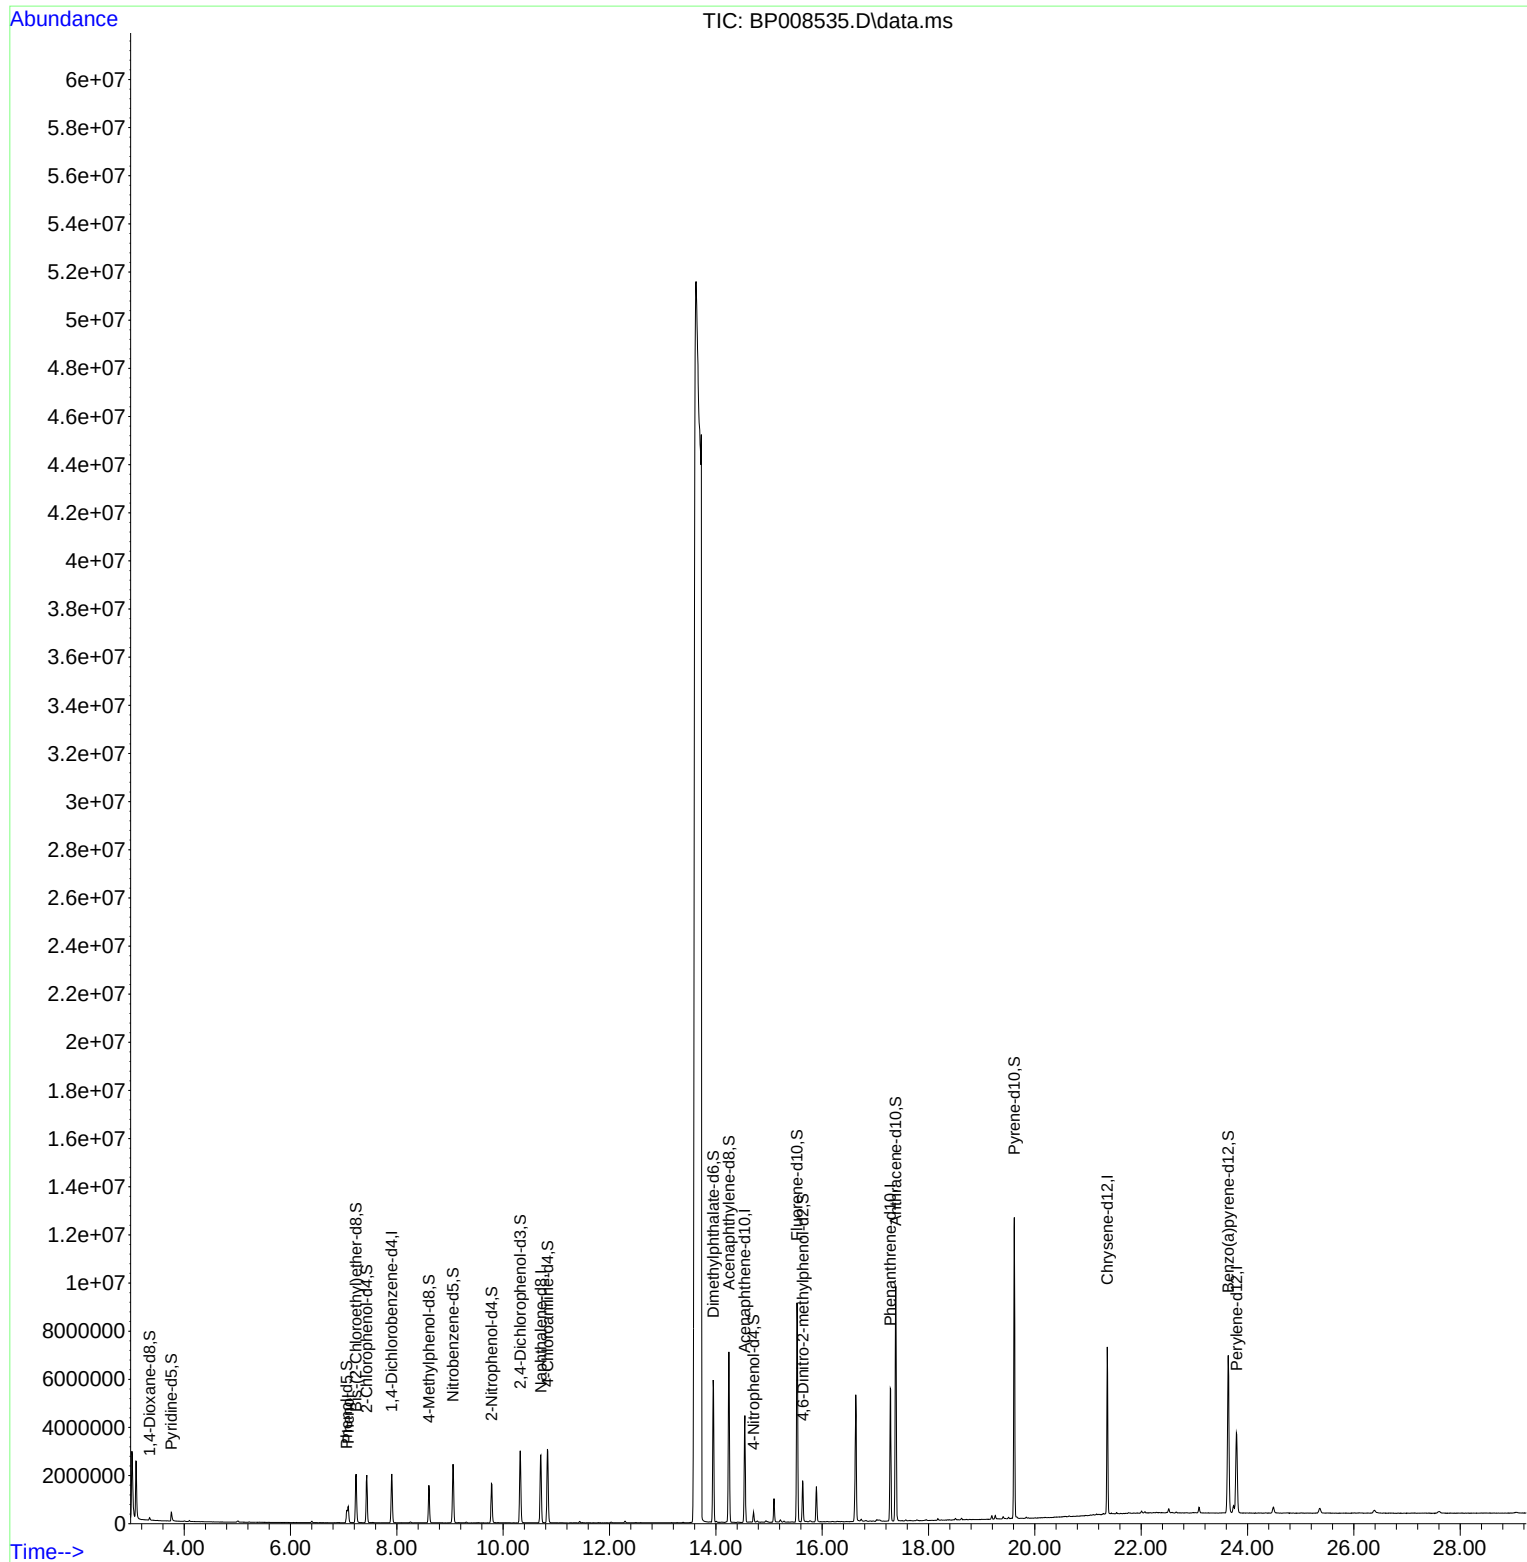

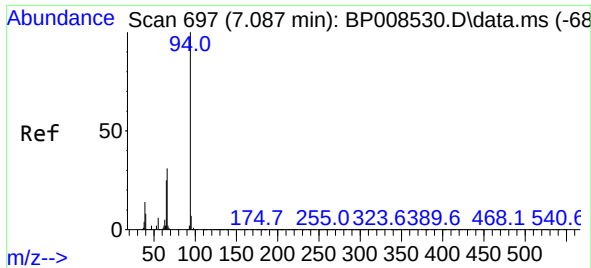

#8
Phenol
Concen: 8.138 ng/ul
RT: 7.087 min Scan# 697
Delta R.T. -0.000 min
Lab File: BP008535.D
Acq: 23 Dec 2021 21:05

Instrument :
BNA_P
ClientSampleId :
BG3C8

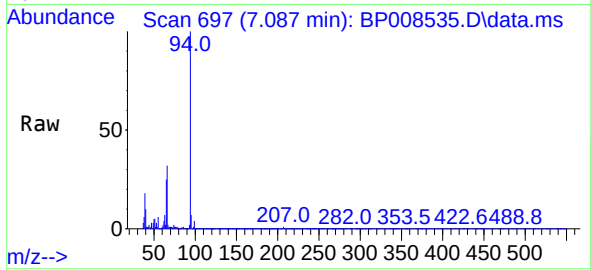

Tgt Ion: 94 Resp: 402888

Ion	Ratio	Lower	Upper
94	100		
65	24.8	20.6	31.0
66	32.1	26.3	39.5

