

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
 Data File : BP008536.D
 Acq On : 23 Dec 2021 21:39
 Operator : CG/JU
 Sample : M5090-19
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BG3F5

Quant Time: Dec 24 04:14:04 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 23 14:48:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	563615	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	2276217	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.540	164	1306837	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	2512360	20.000	ng/ul	0.00
79) Chrysene-d12	21.363	240	1874534	20.000	ng/ul	0.00
88) Perylene-d12	23.792	264	1852953	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	59710	4.775	ng/uL	0.00
4) Pyridine-d5	3.764	84	65201	1.863	ng/ul	0.00
7) Phenol-d5	7.058	99	340385	7.570	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	836232	32.745	ng/ul	0.00
11) 2-Chlorophenol-d4	7.434	132	950020	26.561	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	616086	17.081	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	598316	37.147	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	564539	38.226	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	1095671	30.224	ng/ul	0.00
31) 4-Chloroaniline-d4	10.834	131	666124	13.311	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	3458597	35.819	ng/ul	0.00
49) Acenaphthylene-d8	14.240	160	4481984	37.123	ng/ul	0.01
54) 4-Nitrophenol-d4	14.710	143	100813	6.587	ng/ul	0.00
60) Fluorene-d10	15.528	176	3159870	37.693	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200	346815	31.359	ng/ul	0.00
73) Anthracene-d10	17.381	188	4801454	40.330	ng/ul	0.00
81) Pyrene-d10	19.610	212	4963100	44.185	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.633	264	3943567	41.351	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.087	94	239251	5.179	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
Data File : BP008536.D
Acq On : 23 Dec 2021 21:39
Operator : CG/JU
Sample : M5090-19
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3F5


Quant Time: Dec 24 04:14:04 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 23 14:48:11 2021
Response via : Initial Calibration

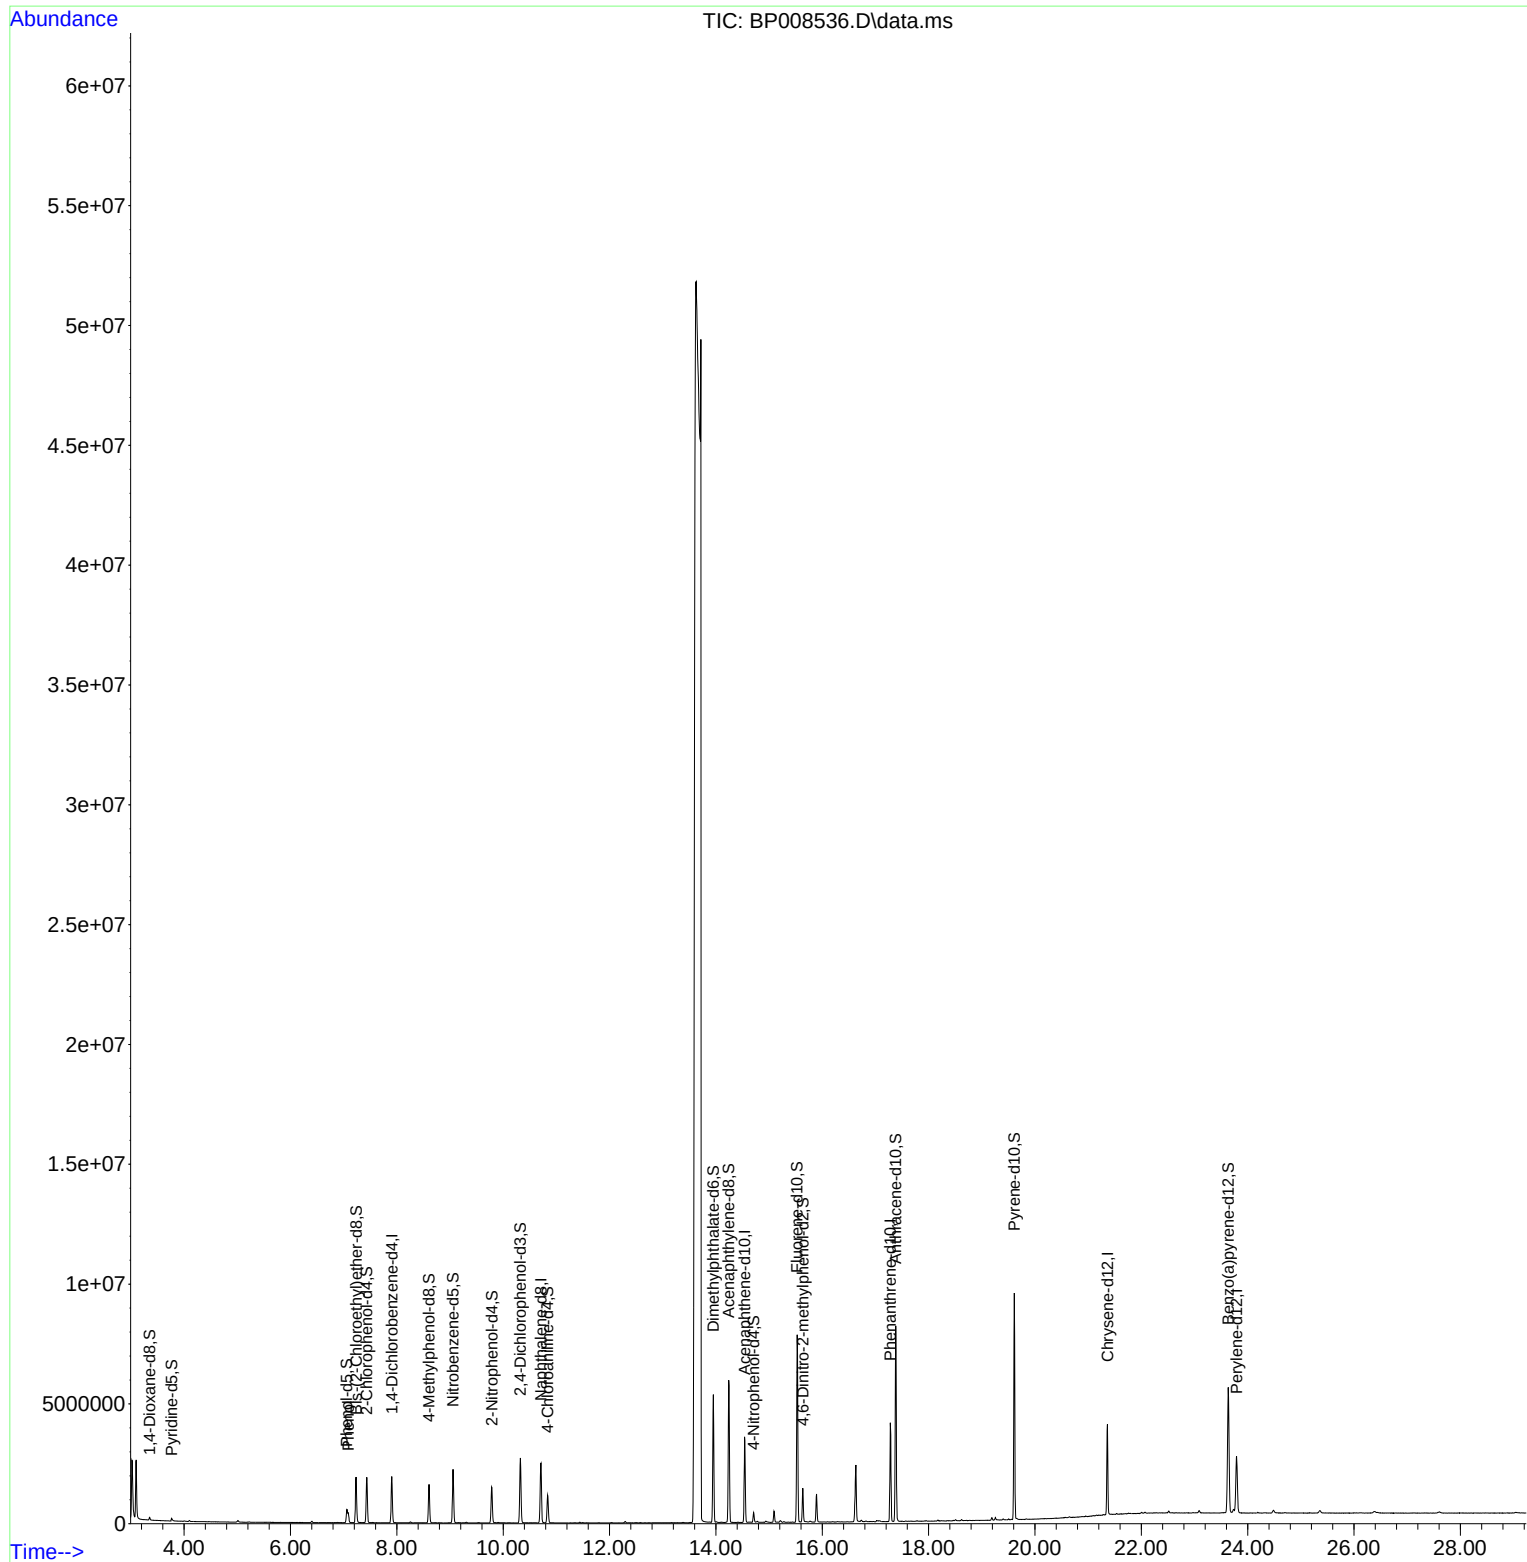

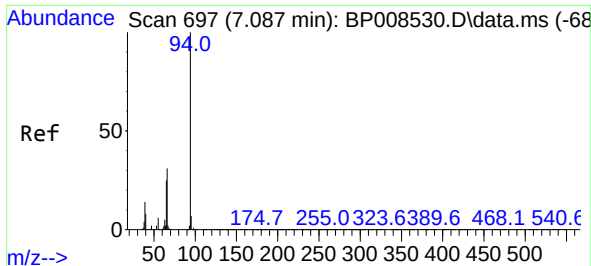

#8
Phenol
Concen: 5.179 ng/ul
RT: 7.087 min Scan# 697
Delta R.T. 0.000 min
Lab File: BP008536.D
Acq: 23 Dec 2021 21:39

Instrument :
BNA_P
ClientSampleId :
BG3F5

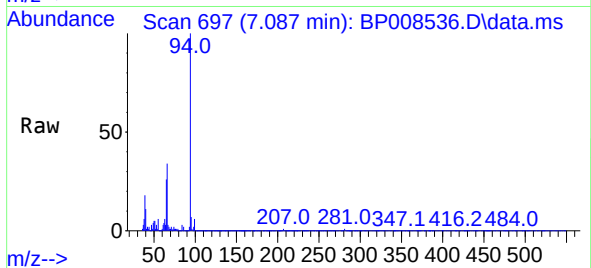

Tgt Ion: 94 Resp: 239251

Ion	Ratio	Lower	Upper
94	100		
65	25.8	20.6	31.0
66	33.9	26.3	39.5

