

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
 Data File : BP008523.D
 Acq On : 23 Dec 2021 14:18
 Operator : CG/JU
 Sample : PB141621BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK621

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
 Title : SVOA CALIBRATION

Signal : TIC: BP008523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.023	3	6	16	rVB	306819	425144	4.18%	0.413%
2	3.352	59	62	69	rVB	140806	183664	1.81%	0.178%
3	3.758	128	131	151	rVB	1271084	1814533	17.84%	1.762%
4	4.105	187	190	194	rVB	25948	31683	0.31%	0.031%
5	7.064	686	693	704	rBV	1739298	2735893	26.90%	2.656%
6	7.240	716	723	738	rVB	1428751	2240017	22.03%	2.175%
7	7.440	750	757	768	rBV	1829401	2889774	28.42%	2.805%
8	7.911	830	837	844	rVB	1448380	2284289	22.46%	2.218%
9	8.611	948	956	965	rBV	2135475	3400121	33.43%	3.301%
10	9.063	1026	1033	1043	rBV	1514532	2531867	24.90%	2.458%
11	9.793	1146	1157	1166	rBV	1037239	1744936	17.16%	1.694%
12	10.328	1238	1248	1259	rBV	2087595	3479893	34.22%	3.378%
13	10.716	1306	1314	1322	rVB	1789956	3108600	30.57%	3.018%
14	10.840	1327	1335	1350	rBV	1789116	3023006	29.73%	2.935%
15	12.299	1578	1583	1588	rBV	40563	63411	0.62%	0.062%
16	13.281	1743	1750	1753	rBV6	6111	11086	0.11%	0.011%
17	13.516	1787	1790	1795	rVB3	9927	14403	0.14%	0.014%
18	13.951	1856	1864	1878	rBV	3889674	5327246	52.38%	5.172%
19	14.234	1904	1912	1925	rBV	4549671	6606959	64.97%	6.414%
20	14.546	1957	1965	1973	rBV	2842778	4252136	41.81%	4.128%
21	14.716	1984	1994	2007	rBV	1417511	2046108	20.12%	1.986%
22	15.534	2126	2133	2144	rVB	5643840	8173761	80.38%	7.935%
23	15.640	2145	2151	2170	rVV	950235	1345716	13.23%	1.306%
24	15.775	2170	2174	2182	rVB	26738	45232	0.44%	0.044%
25	16.204	2243	2247	2255	rBV	9645	20900	0.21%	0.020%
26	16.328	2264	2268	2273	rVB6	8201	16656	0.16%	0.016%
27	16.969	2373	2377	2381	rVB7	8179	13163	0.13%	0.013%
28	17.075	2389	2395	2402	rBV2	17463	33295	0.33%	0.032%
29	17.292	2425	2432	2441	rBV	3520719	4881908	48.01%	4.740%
30	17.392	2441	2449	2458	rBV	6092805	8725802	85.80%	8.471%
31	17.663	2490	2495	2496	rBV4	12732	17353	0.17%	0.017%
32	19.198	2752	2756	2761	rBV2	76158	107674	1.06%	0.105%
33	19.269	2763	2768	2771	rBV	73426	105410	1.04%	0.102%
34	19.622	2822	2828	2839	rBV	7605508	10169488	100.00%	9.873%
35	21.375	3121	3126	3143	rVB	3977315	5483985	53.93%	5.324%
36	23.651	3506	3513	3525	rVB2	4990001	10152482	99.83%	9.856%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
Data File : BP008523.D
Acq On : 23 Dec 2021 14:18
Operator : CG/JU
Sample : PB141621BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Title : SVOA CALIBRATION

37 23.810 3534 3540 3551 rVB2 2657205 5496972 54.05% 5.337%




Sum of corrected areas: 103004566

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
Data File : BP008523.D
Acq On : 23 Dec 2021 14:18
Operator : CG/JU
Sample : PB141621BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

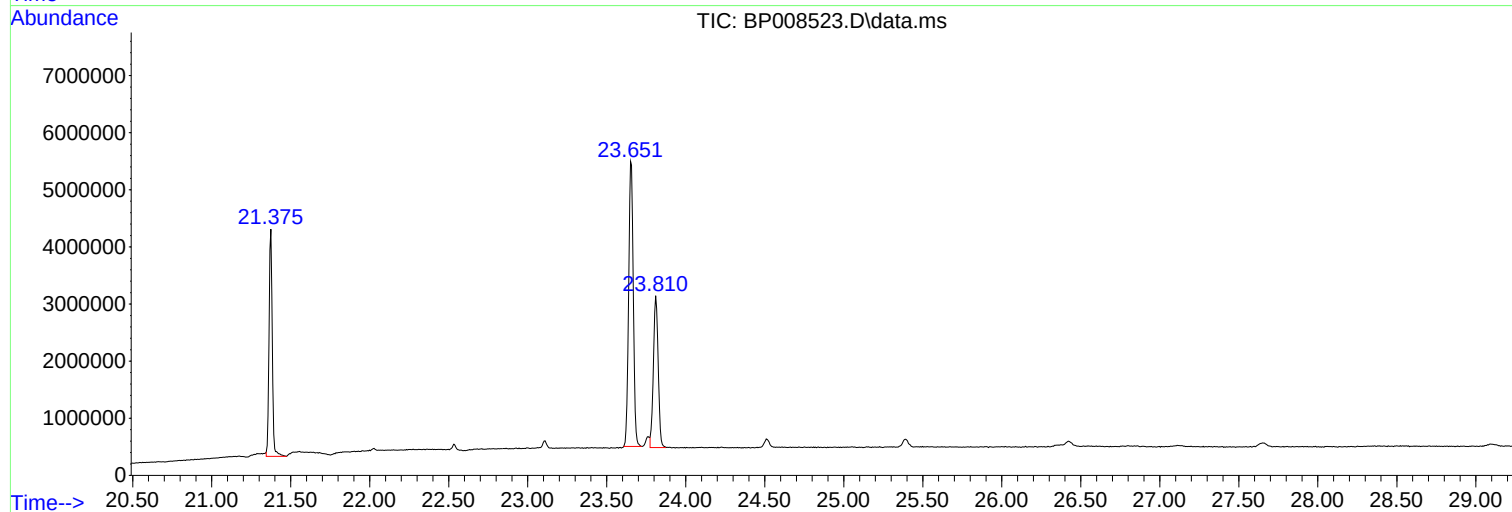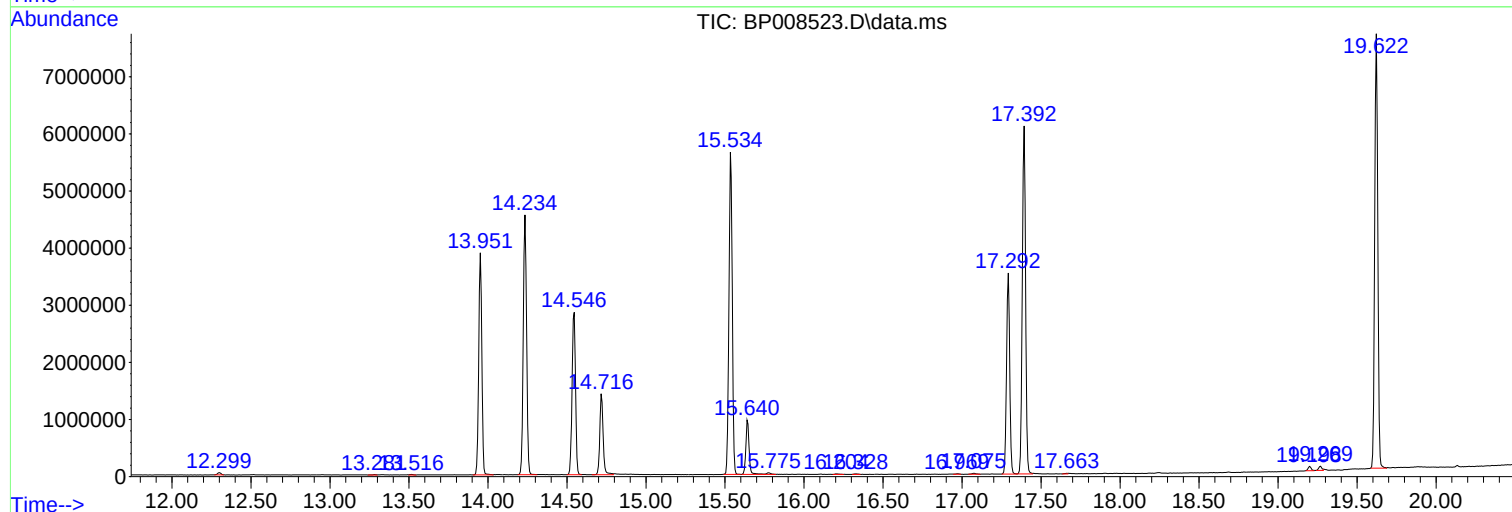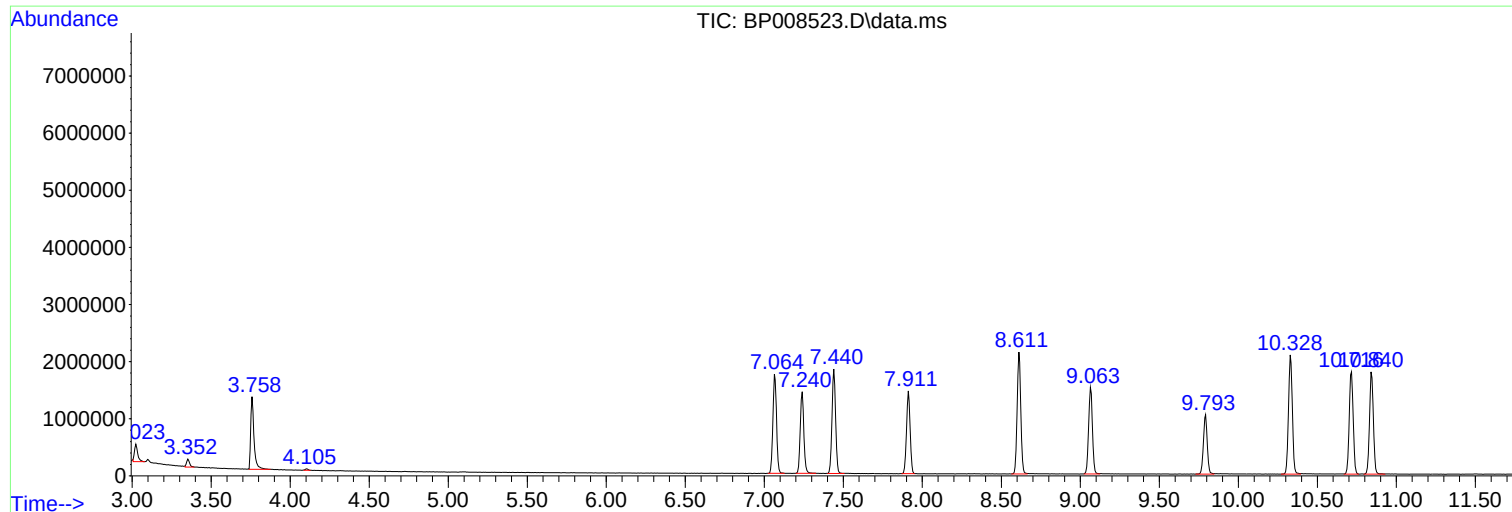

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
Data File : BP008523.D
Acq On : 23 Dec 2021 14:18
Operator : CG/JU
Sample : PB141621BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic3.023 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.023	3.72 ng/ul	425144	1,4-Dichlorobenzene-d4	7.911

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexane	84	C6H12	000110-82-7	91
2			Cyclohexane	84	C6H12	000110-82-7	91
3			Cyclohexane	84	C6H12	000110-82-7	91
4			Cyclohexane	84	C6H12	000110-82-7	91
5			Cyclopentane, methyl-	84	C6H12	000096-37-7	90

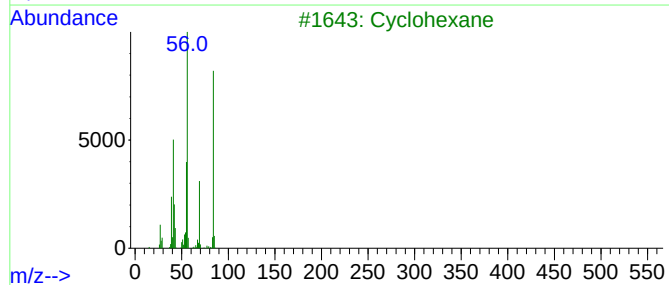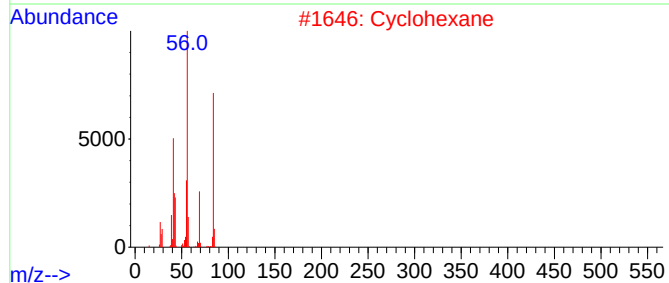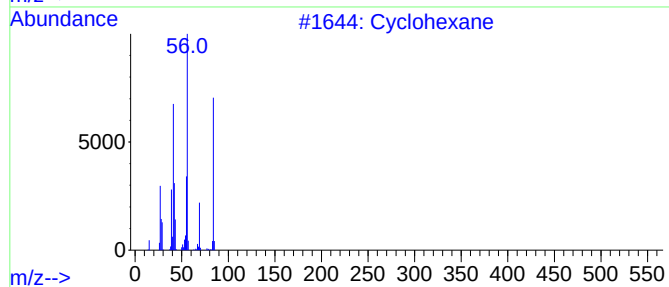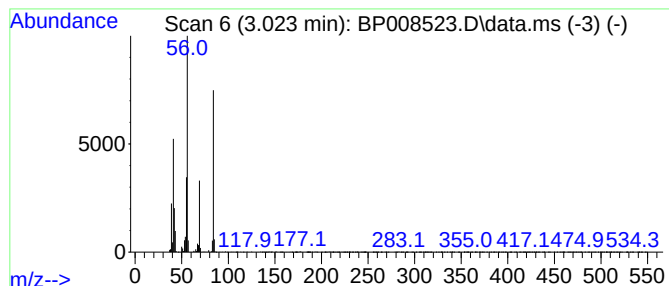

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
Data File : BP008523.D
Acq On : 23 Dec 2021 14:18
Operator : CG/JU
Sample : PB141621BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	3.023	3.7	ng/u1	425144	1	7.911	2284290	20.0