

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
 Data File : BP008531.D
 Acq On : 23 Dec 2021 18:50
 Operator : CG/JU
 Sample : PB141621BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK621

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
 Title : SVOA CALIBRATION

Signal : TIC: BP008531.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	15	rVB	309260	480393	3.86%	0.363%
2	3.099	16	19	23	rVB	67840	80494	0.65%	0.061%
3	3.352	58	62	67	rVB	153042	197088	1.58%	0.149%
4	3.758	126	131	147	rBV	1559270	2329409	18.72%	1.759%
5	4.099	186	189	195	rVB	32109	42084	0.34%	0.032%
6	7.058	685	692	704	rBV	2179963	3537050	28.43%	2.671%
7	7.234	715	722	736	rVB	1745071	2873156	23.09%	2.170%
8	7.434	749	756	766	rBV	2300866	3700991	29.74%	2.795%
9	7.905	829	836	845	rBV	1726645	2760968	22.19%	2.085%
10	8.605	947	955	968	rBV	2863416	4602744	36.99%	3.476%
11	9.058	1023	1032	1047	rBV	2090714	3473589	27.92%	2.623%
12	9.781	1144	1155	1170	rBV	1512542	2551393	20.51%	1.927%
13	10.322	1238	1247	1262	rBV	2882629	4799049	38.57%	3.624%
14	10.705	1304	1312	1322	rVB	2320530	4060297	32.63%	3.066%
15	10.834	1326	1334	1345	rBV	2373514	4045268	32.51%	3.055%
16	12.293	1576	1582	1589	rVB2	59401	94385	0.76%	0.071%
17	13.510	1784	1789	1792	rBV2	9573	15042	0.12%	0.011%
18	13.946	1856	1863	1869	rBV	5259279	7624685	61.28%	5.758%
19	14.228	1902	1911	1918	rBV	6199772	9607460	77.21%	7.255%
20	14.534	1955	1963	1970	rBV	4020809	5895103	47.38%	4.452%
21	14.710	1984	1993	2010	rBV	2091693	3031391	24.36%	2.289%
22	14.893	2021	2024	2030	rVB5	8544	13927	0.11%	0.011%
23	15.528	2124	2132	2139	rBV	7895291	11798898	94.83%	8.910%
24	15.634	2144	2150	2167	rVV	1432212	1972473	15.85%	1.489%
25	15.769	2168	2173	2180	rVB3	37554	64486	0.52%	0.049%
26	16.093	2224	2228	2232	rBV5	8354	12734	0.10%	0.010%
27	16.198	2240	2246	2253	rBV10	13025	26918	0.22%	0.020%
28	16.316	2261	2266	2274	rVB9	11503	20647	0.17%	0.016%
29	16.963	2372	2376	2381	rVB7	13597	21614	0.17%	0.016%
30	17.063	2388	2393	2401	rBV	21876	36319	0.29%	0.027%
31	17.281	2423	2430	2438	rBV	4643337	6647847	53.43%	5.020%
32	17.381	2440	2447	2459	rVV2	8597450	12305891	98.90%	9.293%
33	17.651	2488	2493	2497	rBV	12527	20488	0.16%	0.015%
34	19.186	2750	2754	2759	rBV2	101766	134055	1.08%	0.101%
35	19.257	2761	2766	2771	rBV	91056	132837	1.07%	0.100%
36	19.610	2820	2826	2835	rBV	9436768	12442547	100.00%	9.396%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
Data File : BP008531.D
Acq On : 23 Dec 2021 18:50
Operator : CG/JU
Sample : PB141621BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Title : SVOA CALIBRATION

37	21.357	3118	3123	3133	rVB	3981526	5344495	42.95%	4.036%
38	23.633	3502	3510	3521	rBV2	4925918	9970191	80.13%	7.529%
39	23.739	3524	3528	3530	rVV2	213559	363346	2.92%	0.274%
40	23.792	3530	3537	3549	rVB2	2489860	5293813	42.55%	3.998%


Sum of corrected areas: 132425565

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
Data File : BP008531.D
Acq On : 23 Dec 2021 18:50
Operator : CG/JU
Sample : PB141621BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

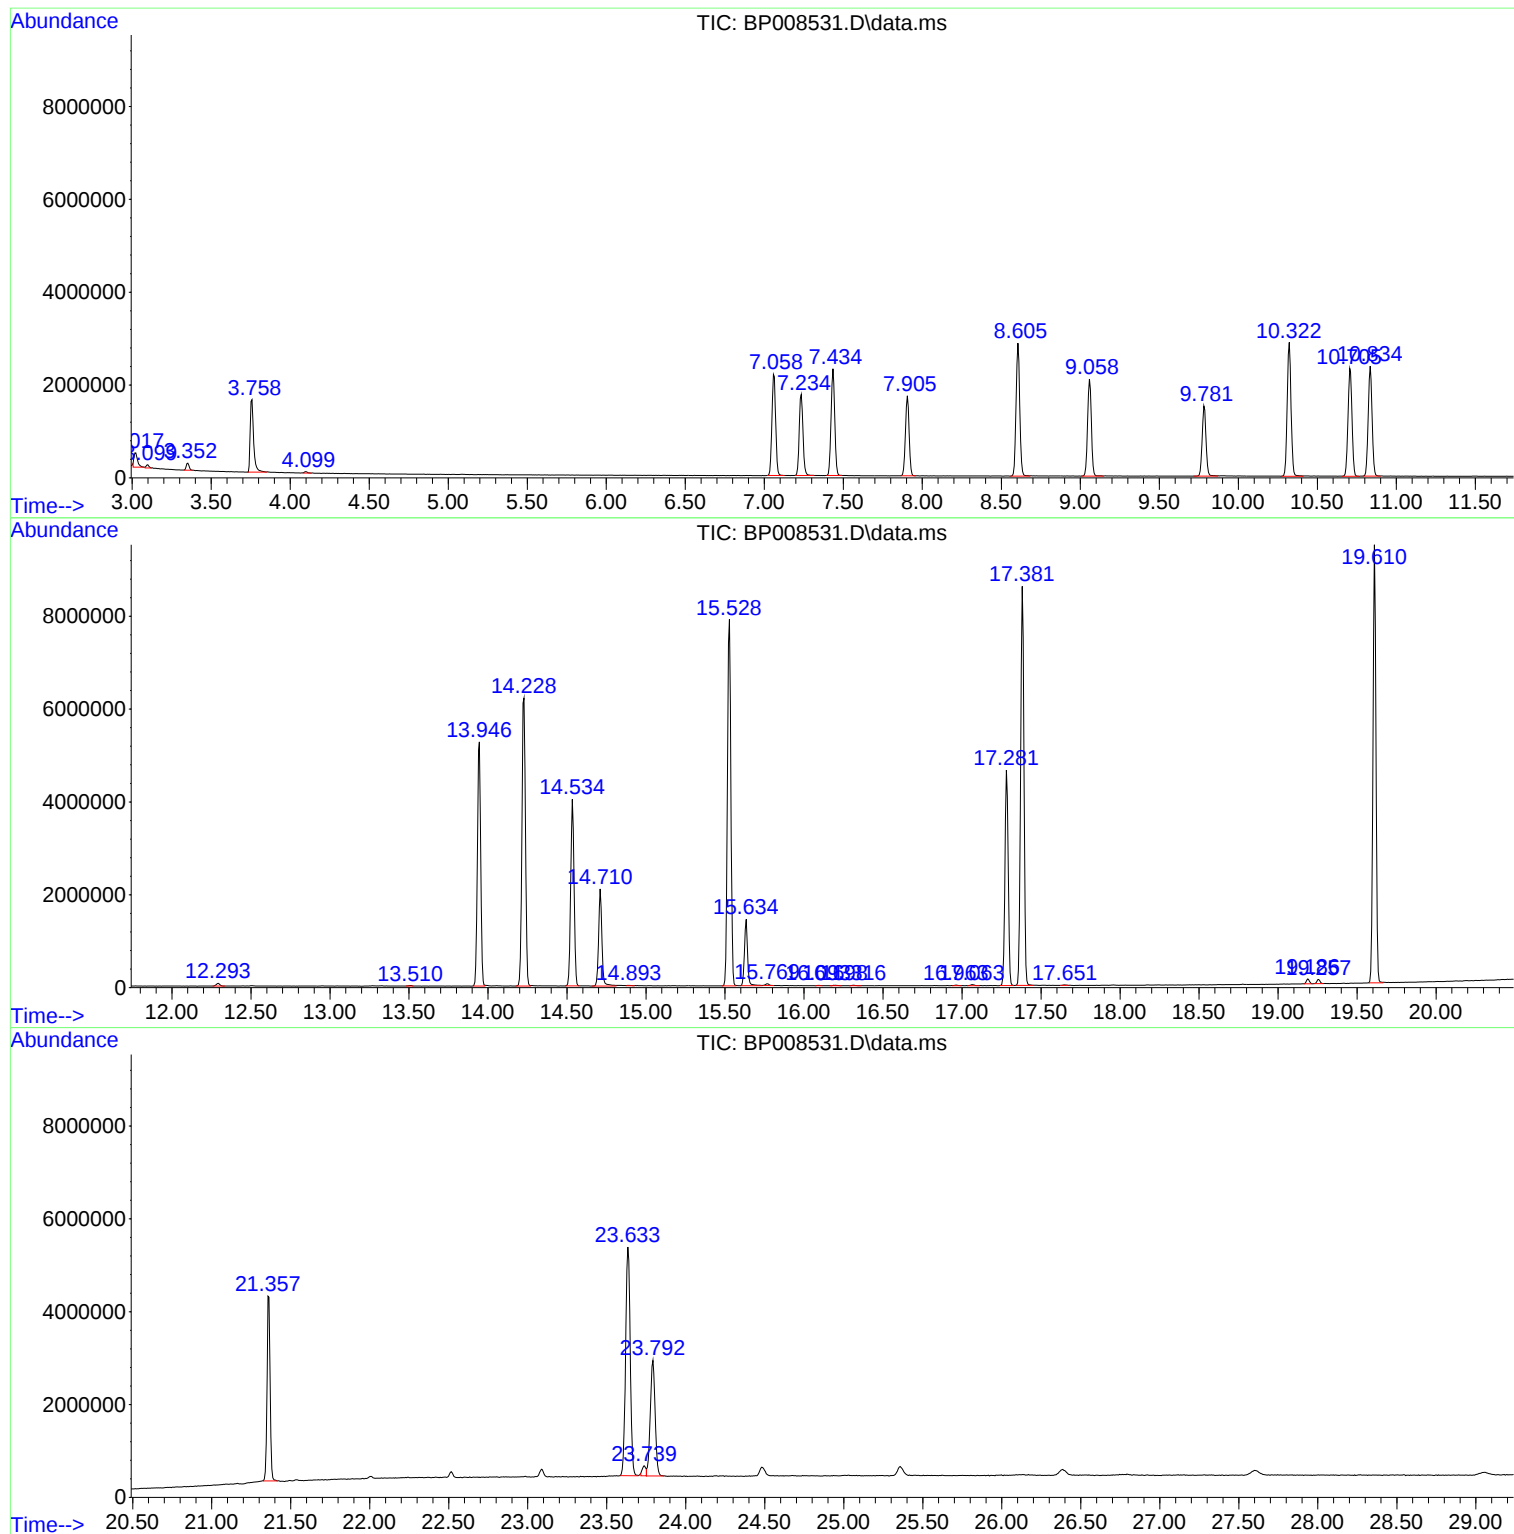

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
Data File : BP008531.D
Acq On : 23 Dec 2021 18:50
Operator : CG/JU
Sample : PB141621BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic3.017 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.017	3.48 ng/ul	480393	1,4-Dichlorobenzene-d4	7.905

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexane	84	C6H12	000110-82-7	91
2			Cyclohexane	84	C6H12	000110-82-7	91
3			Cyclohexane	84	C6H12	000110-82-7	91
4			Cyclohexane	84	C6H12	000110-82-7	91
5			1-Pentene, 2-methyl-	84	C6H12	000763-29-1	83

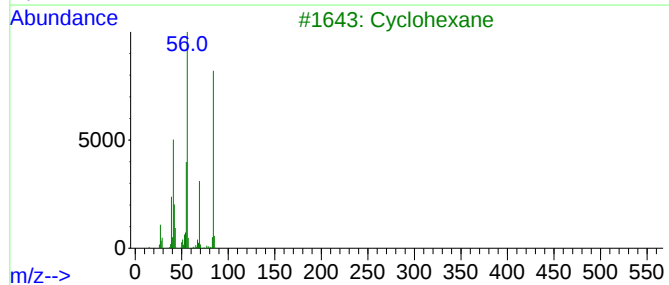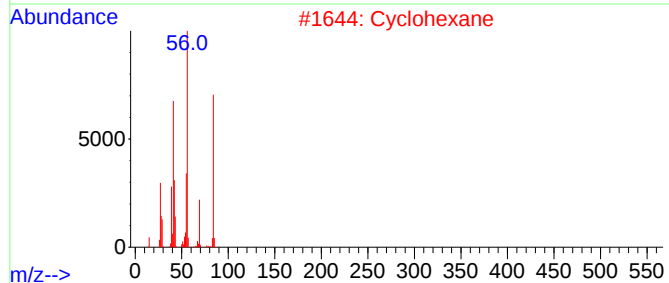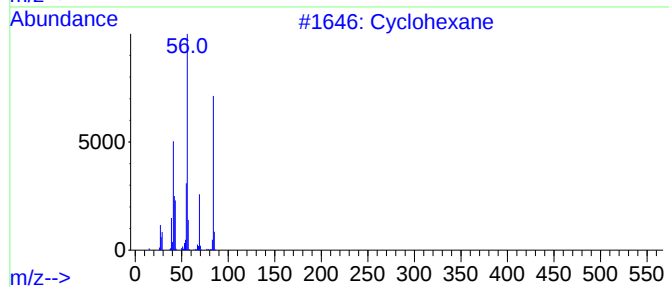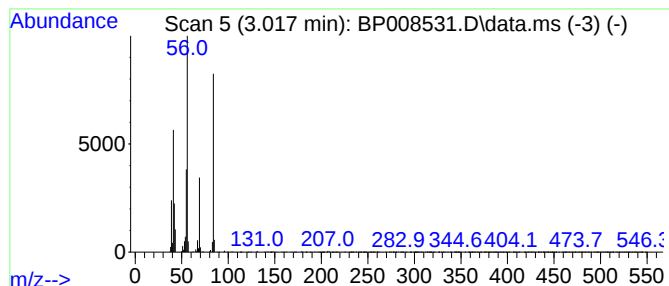

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
Data File : BP008531.D
Acq On : 23 Dec 2021 18:50
Operator : CG/JU
Sample : PB141621BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	3.017	3.5	ng/u1	480393	1	7.905	2760970	20.0