

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
 Data File : BP008533.D
 Acq On : 23 Dec 2021 19:57
 Operator : CG/JU
 Sample : PB141581BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK581

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
 Title : SVOA CALIBRATION

Signal : TIC: BP008533.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.023	3	6	15	rVB	341632	518119	5.16%	0.469%
2	3.099	16	19	26	rVB	72901	106311	1.06%	0.096%
3	3.352	58	62	69	rVB	149371	204028	2.03%	0.185%
4	3.758	127	131	152	rVB	1389778	2078979	20.70%	1.882%
5	4.099	186	189	193	rVB2	35863	44292	0.44%	0.040%
6	7.058	684	692	702	rBV	1996820	3219289	32.06%	2.914%
7	7.234	715	722	732	rBV	1617322	2617058	26.06%	2.369%
8	7.434	749	756	766	rBV	2146000	3341146	33.27%	3.024%
9	7.905	828	836	845	rVB	1448837	2303863	22.94%	2.085%
10	8.605	948	955	971	rBV	2564782	4101019	40.84%	3.712%
11	9.058	1025	1032	1040	rBV	1857581	3054203	30.41%	2.764%
12	9.781	1145	1155	1168	rBV	1300093	2175056	21.66%	1.969%
13	10.322	1239	1247	1264	rBV	2434422	4216360	41.99%	3.816%
14	10.705	1304	1312	1320	rBV	1908609	3284736	32.71%	2.973%
15	10.834	1325	1334	1346	rBV	2021190	3331974	33.18%	3.016%
16	12.293	1575	1582	1589	rBV2	51686	85974	0.86%	0.078%
17	13.510	1784	1789	1793	rBV4	9127	16721	0.17%	0.015%
18	13.946	1855	1863	1869	rBV	4307756	6292098	62.66%	5.695%
19	14.228	1900	1911	1919	rBV	5425207	8163247	81.29%	7.388%
20	14.534	1956	1963	1971	rBV	3096031	4541714	45.23%	4.111%
21	14.710	1986	1993	2010	rBV	1654163	2392444	23.82%	2.165%
22	15.528	2124	2132	2141	rBV	6360577	9724860	96.84%	8.802%
23	15.634	2143	2150	2167	rVV	1037987	1488162	14.82%	1.347%
24	15.769	2168	2173	2178	rVB2	30460	53076	0.53%	0.048%
25	16.093	2222	2228	2233	rBV7	5654	10313	0.10%	0.009%
26	16.198	2241	2246	2252	rBV8	7828	15979	0.16%	0.014%
27	16.310	2261	2265	2270	rBV7	10350	16053	0.16%	0.015%
28	16.963	2372	2376	2382	rVB7	11357	17381	0.17%	0.016%
29	17.063	2390	2393	2400	rVB3	15591	22239	0.22%	0.020%
30	17.281	2422	2430	2438	rBV	3284366	4783670	47.64%	4.330%
31	17.381	2440	2447	2460	rVV	7044903	9835708	97.95%	8.902%
32	17.645	2488	2492	2496	rBV2	9445	17183	0.17%	0.016%
33	17.957	2542	2545	2548	rVB5	8350	10870	0.11%	0.010%
34	19.186	2750	2754	2760	rVB	78736	110098	1.10%	0.100%
35	19.257	2761	2766	2771	rVV	68851	96004	0.96%	0.087%
36	19.610	2820	2826	2839	rBV	7799749	10041787	100.00%	9.089%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
Data File : BP008533.D
Acq On : 23 Dec 2021 19:57
Operator : CG/JU
Sample : PB141581BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK581

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Title : SVOA CALIBRATION

37	21.363	3118	3124	3133	rVB	3136107	4161248	41.44%	3.766%
38	23.633	3502	3510	3522	rBV2	4753280	9538636	94.99%	8.633%
39	23.792	3530	3537	3546	rVB2	2157319	4455331	44.37%	4.032%




Sum of corrected areas: 110487229

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
Data File : BP008533.D
Acq On : 23 Dec 2021 19:57
Operator : CG/JU
Sample : PB141581BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK581

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

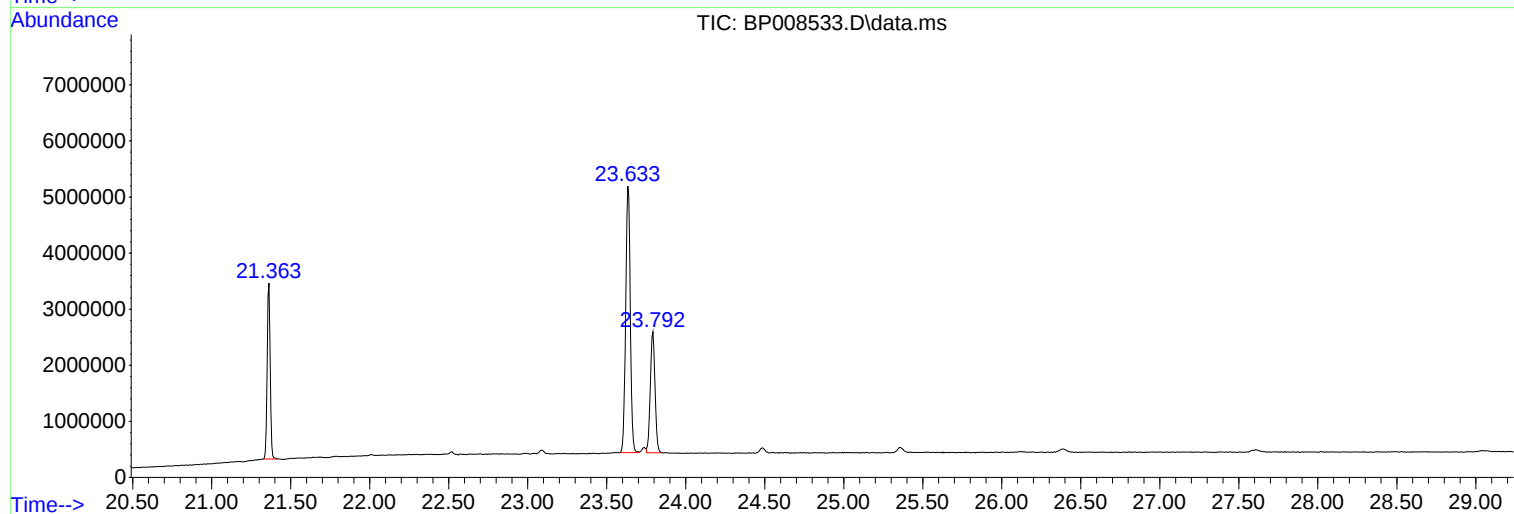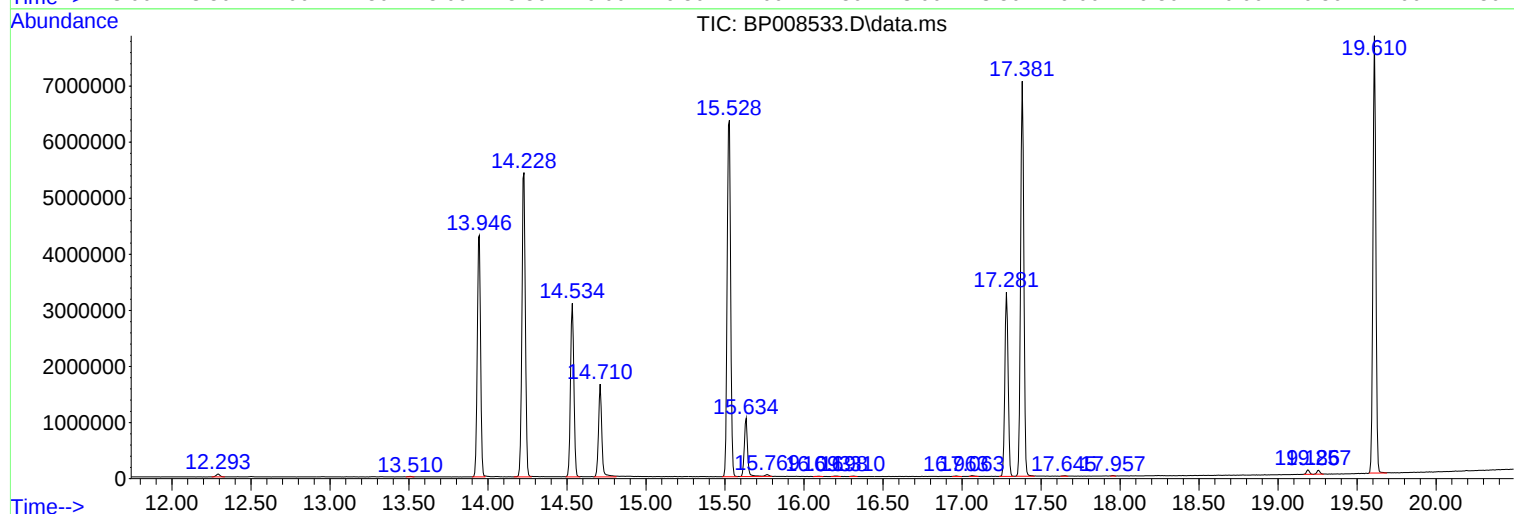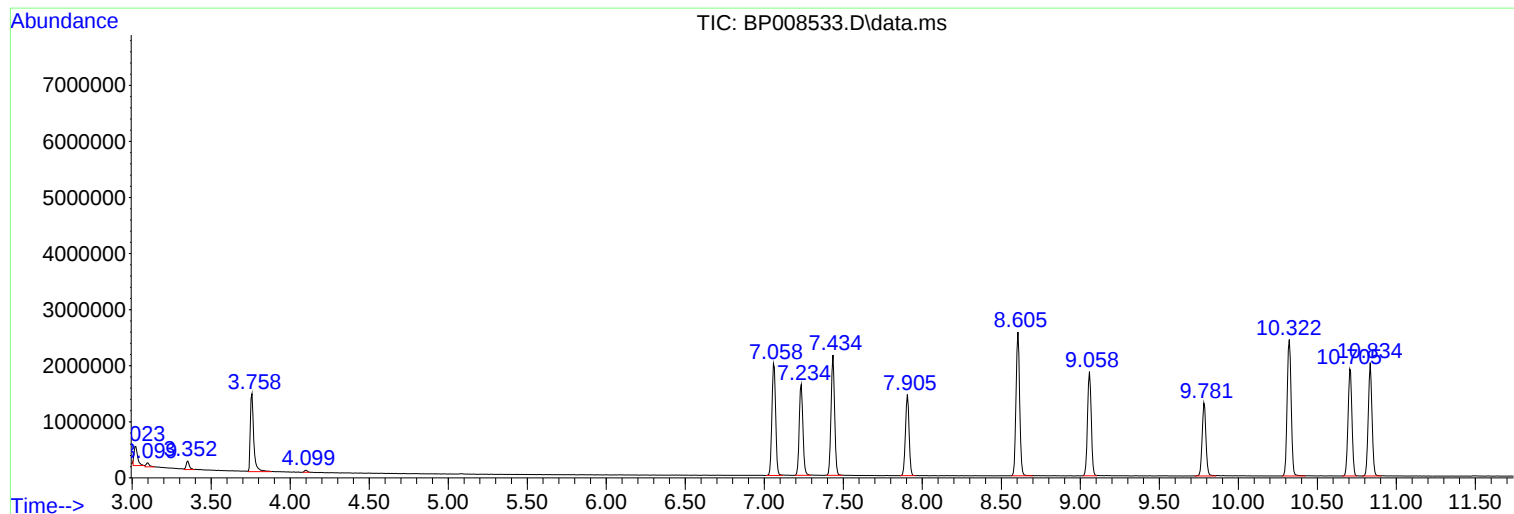

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
Data File : BP008533.D
Acq On : 23 Dec 2021 19:57
Operator : CG/JU
Sample : PB141581BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK581










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic3.023 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.023	4.50 ng/ul	518119	1,4-Dichlorobenzene-d4	7.905

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexane	84	C6H12	000110-82-7	91
2			Cyclohexane	84	C6H12	000110-82-7	91
3			Cyclohexane	84	C6H12	000110-82-7	90
4			Cyclohexane	84	C6H12	000110-82-7	83
5			Cyclopentane, methyl-	84	C6H12	000096-37-7	83

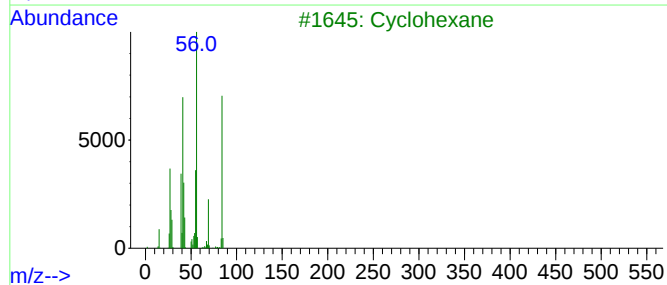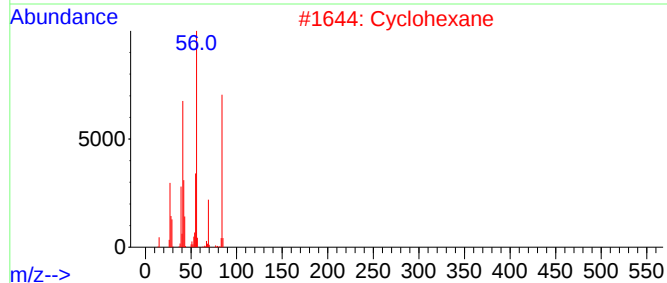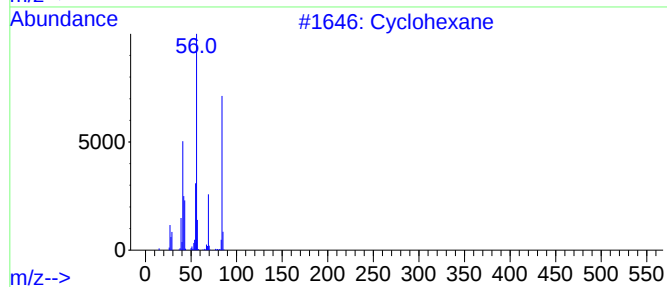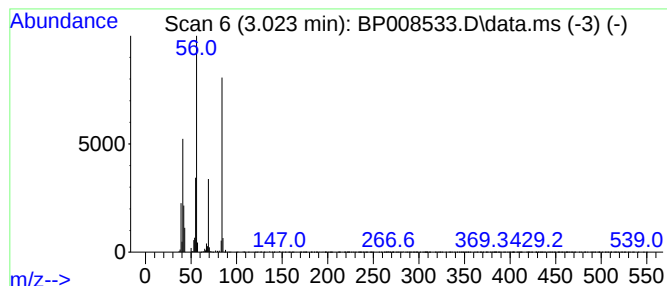

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122321\
Data File : BP008533.D
Acq On : 23 Dec 2021 19:57
Operator : CG/JU
Sample : PB141581BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK581

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	3.023	4.5	ng/u1	518119	1	7.905	2303860	20.0