

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122721\
 Data File : BP008555.D
 Acq On : 27 Dec 2021 14:48
 Operator : CG/JU
 Sample : M5201-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P078-TW001-01

Quant Time: Dec 28 01:28:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 23 14:48:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	332076	20.000	ng/ul	0.00
20) Naphthalene-d8	10.704	136	1392698	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.534	164	1009812	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	2266309	20.000	ng/ul	0.00
79) Chrysene-d12	21.363	240	2286852	20.000	ng/ul	0.00
88) Perylene-d12	23.792	264	2159384	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	62408	8.471	ng/uL	0.00
4) Pyridine-d5	3.758	84	272053	13.195	ng/ul	0.00
7) Phenol-d5	7.058	99	272259	10.277	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	736880	48.973	ng/ul	0.00
11) 2-Chlorophenol-d4	7.434	132	816438	38.742	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	518172	24.383	ng/ul	0.00
21) Nitrobenzene-d5	9.058	128	525756	53.350	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	482191	53.363	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	1002376	45.191	ng/ul	0.00
31) 4-Chloroaniline-d4	10.834	131	1414685	46.204	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	4186842	56.116	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	4963585	53.204	ng/ul	0.00
54) 4-Nitrophenol-d4	14.710	143	109069	9.222	ng/ul	0.00
60) Fluorene-d10	15.528	176	3719057	57.412	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200	453204	45.428	ng/ul	0.00
73) Anthracene-d10	17.381	188	6620460	61.646	ng/ul	0.00
81) Pyrene-d10	19.610	212	7798930	56.914	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.639	264	7155944	64.387	ng/ul	0.00
Target Compounds						
78) Di-n-butylphthalate	18.245	149	176993	1.421	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122721\
Data File : BP008555.D
Acq On : 27 Dec 2021 14:48
Operator : CG/JU
Sample : M5201-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P078-TW001-01

Quant Time: Dec 28 01:28:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 23 14:48:11 2021
Response via : Initial Calibration

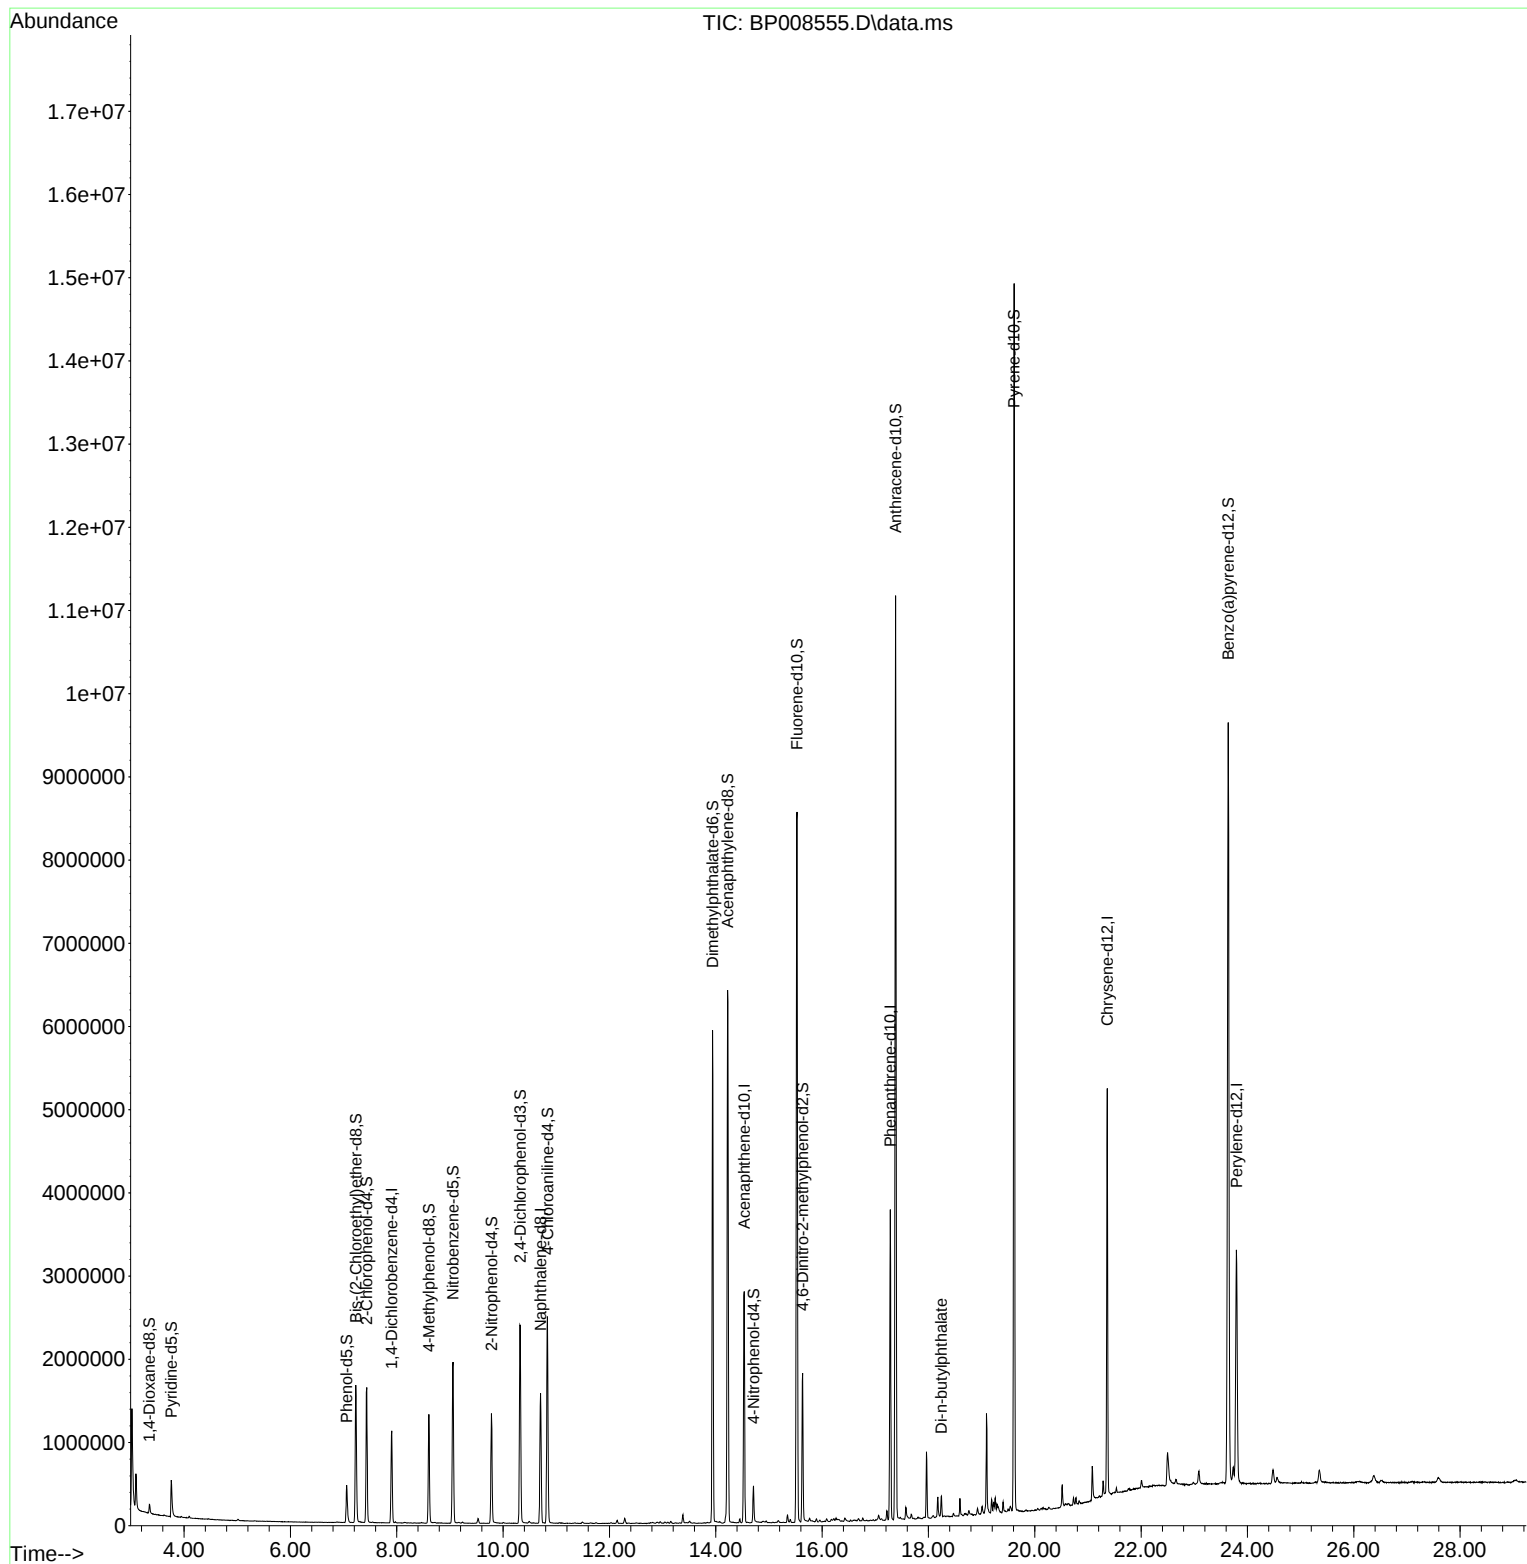

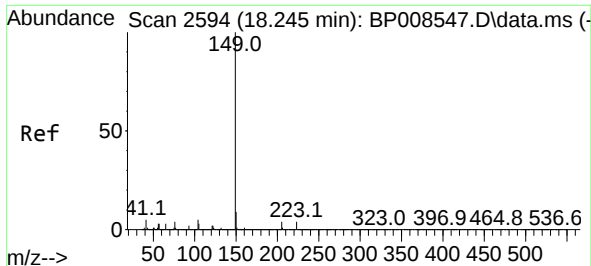

#78
 Di-n-butylphthalate
 Concen: 1.421 ng/ul
 RT: 18.245 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP008555.D
 Acq: 27 Dec 2021 14:48

Instrument :
 BNA_P
 ClientSampleId :
 P078-TW001-01

Tgt Ion:149 Resp: 176993
 Ion Ratio Lower Upper
 149 100
 150 8.5 7.4 11.2
 104 4.7 3.6 5.4

