

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122721\
 Data File : BP008573.D
 Acq On : 28 Dec 2021 10:12
 Operator : CG/JU
 Sample : M5201-13
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P078-TW001-01

Quant Time: Dec 28 12:16:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 23 14:48:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	421963	20.000	ng/ul	0.00
20) Naphthalene-d8	10.699	136	1793731	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.528	164	1300587	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	2915166	20.000	ng/ul	0.00
79) Chrysene-d12	21.363	240	2865976	20.000	ng/ul	0.00
88) Perylene-d12	23.792	264	2717353	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	60322	6.444	ng/uL	0.00
4) Pyridine-d5	3.758	84	258683	9.874	ng/ul	0.00
7) Phenol-d5	7.058	99	266976	7.931	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	720551	37.687	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	805967	30.098	ng/ul	0.00
15) 4-Methylphenol-d8	8.599	113	519866	19.251	ng/ul	-0.01
21) Nitrobenzene-d5	9.052	128	519595	40.937	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	479761	41.224	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.316	165	1001156	35.045	ng/ul	0.00
31) 4-Chloroaniline-d4	10.828	131	1393926	35.348	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	4123153	42.907	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	4920904	40.954	ng/ul	0.00
54) 4-Nitrophenol-d4	14.704	143	106592	6.998	ng/ul	-0.01
60) Fluorene-d10	15.522	176	3687645	44.200	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200	447480	34.871	ng/ul	0.00
73) Anthracene-d10	17.381	188	6508095	47.111	ng/ul	0.00
81) Pyrene-d10	19.610	212	7682437	44.735	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.633	264	6866998	49.100	ng/ul	0.00


Target Compounds					Qvalue
78) Di-n-butylphthalate	18.239	149	177758	1.110 ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122721\
Data File : BP008573.D
Acq On : 28 Dec 2021 10:12
Operator : CG/JU
Sample : M5201-13
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P078-TW001-01

Quant Time: Dec 28 12:16:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 23 14:48:11 2021
Response via : Initial Calibration

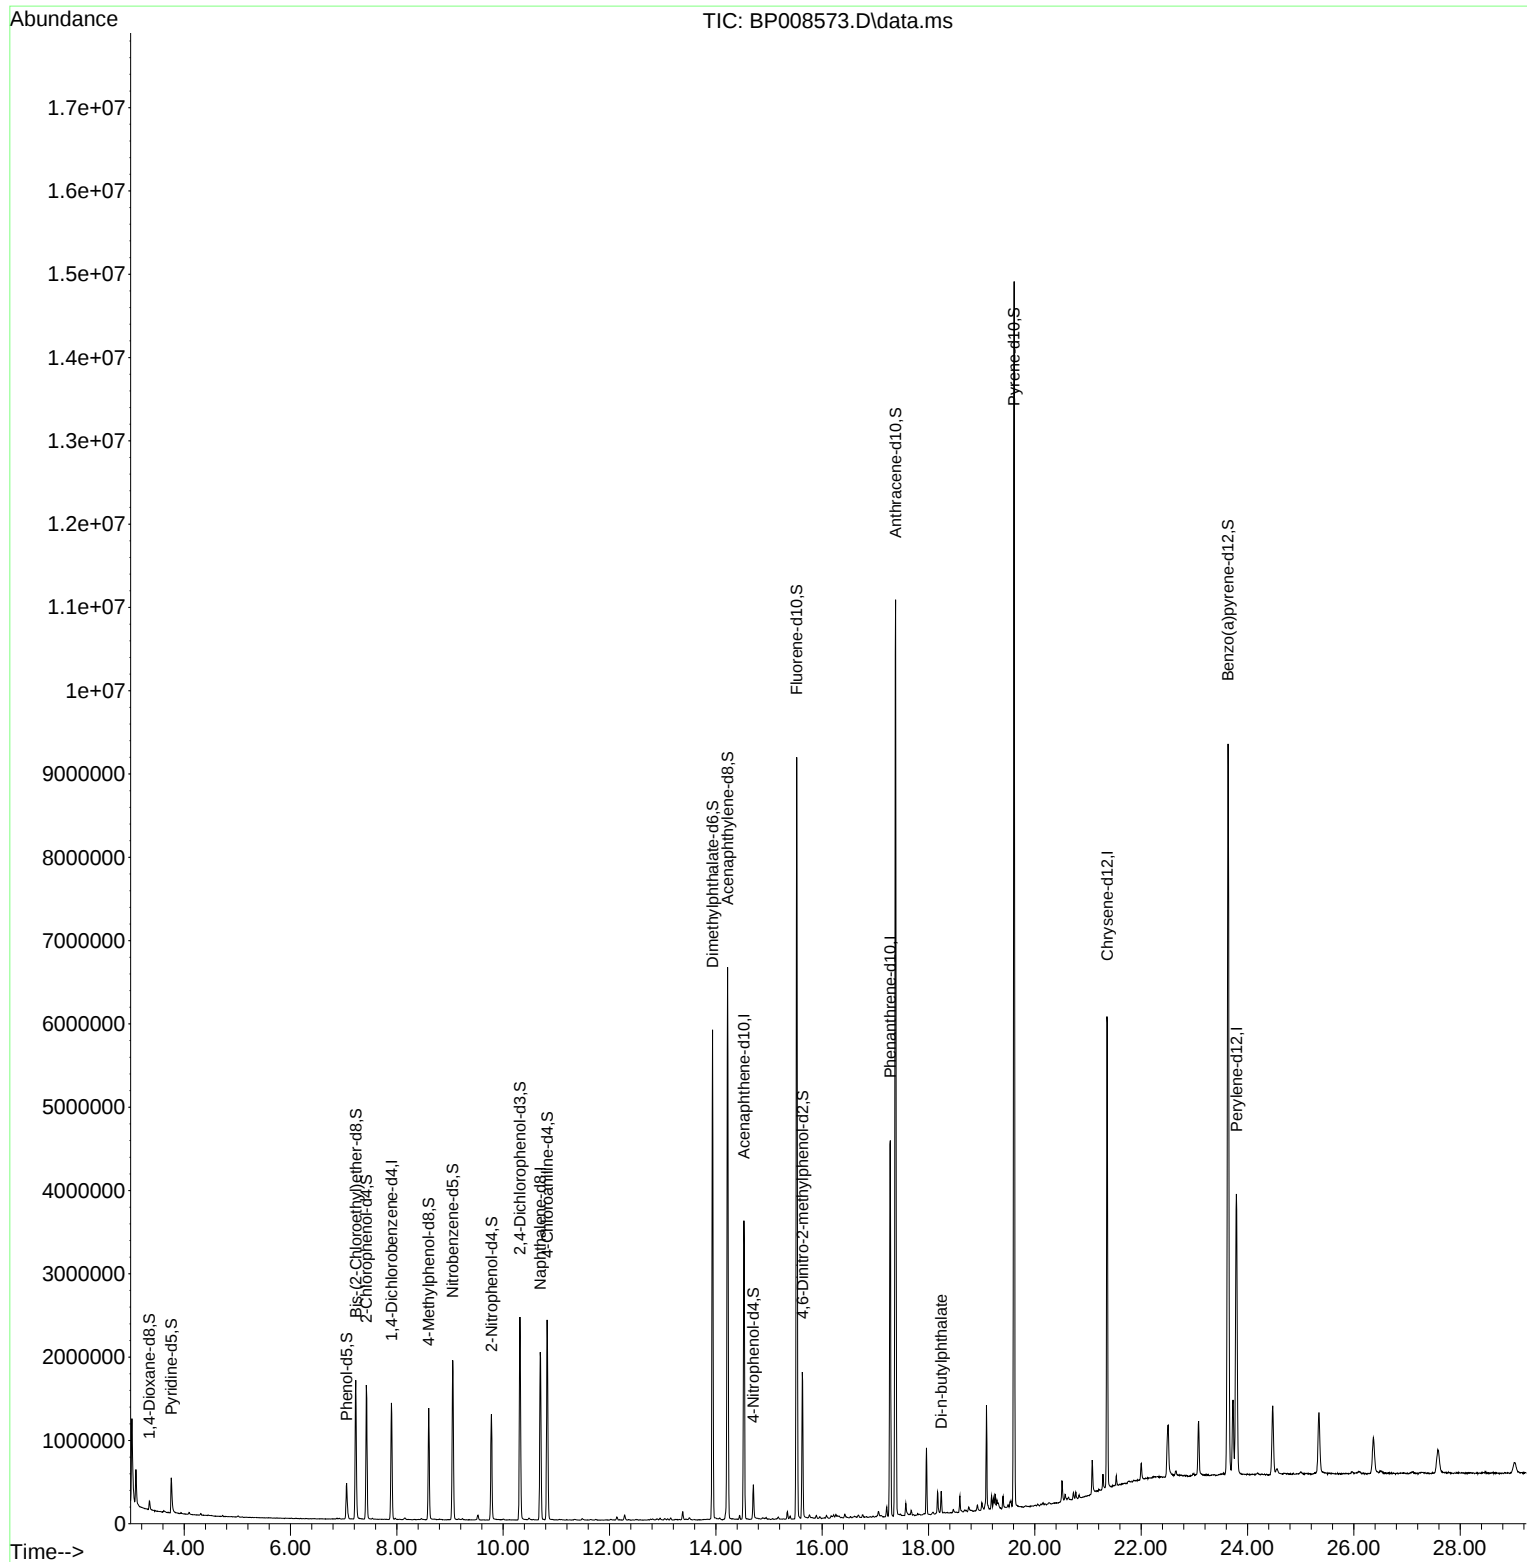

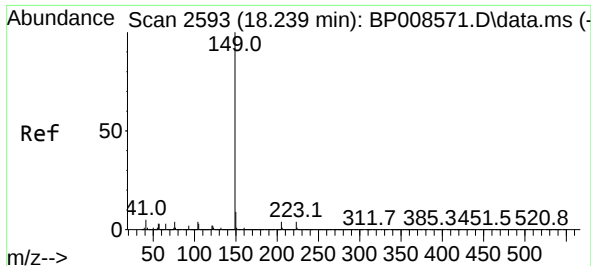

#78
 Di-n-butylphthalate
 Concen: 1.110 ng/ul
 RT: 18.239 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP008573.D
 Acq: 28 Dec 2021 10:12

Instrument :
 BNA_P
 ClientSampleId :
 P078-TW001-01

Tgt Ion:149 Resp: 177758
 Ion Ratio Lower Upper
 149 100
 150 9.2 7.4 11.2
 104 4.7 3.6 5.4

