

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122721\
 Data File : BP008565.D
 Acq On : 27 Dec 2021 21:01
 Operator : CG/JU
 Sample : PB141621BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK621

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
 Title : SVOA CALIBRATION

Signal : TIC: BP008565.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.016	3	5	15	rVB	254281	390442	2.27%	0.247%
2	3.346	58	61	69	rVB	129694	189750	1.10%	0.120%
3	3.757	127	131	151	rBV	1307415	2075144	12.08%	1.312%
4	7.057	685	692	704	rBV	2094480	3283480	19.11%	2.076%
5	7.228	714	721	731	rBV	1746374	2802521	16.31%	1.772%
6	7.428	748	755	768	rBV	2087567	3447652	20.07%	2.179%
7	7.898	828	835	849	rVB	1606269	2656142	15.46%	1.679%
8	8.604	947	955	967	rBV	2647135	4341089	25.27%	2.744%
9	9.051	1024	1031	1043	rBV	1943116	3290960	19.16%	2.080%
10	9.781	1144	1155	1164	rBV	1434134	2350566	13.68%	1.486%
11	10.316	1238	1246	1260	rBV	2719859	4604713	26.80%	2.911%
12	10.704	1304	1312	1320	rVB	2405299	4057765	23.62%	2.565%
13	10.833	1325	1334	1347	rBV	2486640	4247799	24.72%	2.685%
14	12.286	1573	1581	1588	rBV2	57448	95026	0.55%	0.060%
15	13.939	1854	1862	1876	rBV	5972678	8308826	48.36%	5.252%
16	14.222	1902	1910	1928	rBV	6624606	9820817	57.16%	6.208%
17	14.527	1954	1962	1970	rBV	4167835	6277811	36.54%	3.969%
18	14.710	1985	1993	2009	rBV	2377903	3425040	19.94%	2.165%
19	15.521	2124	2131	2143	rBV	9149780	12672268	73.76%	8.011%
20	15.633	2143	2150	2165	rVV	1709846	2416437	14.07%	1.528%
21	15.763	2167	2172	2178	rVB	41552	67625	0.39%	0.043%
22	16.192	2242	2245	2254	rVB10	11959	24233	0.14%	0.015%
23	16.310	2260	2265	2269	rBV6	11644	17895	0.10%	0.011%
24	16.963	2368	2376	2380	rBV7	14450	25332	0.15%	0.016%
25	17.063	2388	2393	2400	rBV	24176	42246	0.25%	0.027%
26	17.280	2423	2430	2440	rBV	5604845	7878342	45.86%	4.980%
27	17.380	2440	2447	2467	rVB	9895801	14421264	83.94%	9.116%
28	17.651	2489	2493	2500	rVB3	13050	20044	0.12%	0.013%
29	18.168	2578	2581	2587	rBV8	11218	20263	0.12%	0.013%
30	19.186	2749	2754	2760	rBV	126026	180703	1.05%	0.114%
31	19.251	2761	2765	2772	rVV	112195	162017	0.94%	0.102%
32	19.609	2820	2826	2838	rBV	13071158	17180385	100.00%	10.861%
33	21.362	3118	3124	3132	rBV	6765788	8844758	51.48%	5.591%
34	22.509	3316	3319	3328	rVB2	227765	341315	1.99%	0.216%
35	23.080	3413	3416	3424	rVB	300304	472615	2.75%	0.299%
36	23.633	3502	3510	3520	rBV2	8397907	16593779	96.59%	10.490%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122721\
Data File : BP008565.D
Acq On : 27 Dec 2021 21:01
Operator : CG/JU
Sample : PB141621BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Title : SVOA CALIBRATION

37	23.727	3522	3526	3530	rVV	492231	865734	5.04%	0.547%
38	23.792	3530	3537	3550	rVB2	4206166	8824510	51.36%	5.578%
39	24.474	3649	3653	3661	rVB	362424	716140	4.17%	0.453%
40	25.350	3797	3802	3812	rVB	316055	736251	4.29%	0.465%




Sum of corrected areas: 158189699

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122721\
Data File : BP008565.D
Acq On : 27 Dec 2021 21:01
Operator : CG/JU
Sample : PB141621BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

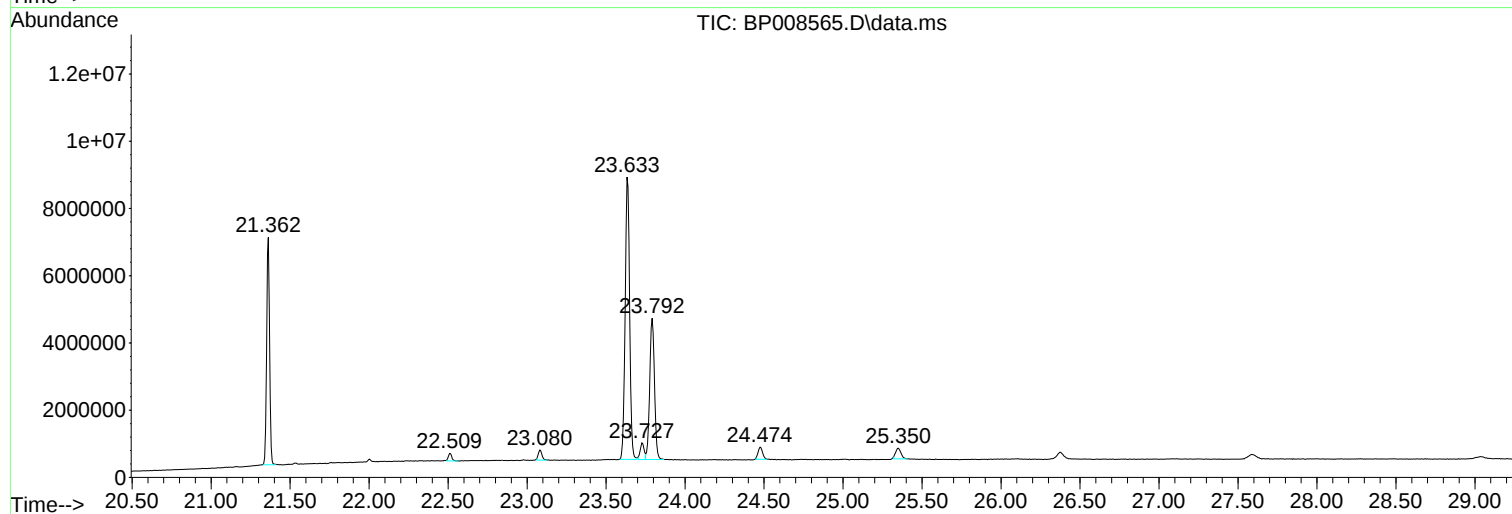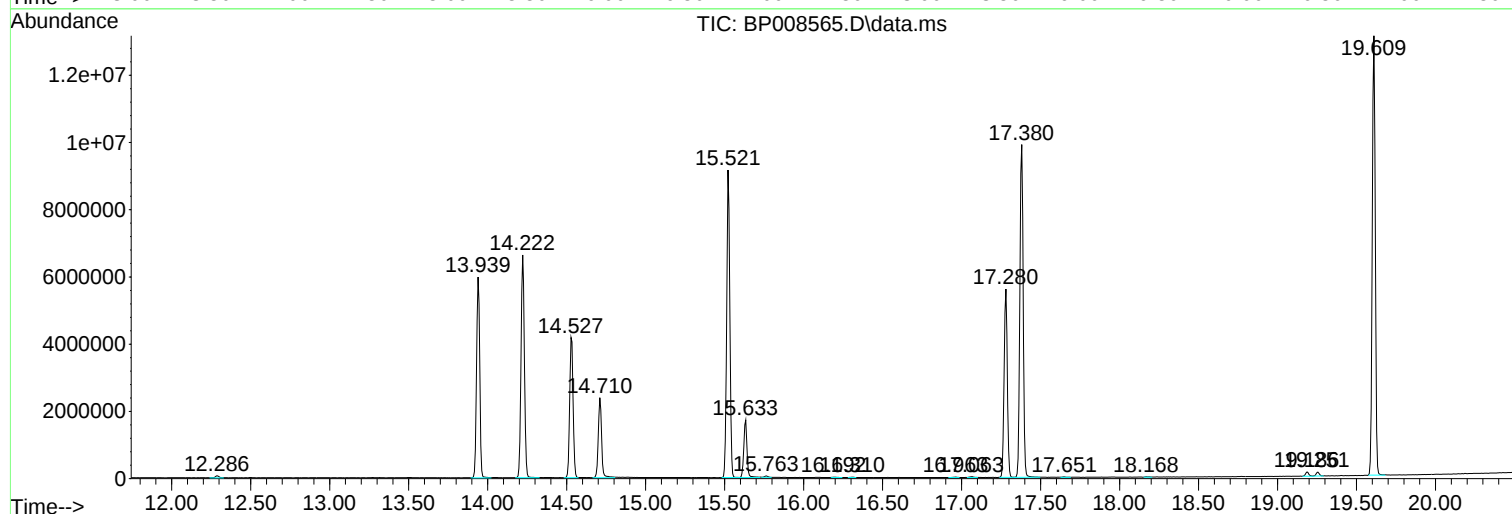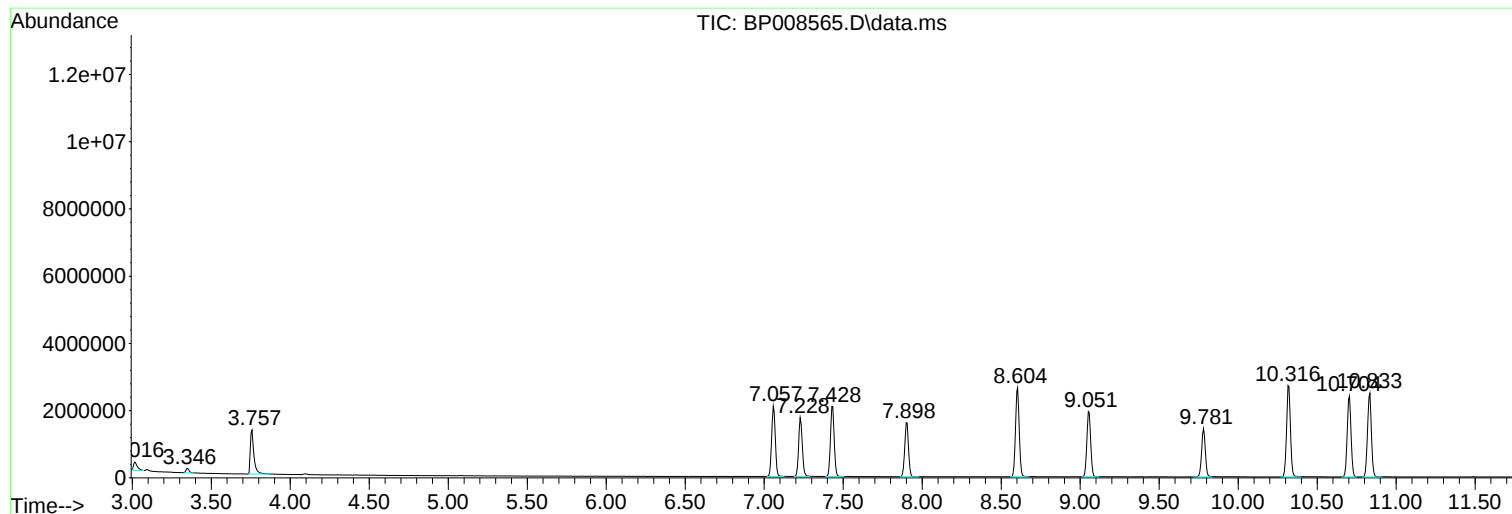

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122721\
Data File : BP008565.D
Acq On : 27 Dec 2021 21:01
Operator : CG/JU
Sample : PB141621BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic3.016 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.016	2.94 ng/ul	390442	1,4-Dichlorobenzene-d4	7.904

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexane	84	C6H12	000110-82-7	91
2			Cyclohexane	84	C6H12	000110-82-7	91
3			Cyclohexane	84	C6H12	000110-82-7	91
4			Cyclohexane	84	C6H12	000110-82-7	91
5			Cyclopentane, methyl-	84	C6H12	000096-37-7	83

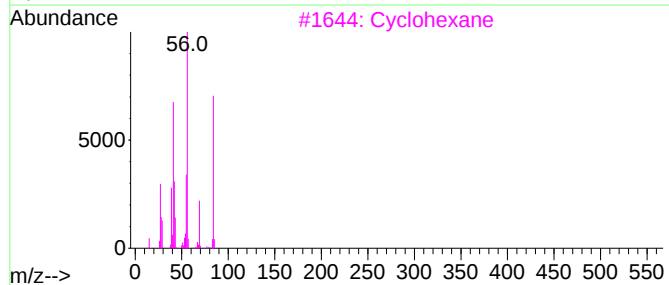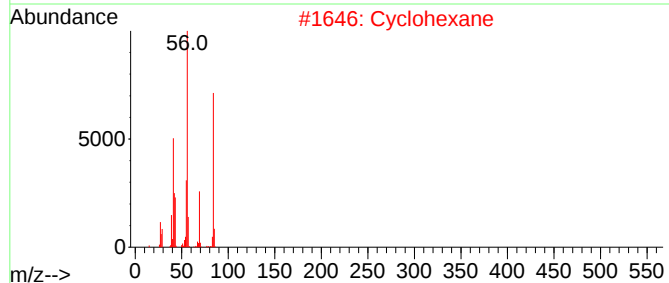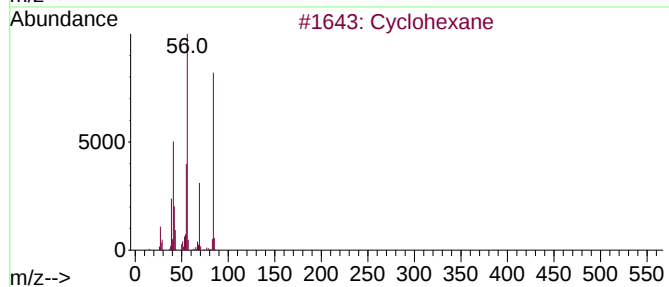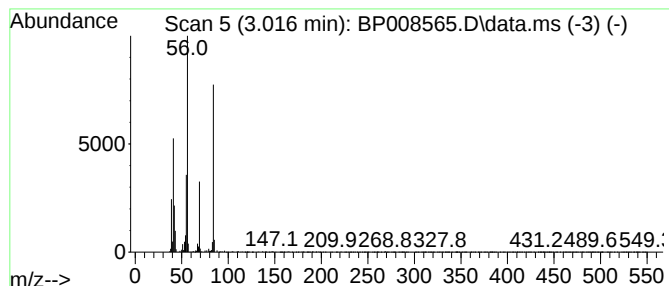

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122721\
Data File : BP008565.D
Acq On : 27 Dec 2021 21:01
Operator : CG/JU
Sample : PB141621BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	3.016	2.9	ng/ul	390442	1	7.904	2656140	20.0