

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122721\
 Data File : BP008577.D
 Acq On : 28 Dec 2021 12:28
 Operator : CG/JU
 Sample : PB141663BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK663

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
 Title : SVOA CALIBRATION

Signal : TIC: BP008577.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	16	rVB	385396	540491	5.14%	0.503%
2	3.346	58	61	71	rVB	137782	189513	1.80%	0.176%
3	3.758	127	131	145	rBV	1515192	2287322	21.77%	2.128%
4	4.093	185	188	195	rVB2	34423	50183	0.48%	0.047%
5	7.058	685	692	704	rBV	1882820	2930356	27.89%	2.726%
6	7.228	713	721	733	rBV	1507785	2410644	22.95%	2.243%
7	7.428	748	755	768	rBV	1928642	3064143	29.17%	2.851%
8	7.899	828	835	844	rVB	1580704	2593541	24.69%	2.413%
9	8.599	947	954	969	rBV	2263421	3672795	34.96%	3.417%
10	9.052	1024	1031	1042	rBV	1663552	2716793	25.86%	2.528%
11	9.775	1147	1154	1163	rBV	1083571	1836652	17.48%	1.709%
12	10.316	1238	1246	1262	rBV	2263222	3729804	35.50%	3.470%
13	10.699	1303	1311	1321	rVB	2068771	3567185	33.96%	3.319%
14	10.828	1325	1333	1347	rBV	2213568	3818406	36.35%	3.553%
15	12.287	1575	1581	1592	rVB2	43630	78864	0.75%	0.073%
16	12.499	1612	1617	1620	rBV7	6236	11867	0.11%	0.011%
17	13.499	1784	1787	1794	rVB3	7611	11889	0.11%	0.011%
18	13.940	1855	1862	1872	rBV	3649306	5141113	48.94%	4.783%
19	14.222	1900	1910	1928	rBV	4643958	6842319	65.13%	6.366%
20	14.528	1955	1962	1969	rBV	3119995	4675447	44.50%	4.350%
21	14.704	1984	1992	2006	rBV	1293997	1942044	18.49%	1.807%
22	15.522	2123	2131	2142	rBV	5749971	8263273	78.66%	7.688%
23	15.628	2142	2149	2166	rVV	891888	1255782	11.95%	1.168%
24	15.763	2166	2172	2177	rVB4	26458	50378	0.48%	0.047%
25	16.192	2238	2245	2248	rBV9	9444	17760	0.17%	0.017%
26	16.310	2260	2265	2271	rVB8	6951	11017	0.10%	0.010%
27	16.957	2371	2375	2379	rBV5	8600	11462	0.11%	0.011%
28	17.057	2384	2392	2399	rBV3	18064	39450	0.38%	0.037%
29	17.275	2423	2429	2437	rBV	3525832	5086770	48.42%	4.733%
30	17.375	2439	2446	2466	rVV2	5891881	8572467	81.60%	7.976%
31	17.651	2488	2493	2498	rBV6	7778	14909	0.14%	0.014%
32	19.186	2749	2754	2759	rBV	75043	100871	0.96%	0.094%
33	19.251	2761	2765	2772	rVV	66734	97197	0.93%	0.090%
34	19.604	2819	2825	2836	rBV	7060416	9780715	93.10%	9.100%
35	21.357	3118	3123	3131	rBV	4295120	5421054	51.60%	5.044%
36	23.633	3502	3510	3520	rBV2	5221278	10505462	100.00%	9.775%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122721\
Data File : BP008577.D
Acq On : 28 Dec 2021 12:28
Operator : CG/JU
Sample : PB141663BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK663

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Title : SVOA CALIBRATION

37 23.786 3529 3536 3552 rVB2 2901104 6137048 58.42% 5.710%




Sum of corrected areas: 107476986

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122721\
Data File : BP008577.D
Acq On : 28 Dec 2021 12:28
Operator : CG/JU
Sample : PB141663BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK663

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

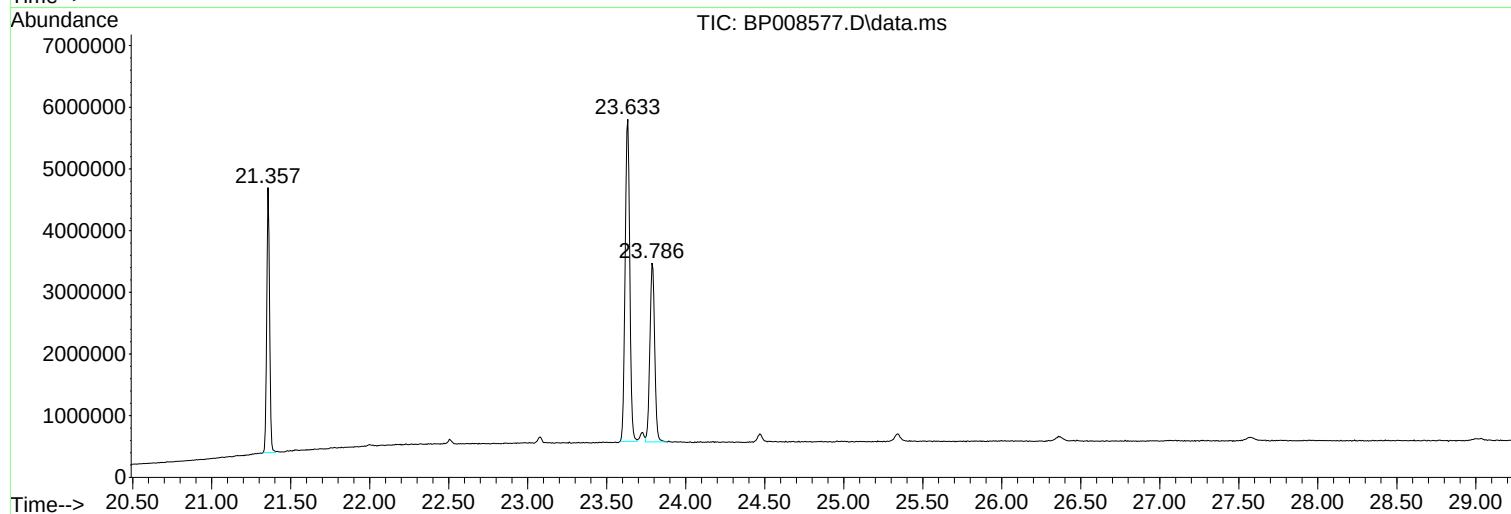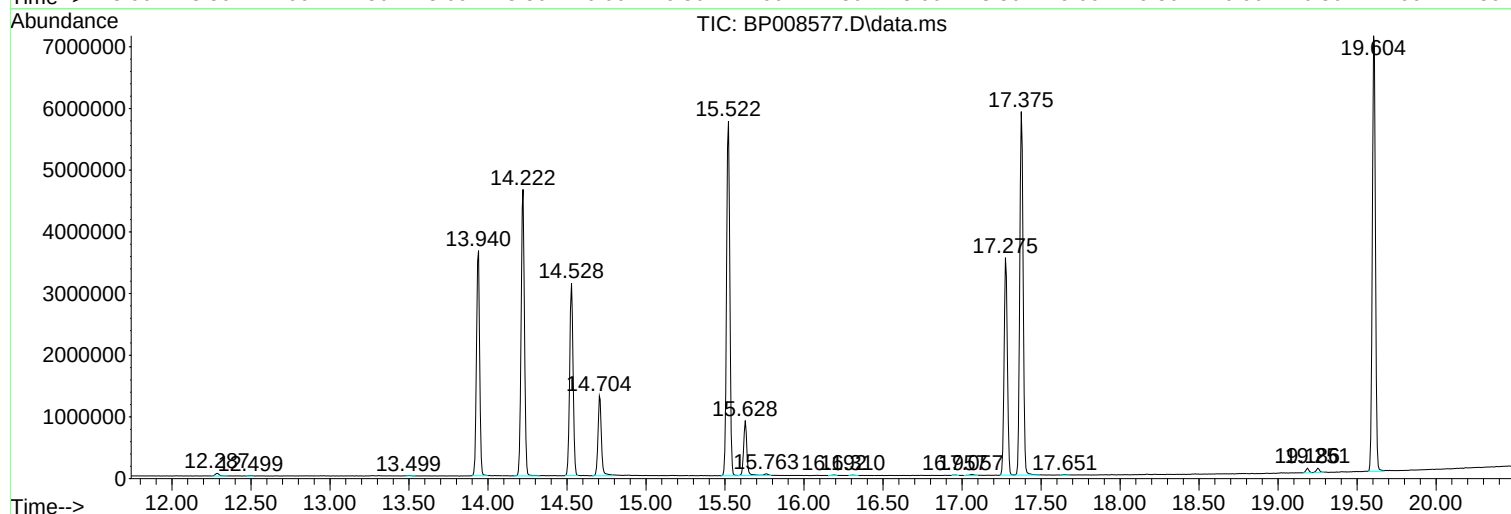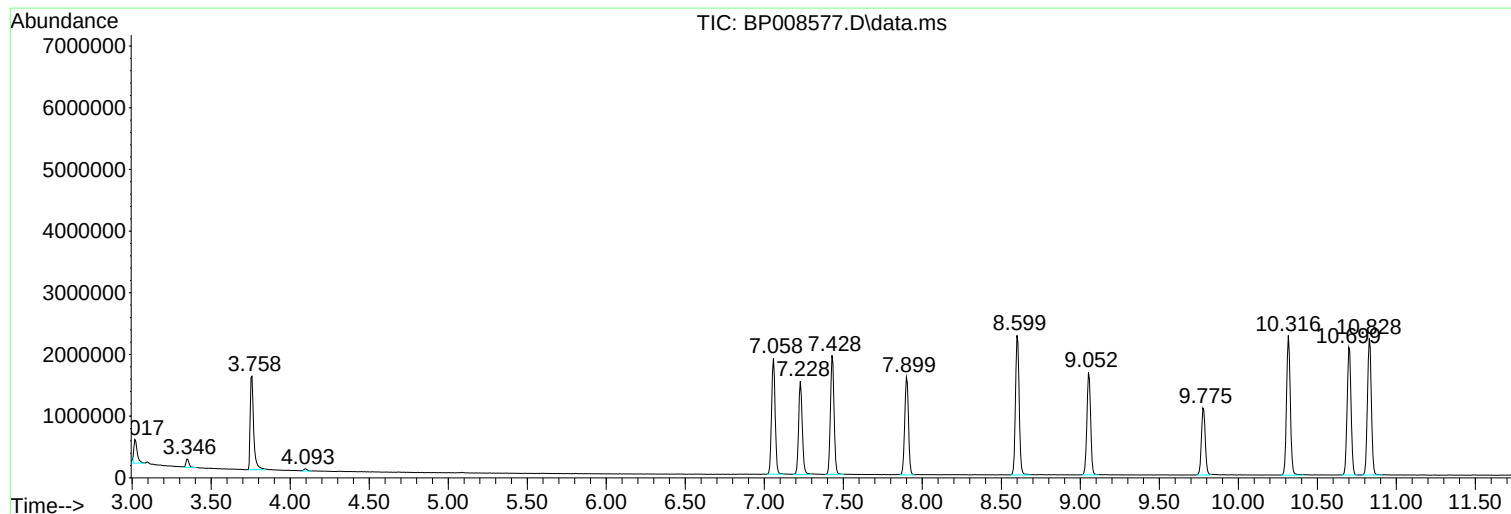

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122721\
Data File : BP008577.D
Acq On : 28 Dec 2021 12:28
Operator : CG/JU
Sample : PB141663BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK663










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic3.017 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.017	4.17 ng/ul	540491	1,4-Dichlorobenzene-d4	7.899

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexane	84	C6H12	000110-82-7	94
2			Cyclohexane	84	C6H12	000110-82-7	91
3			Cyclohexane	84	C6H12	000110-82-7	91
4			Cyclopentane, methyl-	84	C6H12	000096-37-7	83
5			1-Pentene, 2-methyl-	84	C6H12	000763-29-1	64

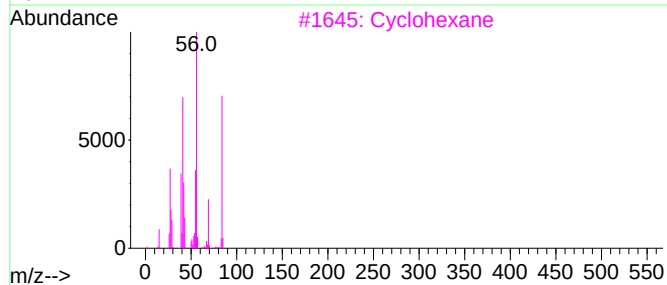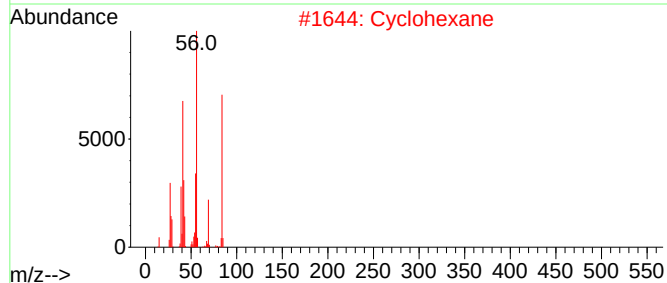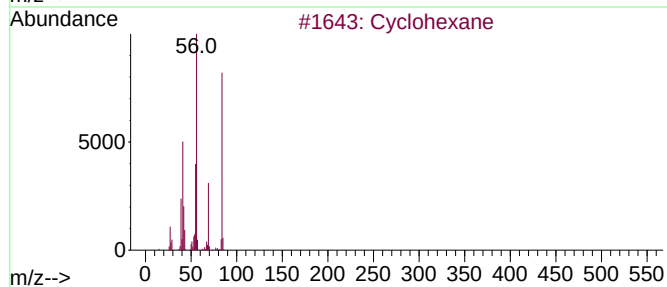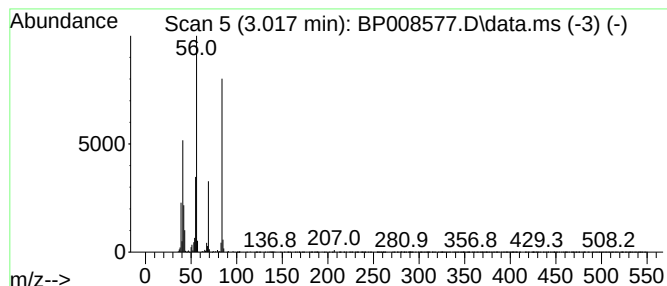

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122721\
Data File : BP008577.D
Acq On : 28 Dec 2021 12:28
Operator : CG/JU
Sample : PB141663BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK663

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP122321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	3.017	4.2	ng/u1	540491	1	7.899	2593540	20.0