


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122819\
 Data File : BP001478.D
 Acq On : 28 Dec 2019 16:32
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP121919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 24 16:04:49 2019

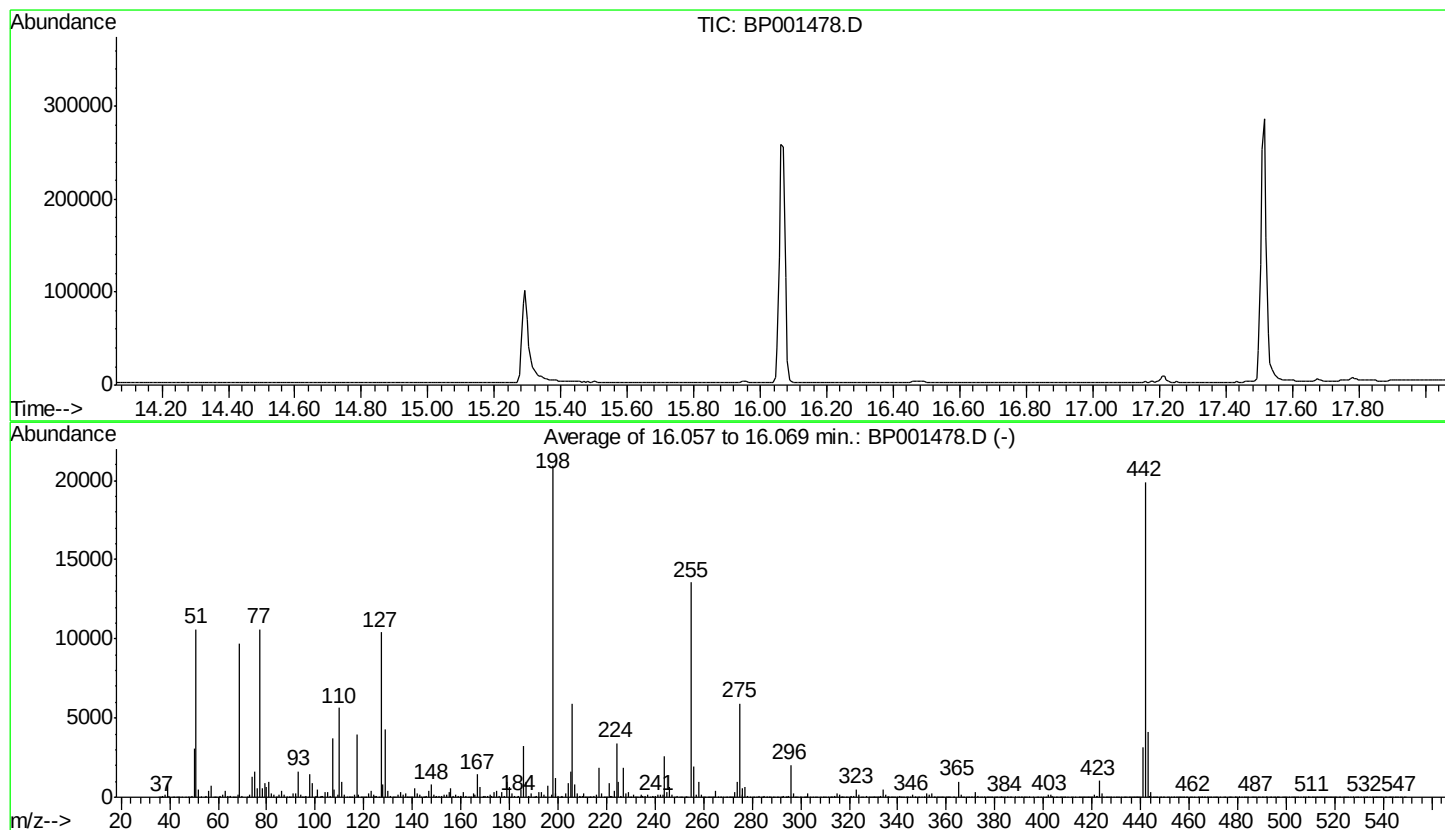

AutoFind: Scans 2375, 2376, 2377; Background Corrected with Scan 2367

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.6	10596	PASS
68	69	0.00	2	1.9	182	PASS
69	198	0.00	100	46.2	9670	PASS
70	69	0.00	2	0.7	69	PASS
127	198	10	80	49.7	10399	PASS
197	198	0.00	2	0.8	161	PASS
198	198	100	100	100.0	20934	PASS
199	198	5	9	5.7	1188	PASS
275	198	10	60	28.4	5937	PASS
365	198	1	100	4.7	978	PASS
441	198	0.01	100	15.1	3168	PASS
442	198	50	100	95.0	19893	PASS
443	442	15	24	20.8	4141	PASS