

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122820\
 Data File : BP004454.D
 Acq On : 28 Dec 2020 15:54
 Operator : CG/JU
 Sample : L5204-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AL5

Quant Time: Dec 28 16:20:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 28 14:00:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	224959	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	923754	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.47	164	574215	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.23	188	1250082	20.00	ng/ul	0.00
78) Chrysene-d12	21.33	240	1224956	20.00	ng/ul	0.00
86) Perylene-d12	23.69	264	1289385	20.00	ng/ul	0.01

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.32	96	19948	3.69	ng/uL	0.00
5) Phenol-d5	6.99	99	127379	6.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	317545	28.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	389616	24.39	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	239416	15.39	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	249325	31.18	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	270223	30.99	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	476129	29.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	43368	2.37	ng/ul	0.00
44) Dimethylphthalate-d6	13.88	166	1552803	33.79	ng/ul	0.00
47) Acenaphthylene-d8	14.16	160	2012106	35.25	ng/ul	0.00
52) 4-Nitrophenol-d4	14.68	143	46196	5.56	ng/ul	0.01
58) Fluorene-d10	15.47	176	1368112	34.02	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.60	200	105819	13.12	ng/ul	0.01
71) Anthracene-d10	17.33	188	2329728	37.73	ng/ul	0.00
79) Pyrene-d10	19.58	212	2576221	39.37	ng/ul	0.01
90) Benzo(a)pyrene-d12	23.54	264	2800543	39.43	ng/ul	0.01


Target Compounds					Ovalue	
45) Dimethylphthalate	13.92	163	63865	1.387	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122820\
Data File : BP004454.D
Acq On : 28 Dec 2020 15:54
Operator : CG/JU
Sample : L5204-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AL5

Quant Time: Dec 28 16:20:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 28 14:00:17 2020
Response via : Initial Calibration

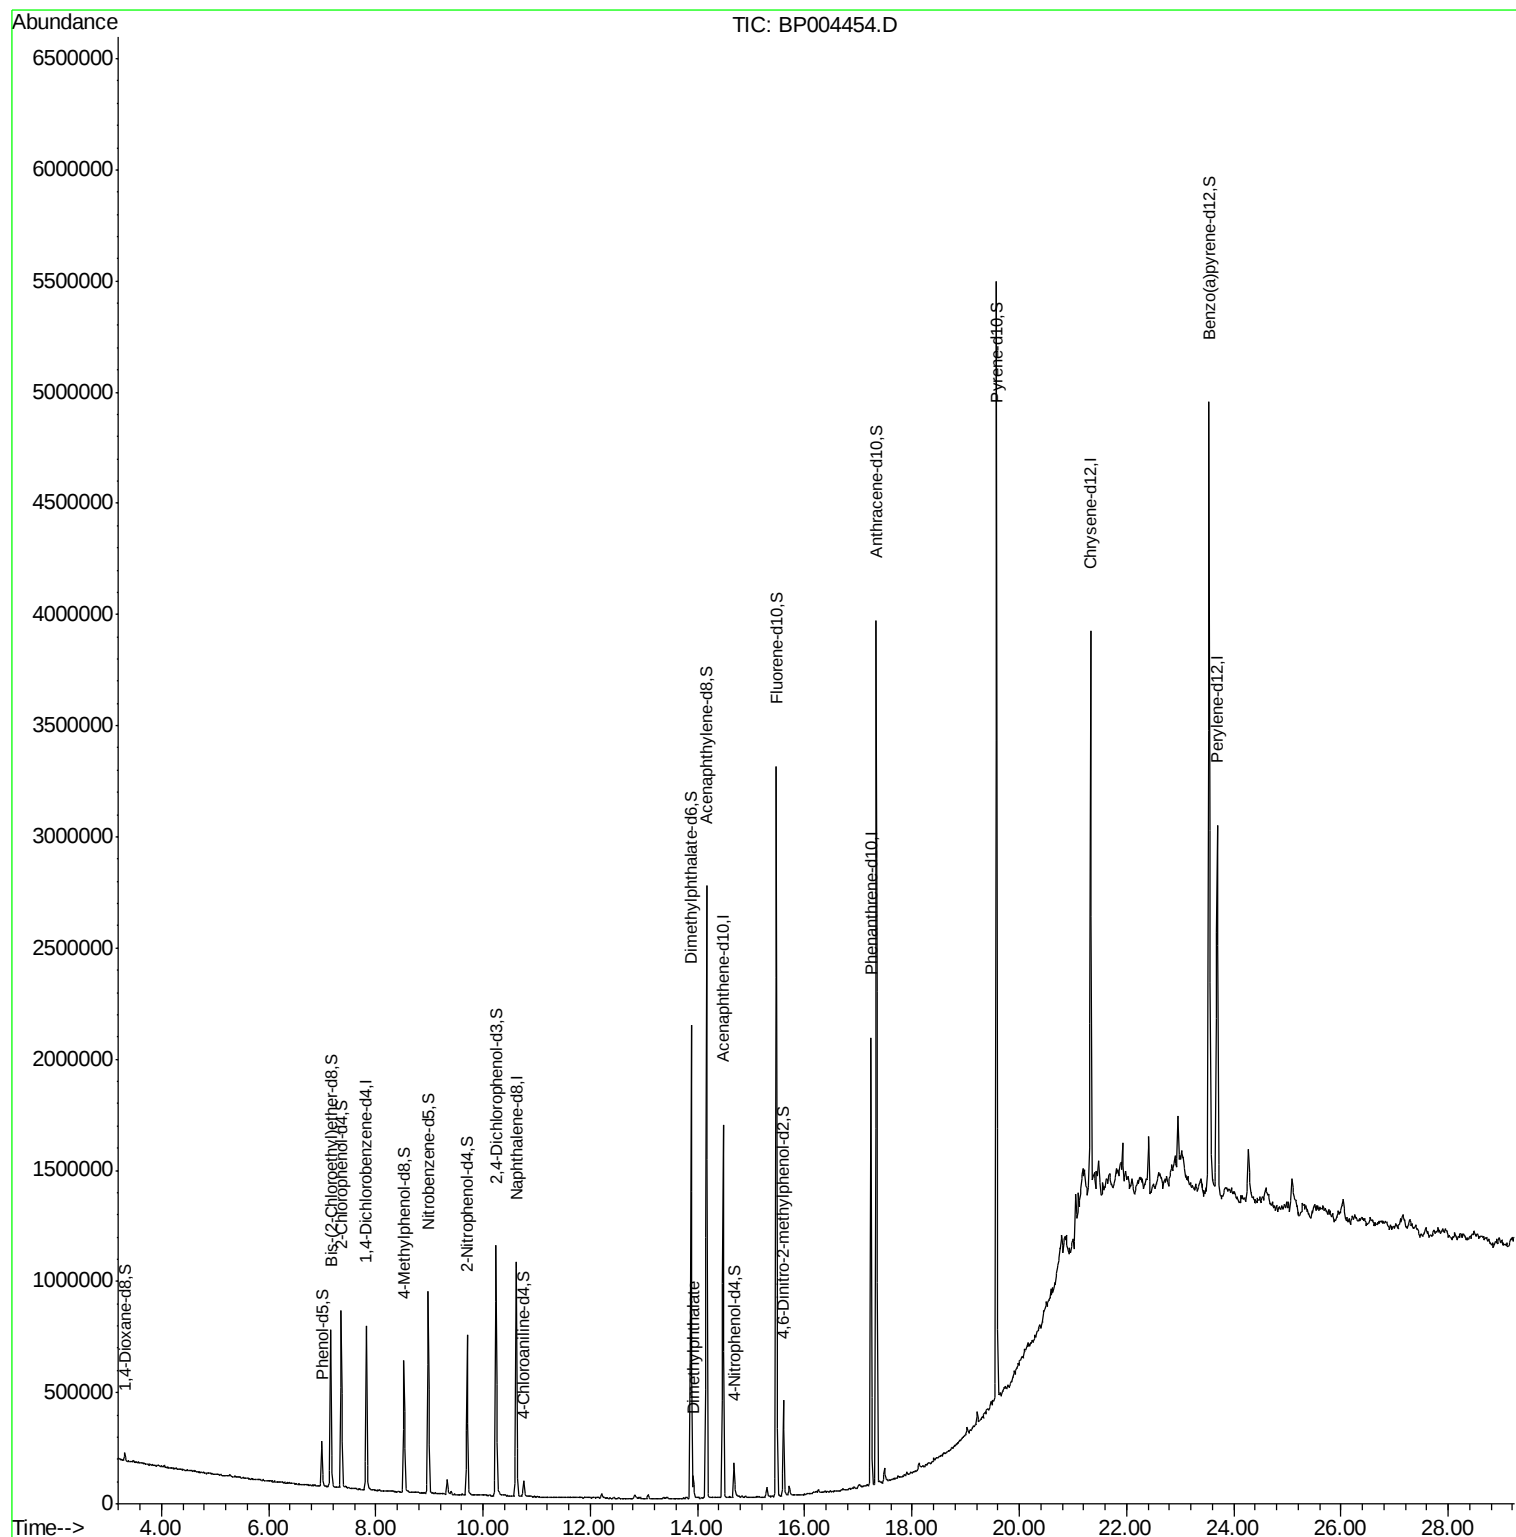

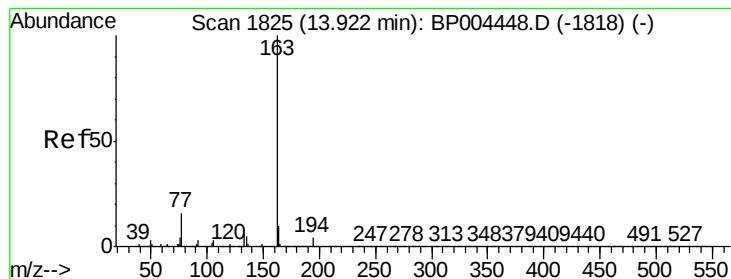

#45

Dimethylphthalate

Concen: 1.387 ng/ul

RT: 13.92 min Scan# 1825

Delta R.T. 0.00 min

Lab File: BP004454.D

Acq: 28 Dec 2020 15:54

Instrument :

BNA_P

ClientSampleId :

C0AL5

Tot Ion:163 Resp: 63865

Ion Ratio Lower Upper

163 100

194 3.5 3.5 5.3#

164 10.2 7.8 11.8

