

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122820\
 Data File : BP004455.D
 Acq On : 28 Dec 2020 16:28
 Operator : CG/JU
 Sample : L5204-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AL7

Quant Time: Dec 28 16:55:43 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 28 14:00:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	196202	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	776780	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.47	164	485871	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.23	188	1063789	20.00	ng/ul	0.00
78) Chrysene-d12	21.33	240	1124746	20.00	ng/ul	0.00
86) Perylene-d12	23.69	264	1228278	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	281271	59.62	ng/uL	-0.02
5) Phenol-d5	6.99	99	135805	7.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	319435	33.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	399532	28.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	252377	18.60	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	246446	36.65	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	271824	37.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	472173	34.73	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	46806	3.04	ng/ul	0.00
44) Dimethylphthalate-d6	13.88	166	1525767	39.23	ng/ul	0.00
47) Acenaphthylene-d8	14.16	160	1988094	41.16	ng/ul	0.00
52) 4-Nitrophenol-d4	14.68	143	49242	7.01	ng/ul	0.01
58) Fluorene-d10	15.47	176	1354124	39.80	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.60	200	117795	17.16	ng/ul	0.00
71) Anthracene-d10	17.33	188	2230644	42.45	ng/ul	0.00
79) Pyrene-d10	19.57	212	2703712	45.00	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.54	264	2953100	43.65	ng/ul	0.01


Target Compounds					Ovalue
45) Dimethylphthalate	13.92	163	92826	2.382	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122820\
Data File : BP004455.D
Acq On : 28 Dec 2020 16:28
Operator : CG/JU
Sample : L5204-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AL7

Quant Time: Dec 28 16:55:43 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 28 14:00:17 2020
Response via : Initial Calibration

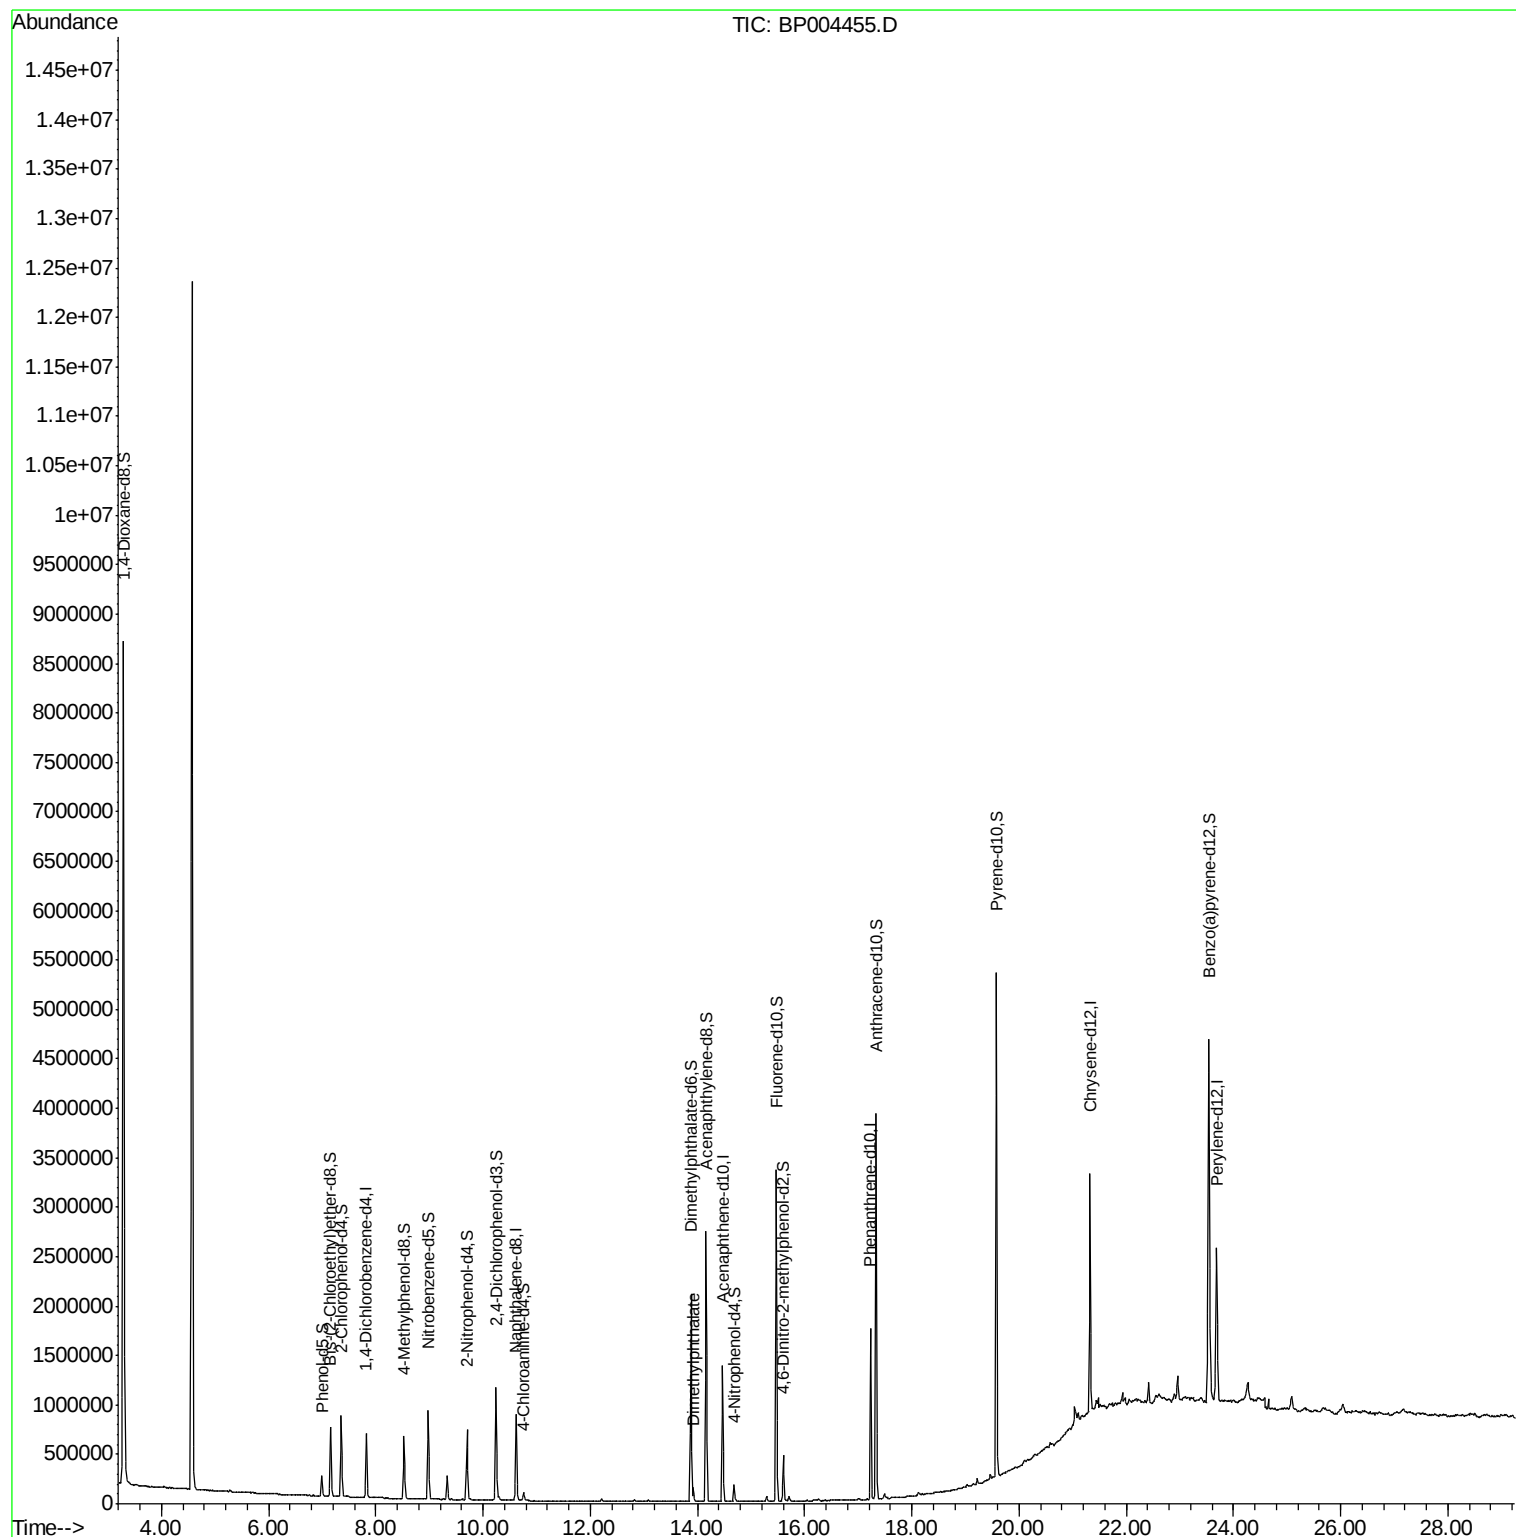

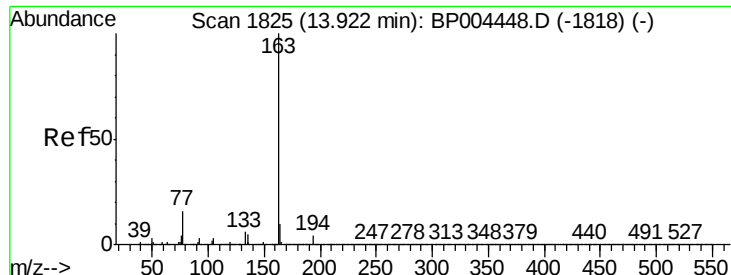

#45

Dimethylphthalate

Concen: 2.382 ng/ul

RT: 13.92 min Scan# 1825

Delta R.T. -0.00 min

Lab File: BP004455.D

Acq: 28 Dec 2020 16:28

Instrument :

BNA_P

ClientSampleId :

C0AL7


Tot Ion:163 Resp: 92826

Ion Ratio Lower Upper

163 100

194 4.9 3.5 5.3

164 9.7 7.8 11.8

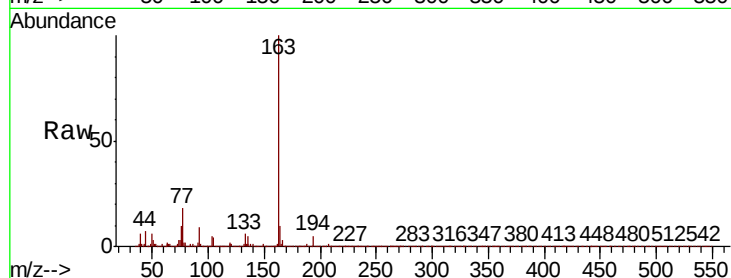

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

