

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122820\
 Data File : BP004457.D
 Acq On : 28 Dec 2020 17:36
 Operator : CG/JU
 Sample : L5195-03DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.993	643	647	657	rVB	37244	69716	1.90%	0.238%
2	7.157	670	675	683	rVB	121085	204573	5.59%	0.698%
3	7.357	703	709	718	rVB	142380	246025	6.72%	0.839%
4	7.822	782	788	799	rVB	812038	1307190	35.71%	4.460%
5	8.193	848	851	857	rVB2	16341	25948	0.71%	0.089%
6	8.528	903	908	916	rVB2	101959	167282	4.57%	0.571%
7	8.981	979	985	995	rVB	155462	277787	7.59%	0.948%
8	9.704	1101	1108	1118	rVB	116384	210121	5.74%	0.717%
9	9.875	1132	1137	1139	rBV4	5389	7523	0.21%	0.026%
10	10.022	1160	1162	1167	rVB4	3859	4181	0.11%	0.014%
11	10.240	1193	1199	1214	rBV	187649	350667	9.58%	1.196%
12	10.616	1255	1263	1278	rVV	1102190	1886670	51.54%	6.437%
13	10.787	1278	1292	1299	rVB3	21554	81085	2.22%	0.277%
14	11.198	1356	1362	1367	rVB8	4140	8417	0.23%	0.029%
15	11.728	1447	1452	1460	rVB	10010	18786	0.51%	0.064%
16	12.022	1496	1502	1503	rBV5	3564	5371	0.15%	0.018%
17	12.181	1523	1529	1533	rBV	15407	27281	0.75%	0.093%
18	12.328	1550	1554	1560	rVB7	4154	8391	0.23%	0.029%
19	12.487	1579	1581	1587	rVB5	5667	10204	0.28%	0.035%
20	12.804	1633	1635	1641	rVB7	2744	3662	0.10%	0.012%
21	12.910	1648	1653	1659	rVB10	3217	7257	0.20%	0.025%
22	13.075	1676	1681	1684	rVB6	3719	5586	0.15%	0.019%
23	13.181	1693	1699	1706	rBV	20242	36194	0.99%	0.123%
24	13.298	1713	1719	1725	rBV2	23643	40091	1.10%	0.137%
25	13.434	1737	1742	1746	rBV8	6673	12919	0.35%	0.044%
26	13.492	1746	1752	1762	rVV2	21243	50459	1.38%	0.172%
27	13.598	1764	1770	1775	rVV5	8943	16675	0.46%	0.057%
28	13.645	1775	1778	1786	rVB10	4540	9990	0.27%	0.034%
29	13.875	1811	1817	1822	rBV	435920	608067	16.61%	2.075%
30	13.922	1822	1825	1830	rVB	27570	38525	1.05%	0.131%
31	14.063	1845	1849	1853	rVB7	2358	4028	0.11%	0.014%
32	14.163	1853	1866	1876	rBV	503980	776491	21.21%	2.649%
33	14.469	1908	1918	1929	rBV	1665571	2550305	69.67%	8.701%
34	14.557	1929	1933	1940	rVB6	5848	9942	0.27%	0.034%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122820\
 Data File : BP004457.D
 Acq On : 28 Dec 2020 17:36
 Operator : CG/JU
 Sample : L5195-03DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

35	14.639	1944	1947	1950	rBV5	4638	6701	0.18%	0.023%
36	14.681	1950	1954	1962	rVB2	21513	38079	1.04%	0.130%
37	14.869	1983	1986	1993	rVB	11822	21274	0.58%	0.073%
38	15.022	2007	2012	2017	rVV4	12119	20633	0.56%	0.070%
39	15.104	2017	2026	2031	rBV3	32215	61898	1.69%	0.211%
40	15.216	2041	2045	2050	rVV8	2946	4995	0.14%	0.017%
41	15.292	2053	2058	2064	rVB6	6199	12523	0.34%	0.043%
42	15.469	2080	2088	2094	rBV	679839	951832	26.00%	3.248%
43	15.522	2094	2097	2103	rVB	33381	47380	1.29%	0.162%
44	15.610	2105	2112	2123	rBV	727184	1191002	32.54%	4.064%
45	15.816	2142	2147	2153	rVB5	10073	18720	0.51%	0.064%
46	15.969	2170	2173	2176	rBV5	3792	4642	0.13%	0.016%
47	15.992	2176	2177	2182	rVB5	5858	4776	0.13%	0.016%
48	16.057	2182	2188	2193	rBV9	5739	11460	0.31%	0.039%
49	16.163	2200	2206	2209	rBV6	4125	6985	0.19%	0.024%
50	16.351	2232	2238	2241	rBV8	3559	6361	0.17%	0.022%
51	16.516	2257	2266	2268	rBV6	12526	25249	0.69%	0.086%
52	16.580	2274	2277	2281	rBV2	11545	14467	0.40%	0.049%
53	16.686	2291	2295	2299	rBV5	8114	11376	0.31%	0.039%
54	16.886	2322	2329	2345	rBV	2145543	3374901	92.20%	11.515%
55	17.233	2381	2388	2399	rBV	2088510	3032192	82.84%	10.346%
56	17.333	2399	2405	2415	rVB	768821	1124934	30.73%	3.838%
57	17.433	2417	2422	2425	rBV4	13584	20114	0.55%	0.069%
58	19.574	2781	2786	2798	rBV	1040328	1421518	38.84%	4.850%
59	21.327	3079	3084	3092	rBV	2791984	3571912	97.58%	12.187%
60	23.533	3453	3459	3474	rVB	706855	1555280	42.49%	5.306%
61	23.686	3478	3485	3497	rVB2	1810269	3660392	100.00%	12.489%


Sum of corrected areas: 29309005

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122820\
Data File : BP004457.D
Acq On : 28 Dec 2020 17:36
Operator : CG/JU
Sample : L5195-03DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC4DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

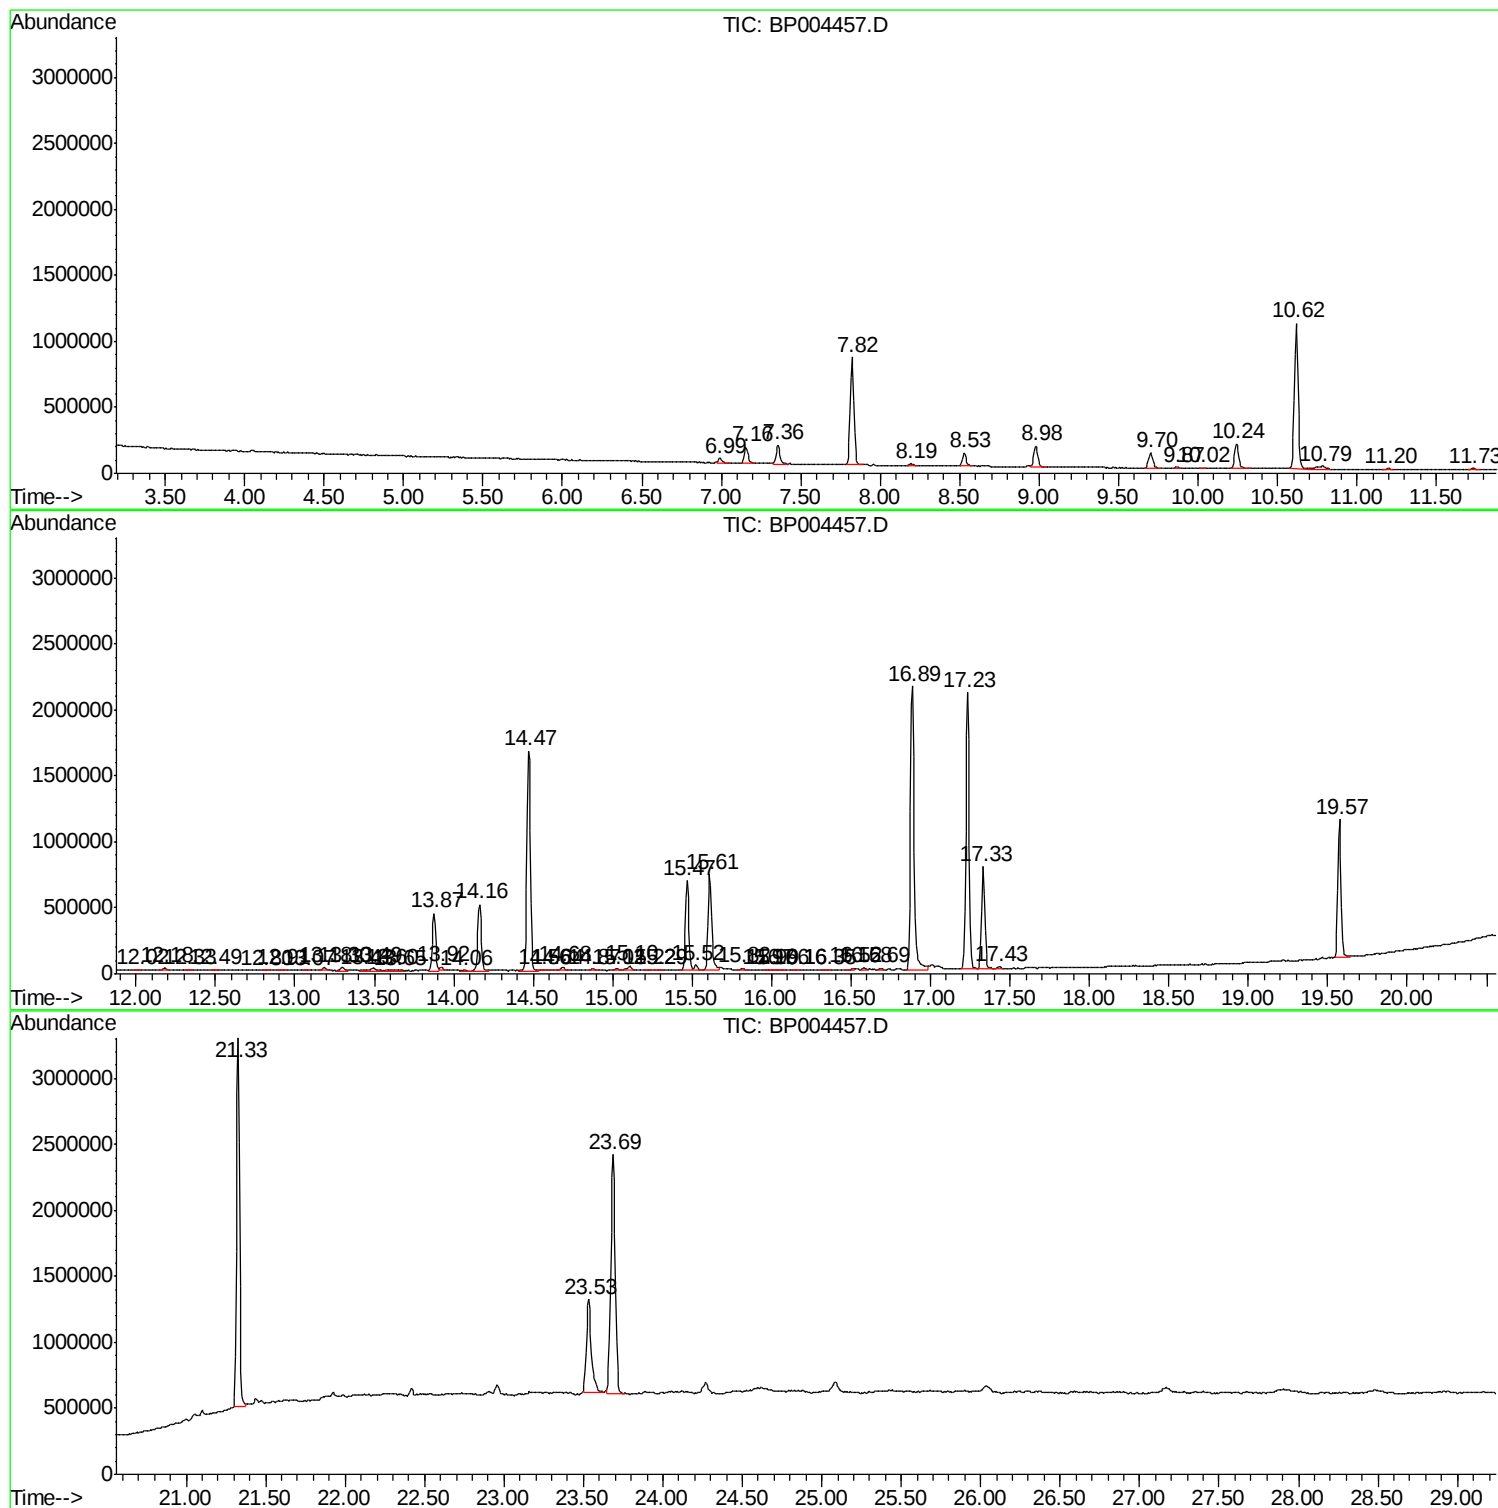

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122820\
Data File : BP004457.D
Acq On : 28 Dec 2020 17:36
Operator : CG/JU
Sample : L5195-03DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC4DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122820\
Data File : BP004457.D
Acq On : 28 Dec 2020 17:36
Operator : CG/JU
Sample : L5195-03DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC4DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc