
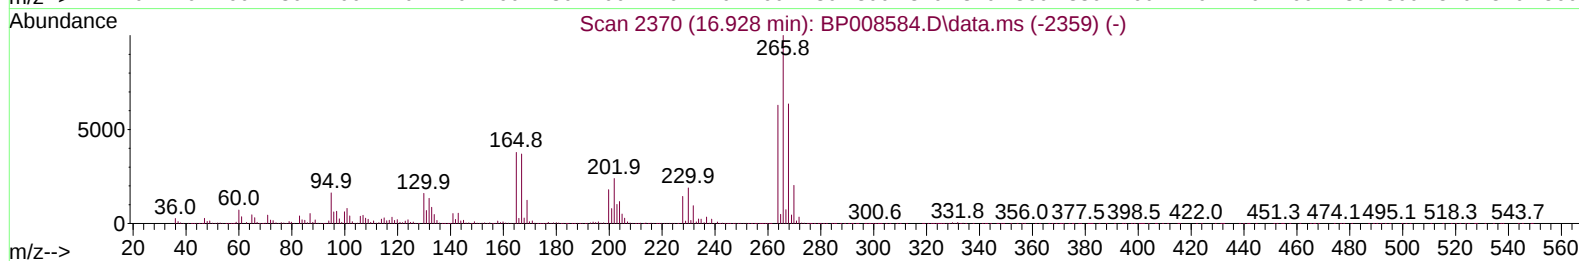
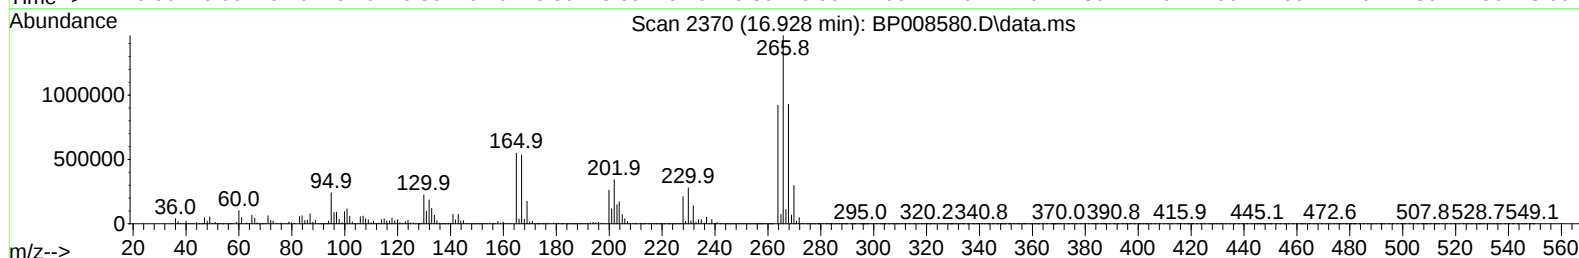


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122821\
 Data File : BP008580.D
 Acq On : 28 Dec 2021 16:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 10:47:27 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 29 09:31:54 2021
 Response via : Initial Calibration

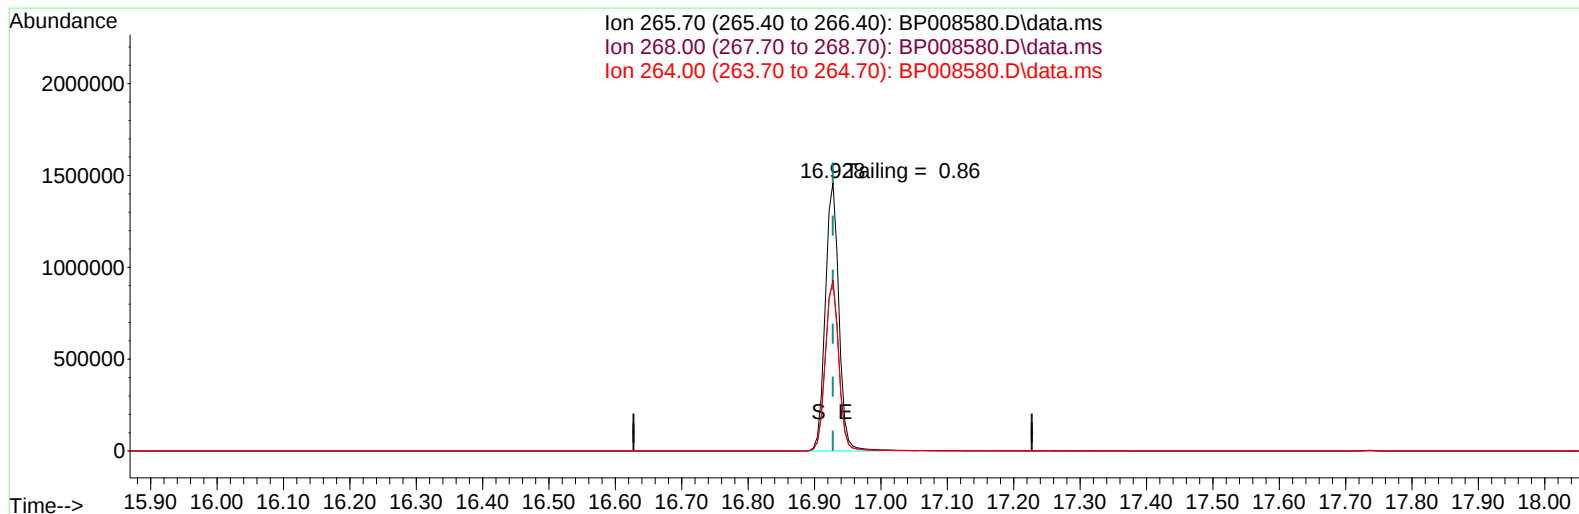

TIC: BP008580.D\data.ms

(70) Pentachlorophenol (C)




16.928min (+ 0.000) 9808541.03 ng

response 2080953

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.56
264.00	62.90	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122821\
 Data File : BP008580.D
 Acq On : 28 Dec 2021 16:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 10:47:27 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 29 09:31:54 2021
 Response via : Initial Calibration

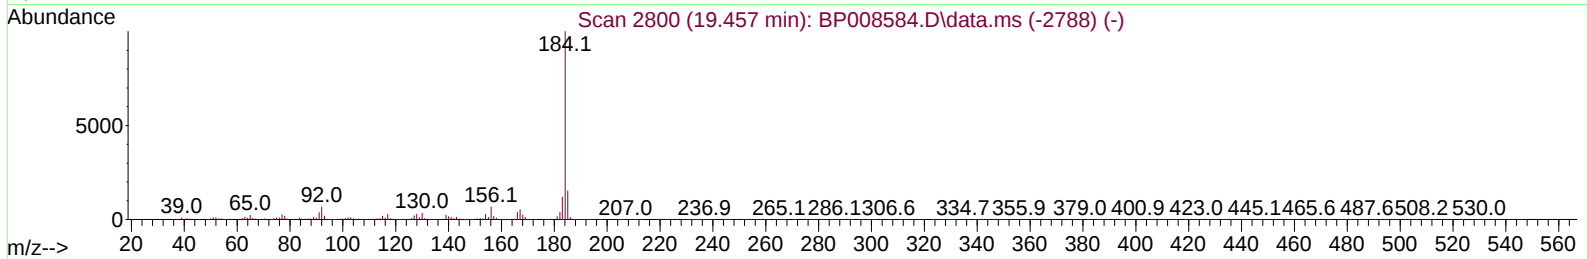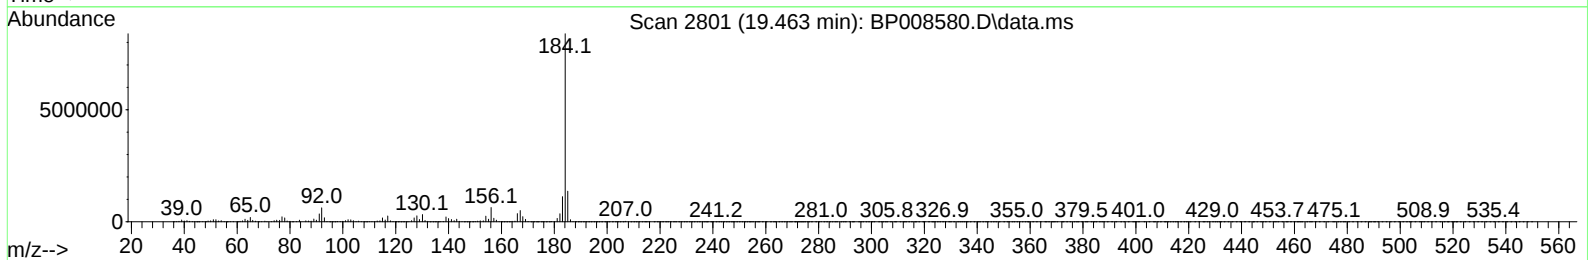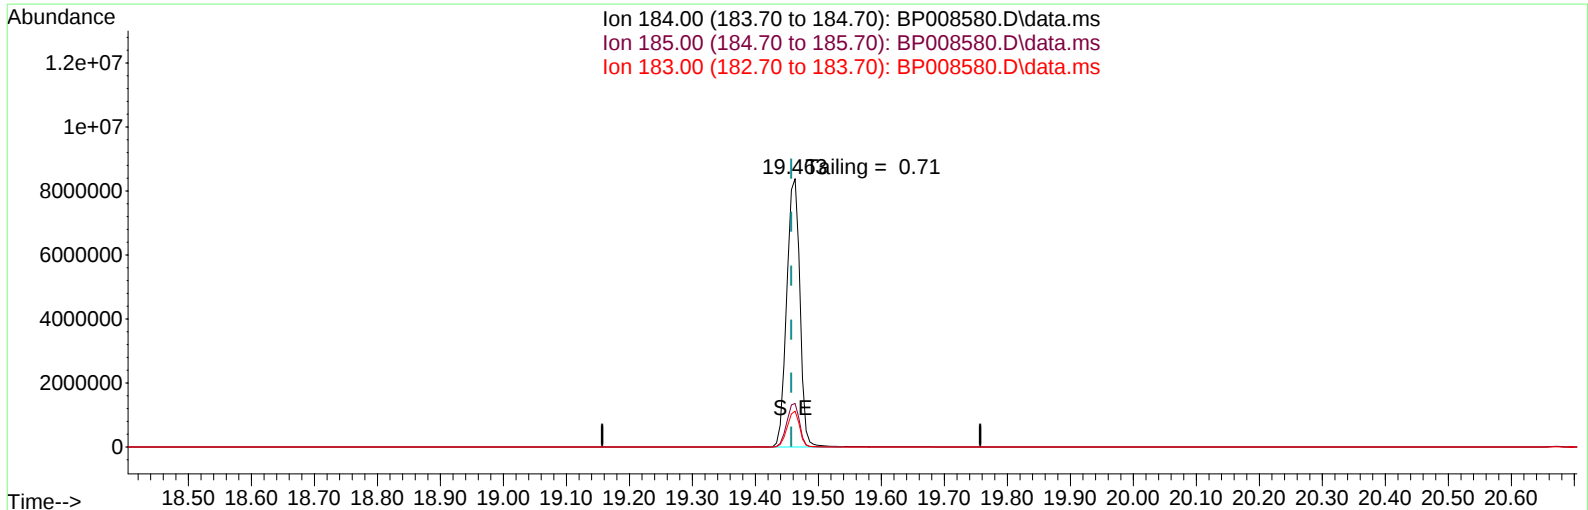

TIC: BP008580.D\data.ms

(77) Benzidine**19.463min (+ 0.006) 2410564.94 ng****response 12285090**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	16.25
183.00	11.90	13.37
0.00	0.00	0.00