

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122821\
 Data File : BP008589.D
 Acq On : 28 Dec 2021 22:16
 Operator : CG/JU
 Sample : PB141705BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB141705BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008589.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.469	415	422	437	rBV	9228352	14303867	33.11%	8.180%
2	7.063	684	693	708	rBV	8913845	14843265	34.36%	8.488%
3	7.898	827	835	844	rBV	2034241	3322531	7.69%	1.900%
4	9.051	1023	1031	1045	rBV	5804624	9709217	22.48%	5.552%
5	10.698	1302	1311	1323	rVB	2861861	4852899	11.23%	2.775%
6	13.157	1721	1729	1739	rBV	18642053	28102043	65.05%	16.070%
7	14.528	1954	1962	1970	rBV	4963654	7456733	17.26%	4.264%
8	16.016	2207	2215	2238	rBV	14528111	21131333	48.92%	12.084%
9	17.274	2422	2429	2437	rBV	6567552	9413491	21.79%	5.383%
10	19.833	2858	2864	2869	rBV2	32023206	43198289	100.00%	24.703%
11	21.357	3117	3123	3131	rBV	7317769	9558591	22.13%	5.466%
12	23.780	3528	3535	3548	rVB2	4403301	8981676	20.79%	5.136%




Sum of corrected areas: 174873935

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122821\
Data File : BP008589.D
Acq On : 28 Dec 2021 22:16
Operator : CG/JU
Sample : PB141705BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141705BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

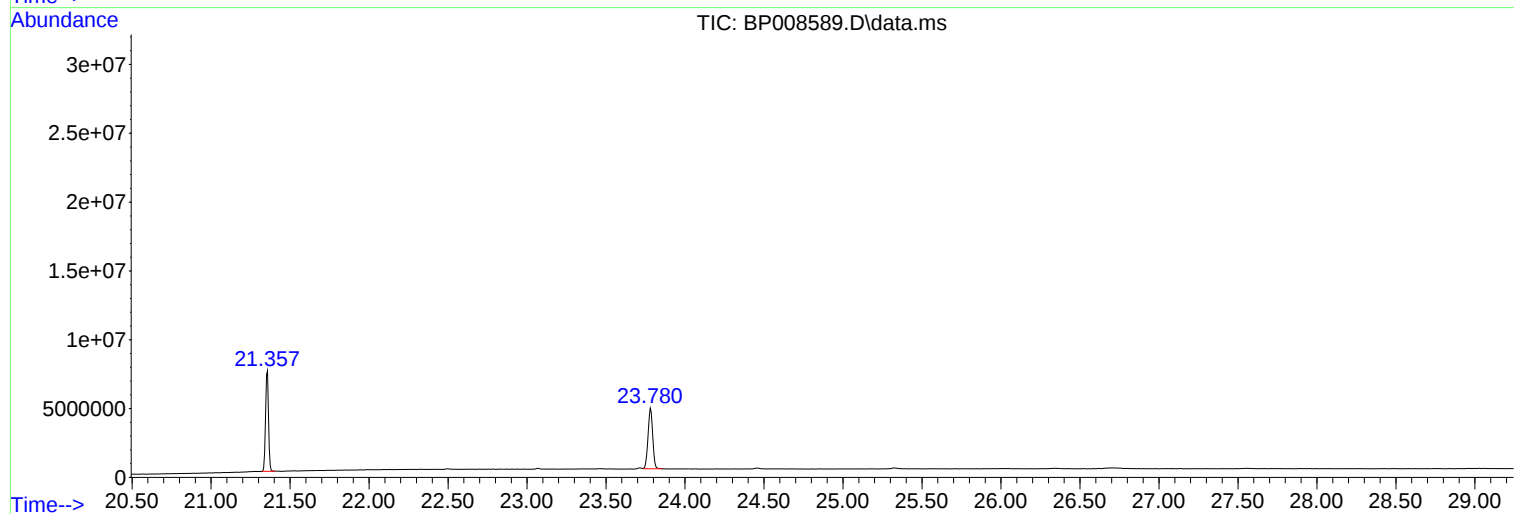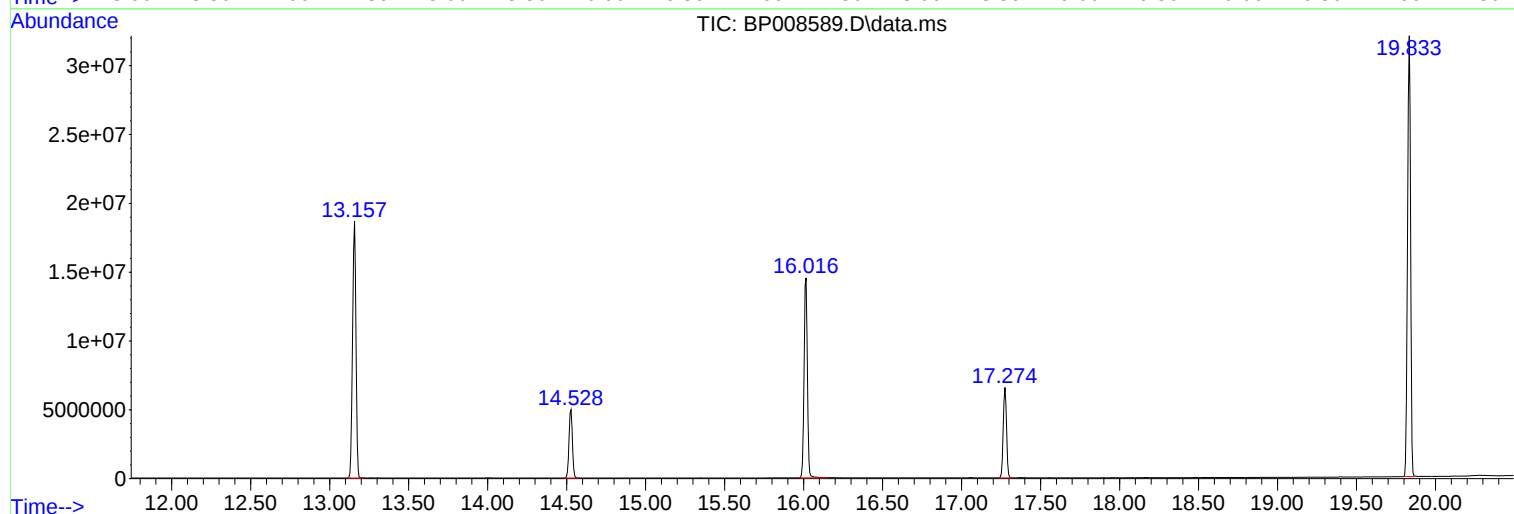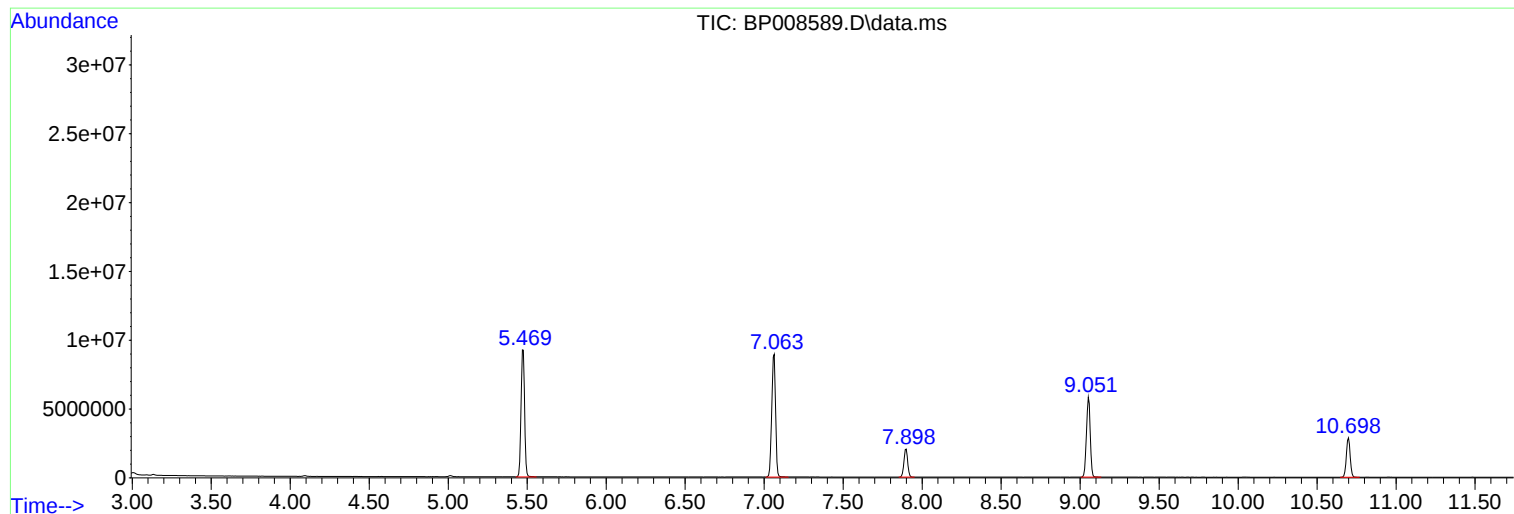

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122821\
Data File : BP008589.D
Acq On : 28 Dec 2021 22:16
Operator : CG/JU
Sample : PB141705BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141705BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122821\
Data File : BP008589.D
Acq On : 28 Dec 2021 22:16
Operator : CG/JU
Sample : PB141705BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141705BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------