
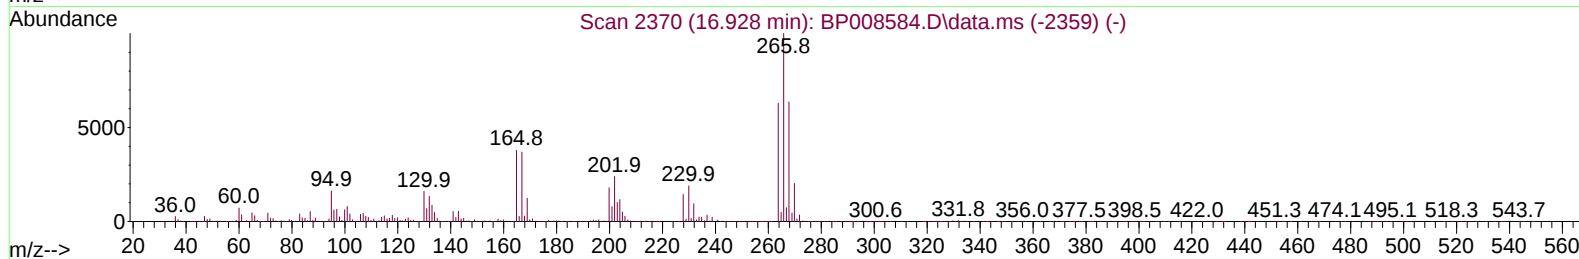
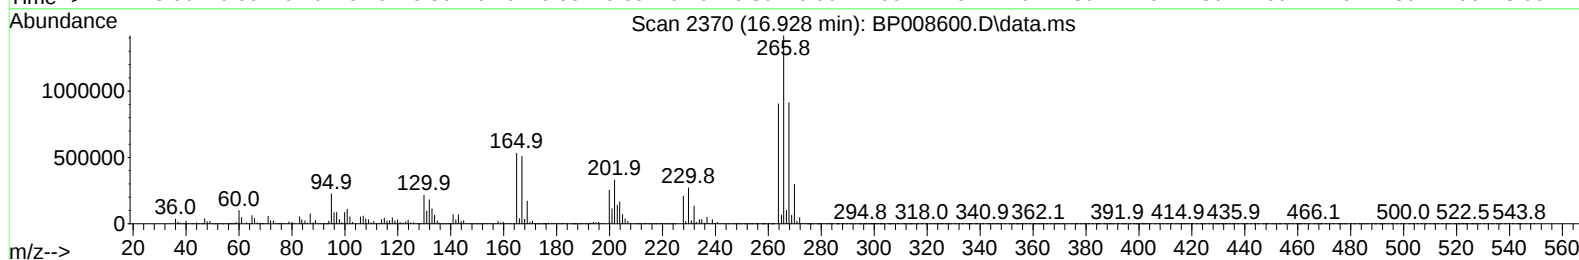


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP123021\  
 Data File : BP008600.D  
 Acq On : 30 Dec 2021 09:09  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 06:51:17 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP122821.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Dec 30 08:44:33 2021  
 Response via : Initial Calibration

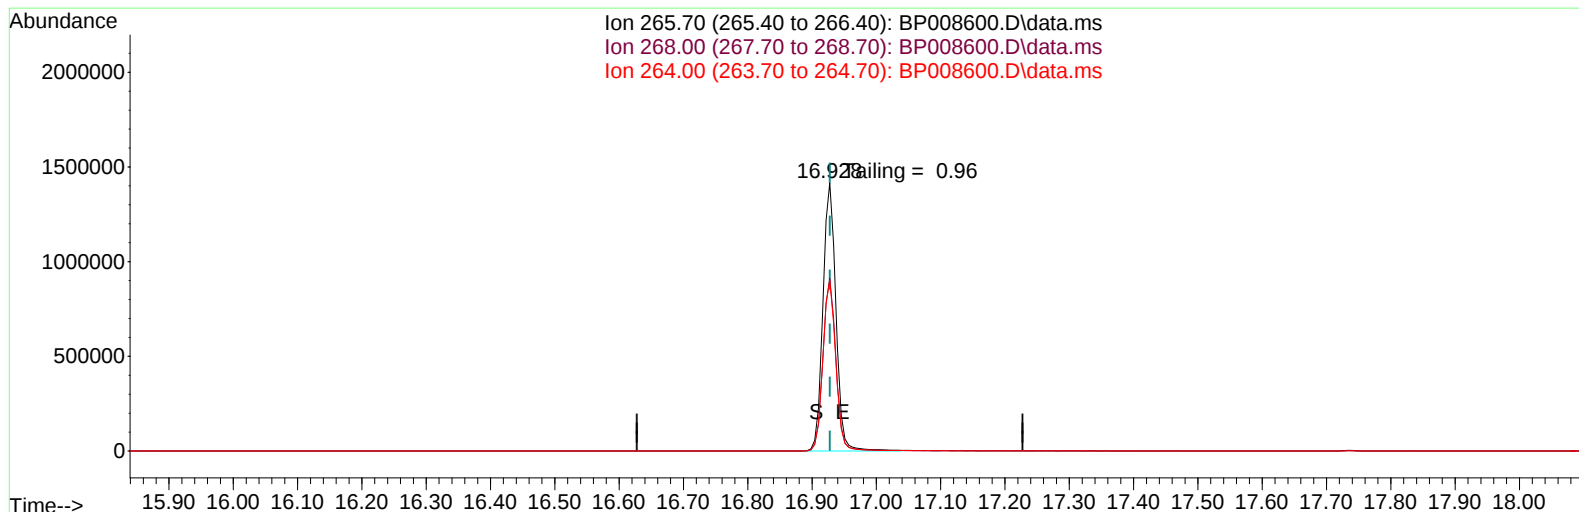

TIC: BP008600.D\data.ms

**(70) Pentachlorophenol (C)**




16.928min (+ 0.000) 252481.25 ng

response 2004097

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.60  | 64.32  |
| 264.00 | 62.90  | 63.71  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP123021\  
 Data File : BP008600.D  
 Acq On : 30 Dec 2021 09:09  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 06:51:17 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP122821.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Dec 30 08:44:33 2021  
 Response via : Initial Calibration

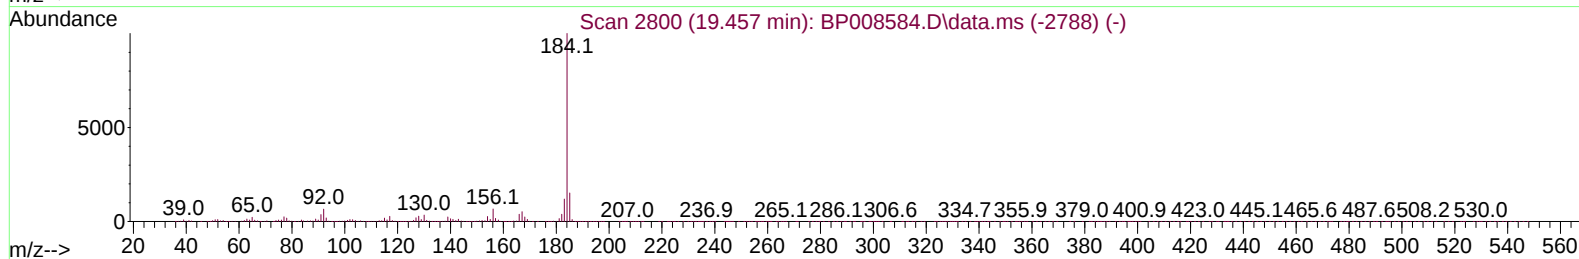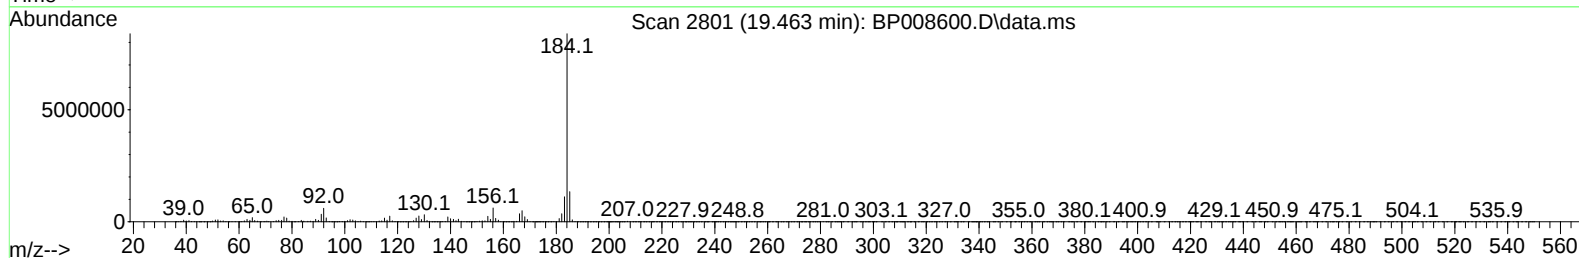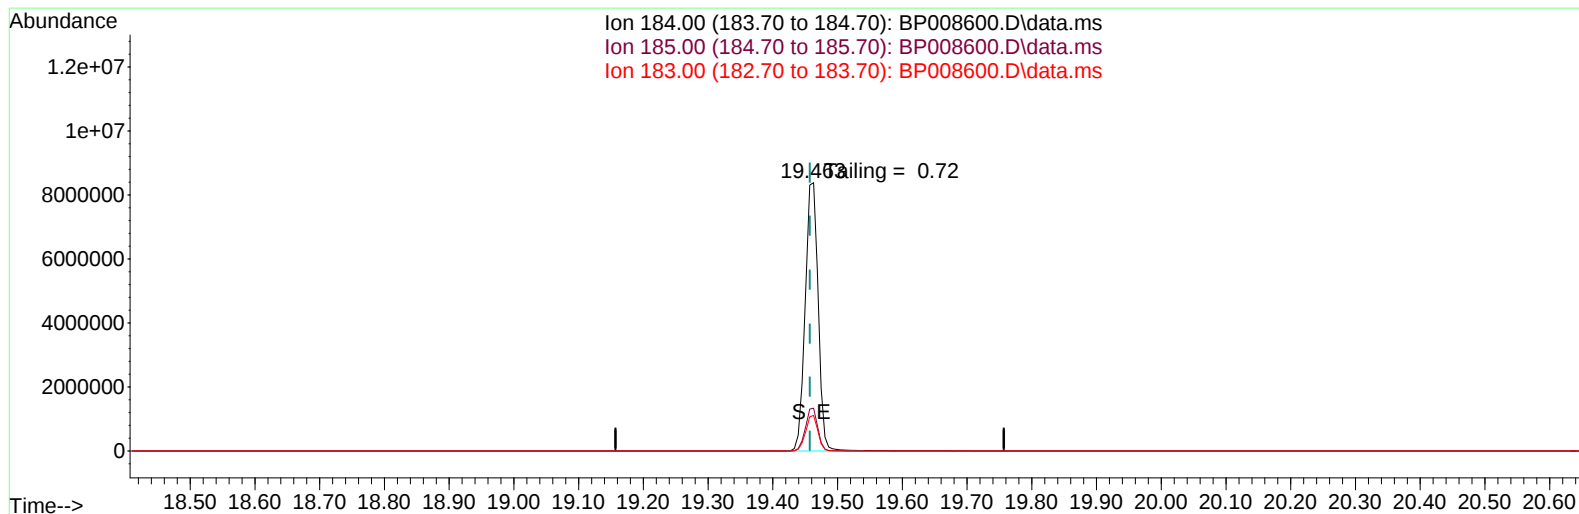

TIC: BP008600.D\data.ms

**(77) Benzidine****19.463min (+ 0.006) 208075.99 ng****response 11739987**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.20  | 15.97  |
| 183.00 | 11.90  | 13.27  |
| 0.00   | 0.00   | 0.00   |