
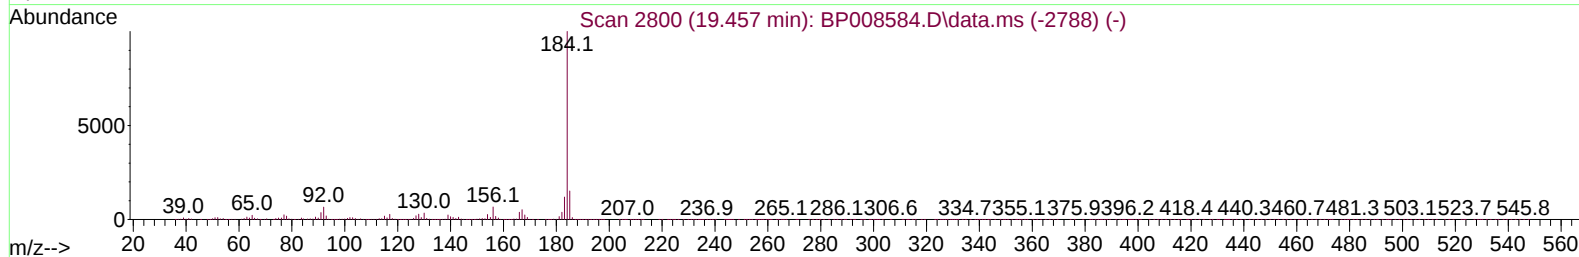
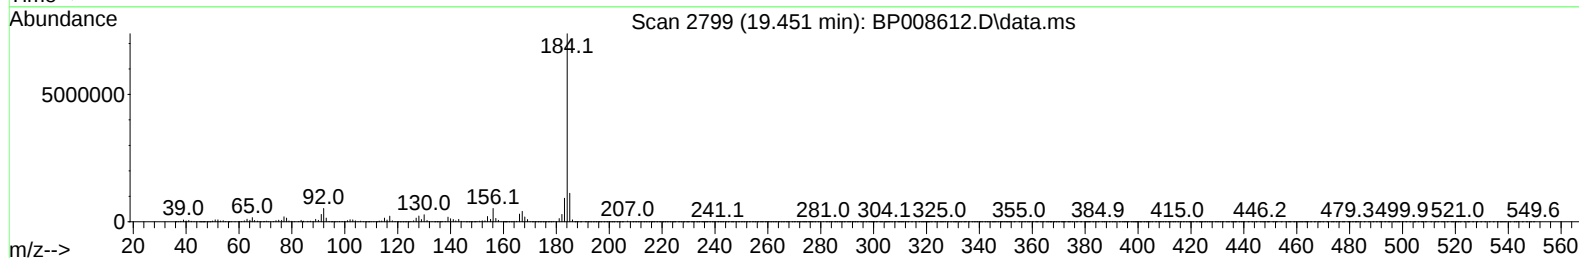


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123021\
Data File : BP008612.D
Acq On : 30 Dec 2021 16:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 07:02:54 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 08:44:33 2021
Response via : Initial Calibration

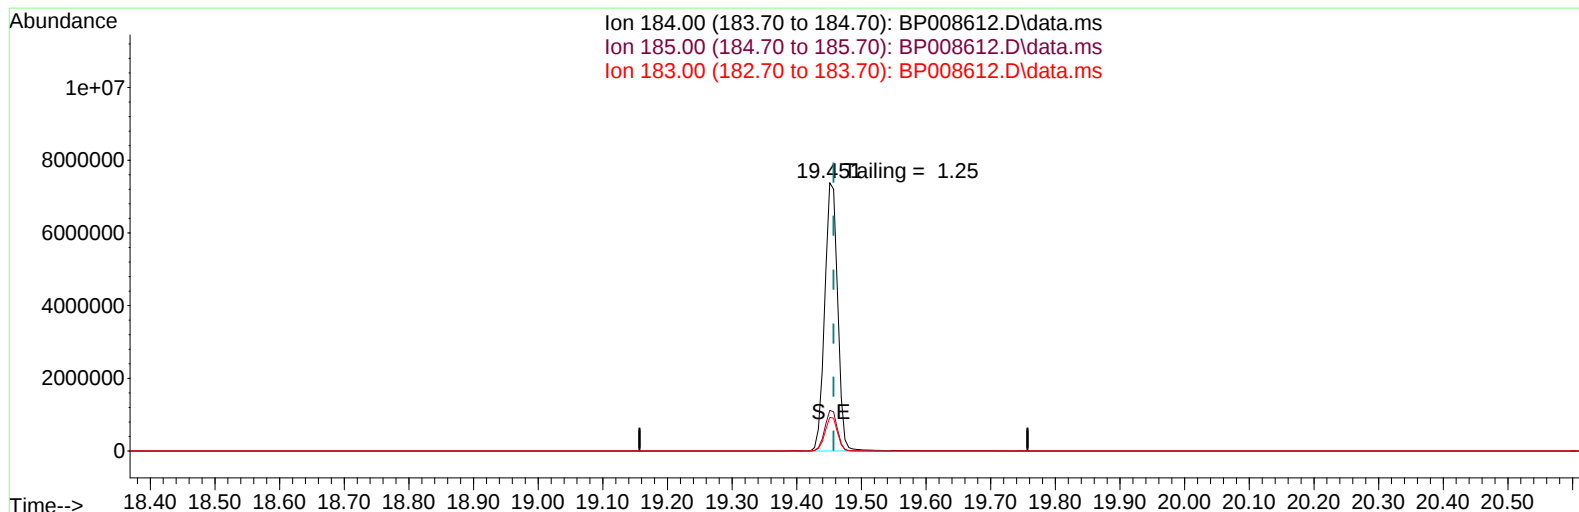




TIC: BP008612.D\data.ms

(77) Benzidine**19.451min (-0.006) 45209.96 ng****response 10325523**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.14
183.00	11.90	12.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123021\
 Data File : BP008612.D
 Acq On : 30 Dec 2021 16:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 07:02:54 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 08:44:33 2021
 Response via : Initial Calibration

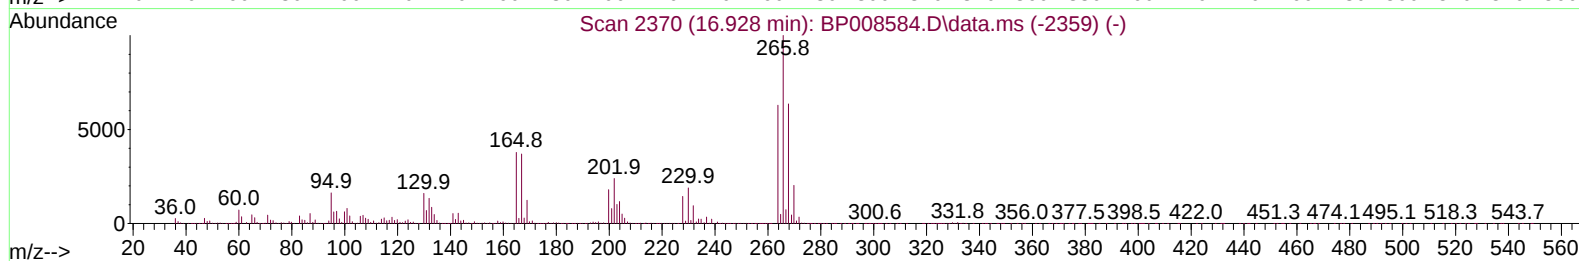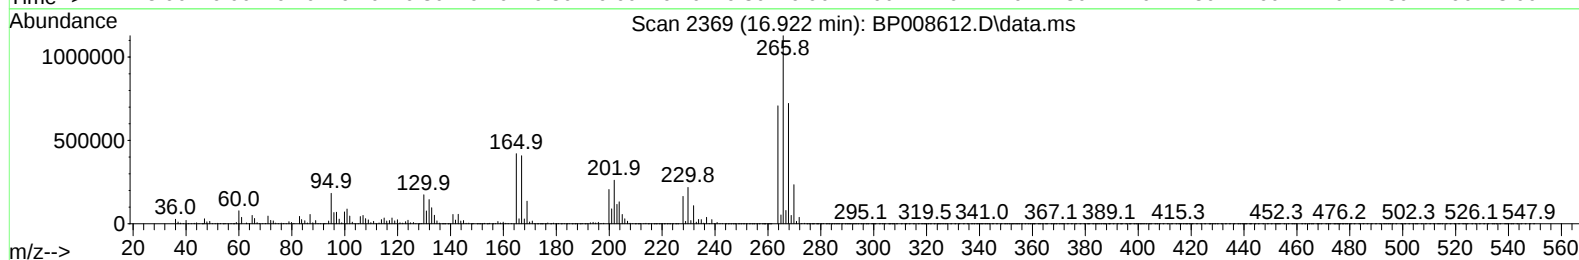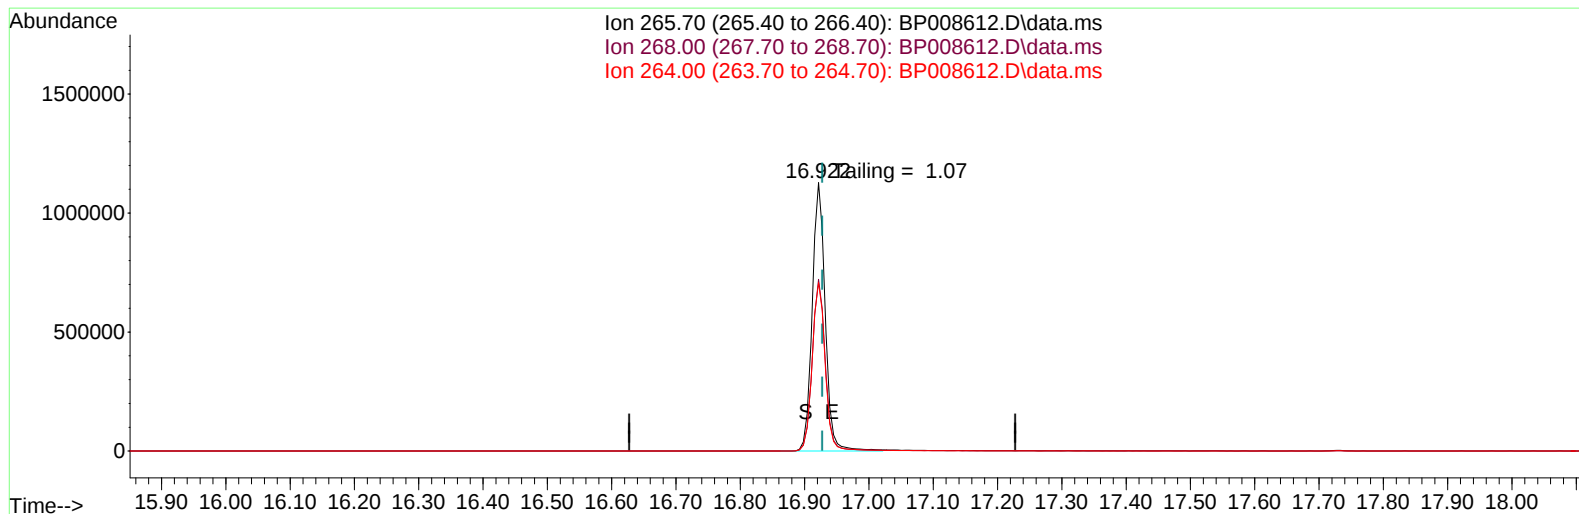

TIC: BP008612.D\data.ms

(70) Pentachlorophenol (C)

16.922min (-0.006) 108059.57 ng

response 1607165

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.96
264.00	62.90	62.71
0.00	0.00	0.00