

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123021\
 Data File : BP008626.D
 Acq On : 31 Dec 2021 01:32
 Operator : CG/JU
 Sample : M5244-30
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONC-11E

Quant Time: Dec 31 08:16:51 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 08:44:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	1077868	20.000	ng	0.00
21) Naphthalene-d8	10.693	136	4295739	20.000	ng	0.00
39) Acenaphthene-d10	14.522	164	2843708	20.000	ng	0.00
64) Phenanthrene-d10	17.269	188	5887155	20.000	ng	0.00
76) Chrysene-d12	21.357	240	4760676	20.000	ng	0.00
86) Perylene-d12	23.780	264	4600016	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.475	112	5523580	93.537	ng	0.00
7) Phenol-d6	7.075	99	6962927	84.712	ng	0.02
23) Nitrobenzene-d5	9.052	82	4140681	57.341	ng	0.00
42) 2,4,6-Tribromophenol	16.016	330	3963650	103.021	ng	0.00
45) 2-Fluorobiphenyl	13.151	172	11170891	56.914	ng	0.00
79) Terphenyl-d14	19.828	244	13189470	56.568	ng	0.00
Target Compounds						
74) Di-n-butylphthalate	18.234	149	1264576	3.808	ng	Qvalue 98
80) Butylbenzylphthalate	20.510	149	2155883	17.452	ng	93
84) Bis(2-ethylhexyl)phtha...	21.275	149	5388717	28.877	ng	99
85) Di-n-octyl phthalate	22.210	149	1174231	4.065	ng	# 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123021\
Data File : BP008626.D
Acq On : 31 Dec 2021 01:32
Operator : CG/JU
Sample : M5244-30
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONC-11E

Quant Time: Dec 31 08:16:51 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 08:44:33 2021
Response via : Initial Calibration




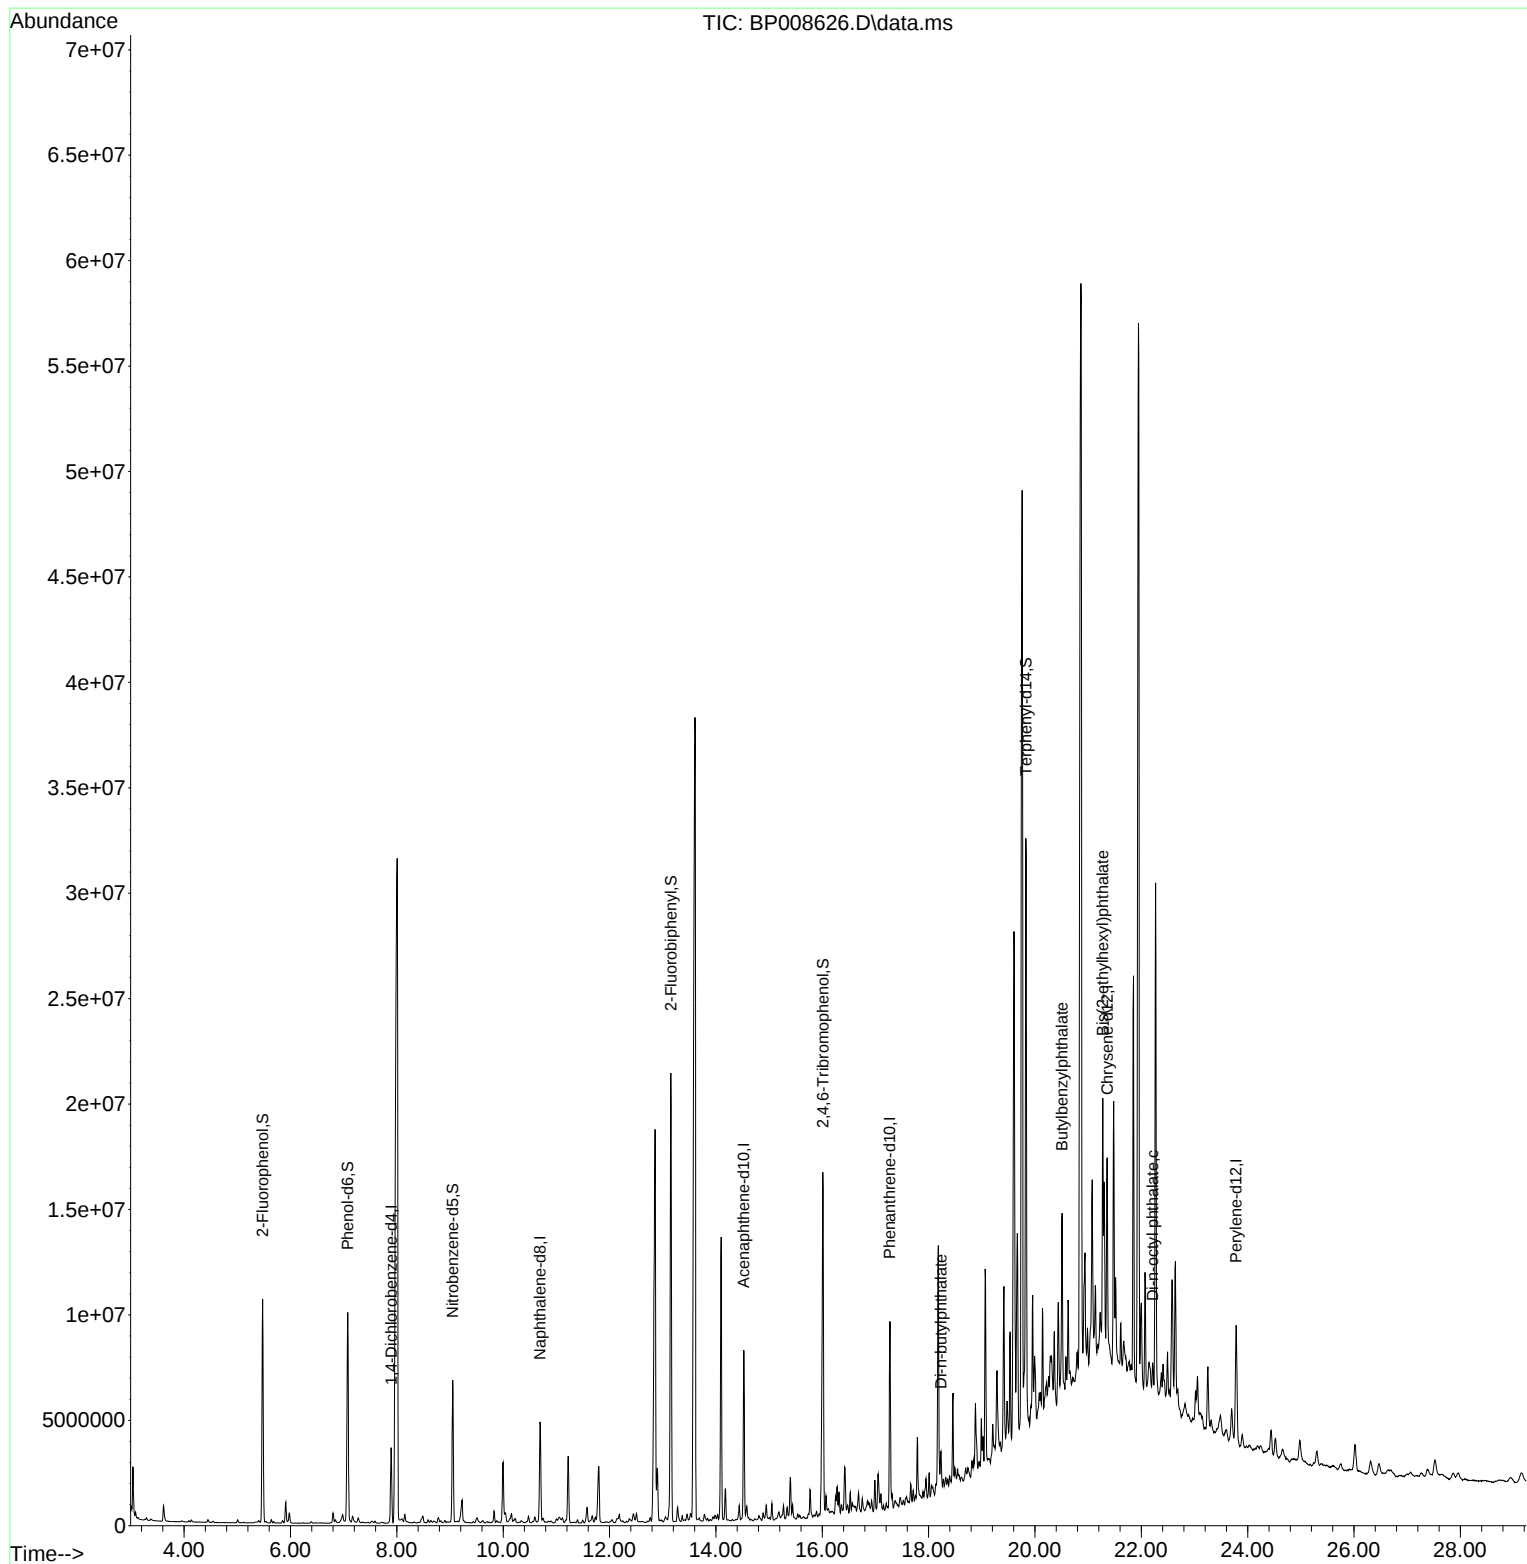




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.893 min Scan# 81
Delta R.T. -0.006 min
Lab File: BP008626.D
Acq: 31 Dec 2021 01:32




Instrument :
BNA_P
ClientSampleId :
CONC-11E


Tgt Ion:152 Resp: 1077868
Ion Ratio Lower Upper
152 100
150 154.6 127.0 190.6
115 53.4 43.7 65.5

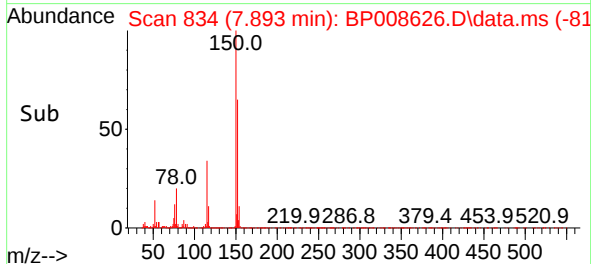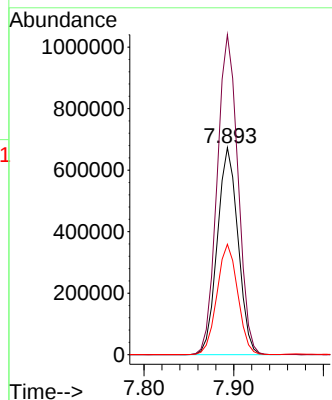

#5
2-Fluorophenol
Concen: 93.537 ng
RT: 5.475 min Scan# 423
Delta R.T. 0.006 min
Lab File: BP008626.D
Acq: 31 Dec 2021 01:32

Tgt Ion:112 Resp: 5523580
Ion Ratio Lower Upper
112 100
64 48.6 39.7 59.5
63 24.5 20.0 30.0

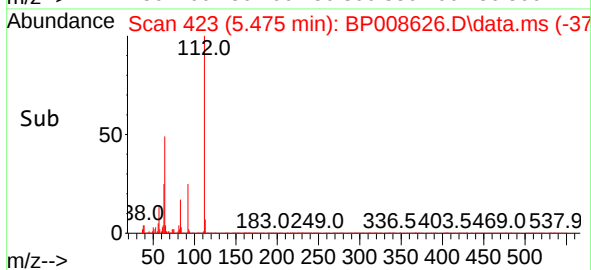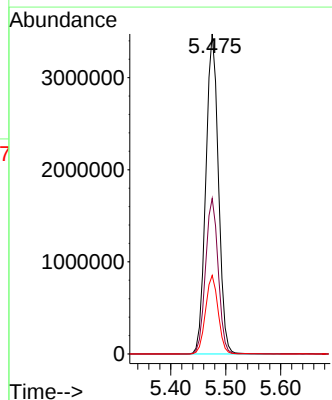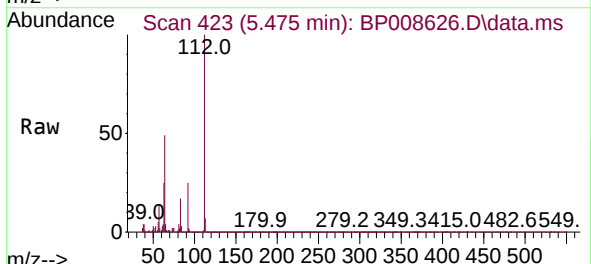







#7
Phenol-d6
Concen: 84.712 ng
RT: 7.075 min Scan# 64
Delta R.T. 0.018 min
Lab File: BP008626.D
Acq: 31 Dec 2021 01:32

Instrument :
BNA_P
ClientSampleId :
CONC-11E

Tgt Ion: 99 Resp: 6962927




Ion	Ratio	Lower	Upper
99	100		
42	13.0	10.8	16.2
71	30.7	23.8	35.6

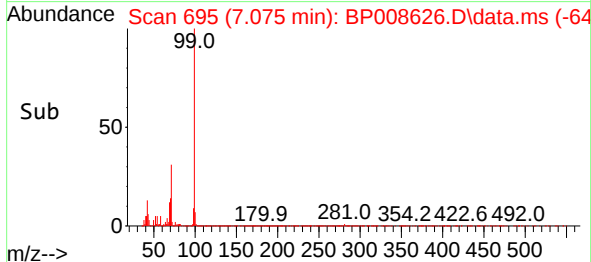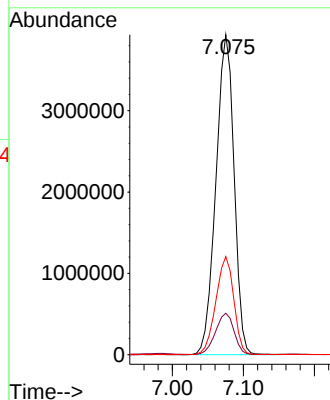


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.693 min Scan# 1310
Delta R.T. -0.006 min
Lab File: BP008626.D
Acq: 31 Dec 2021 01:32

Tgt Ion: 136 Resp: 4295739

Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.0	13.4
54	5.9	4.9	7.3
68	5.6	4.3	6.5


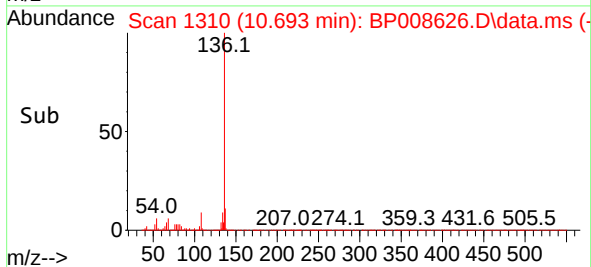
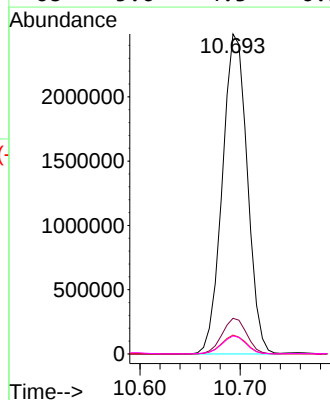
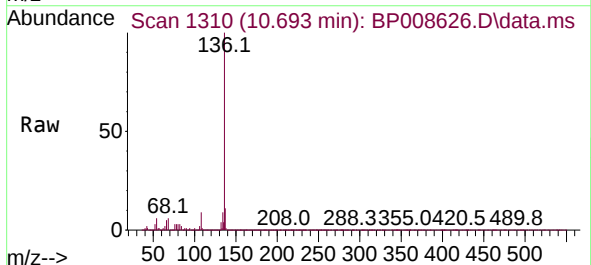




#23
Nitrobenzene-d5
Concen: 57.341 ng
RT: 9.052 min Scan# 1031
Delta R.T. -0.006 min
Lab File: BP008626.D
Acq: 31 Dec 2021 01:32




Instrument :
BNA_P
ClientSampleId :
CONC-11E


Tgt Ion: 82 Resp: 4140681
Ion Ratio Lower Upper
82 100
128 50.7 39.4 59.2
54 39.7 32.6 48.8

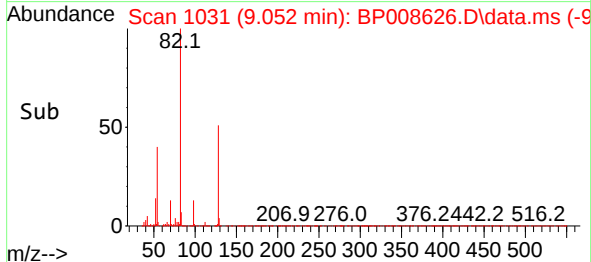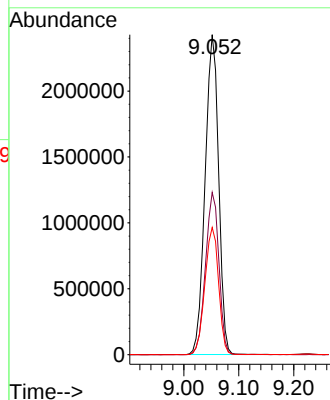

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.522 min Scan# 1961
Delta R.T. -0.006 min
Lab File: BP008626.D
Acq: 31 Dec 2021 01:32

Tgt Ion: 164 Resp: 2843708
Ion Ratio Lower Upper
164 100
162 100.3 79.9 119.9
160 43.7 35.5 53.3


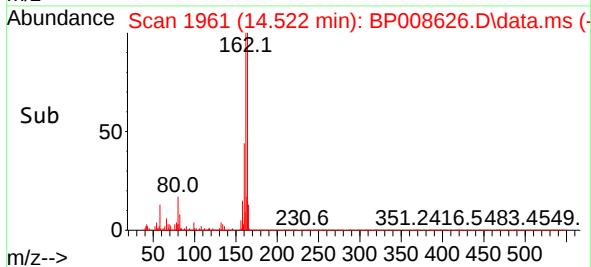
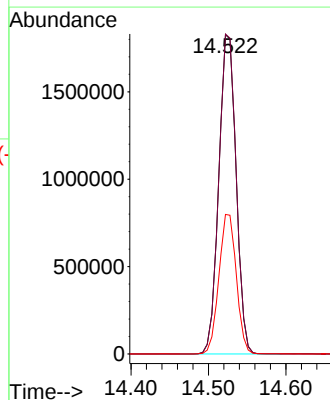
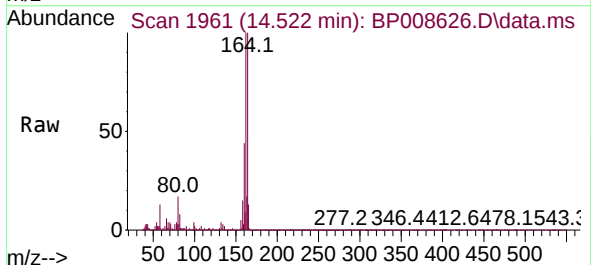




#42
2,4,6-Tribromophenol
Concen: 103.021 ng
RT: 16.016 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP008626.D
Acq: 31 Dec 2021 01:32




Instrument :
BNA_P
ClientSampleId :
CONC-11E


Tgt Ion:330 Resp: 3963650
Ion Ratio Lower Upper
330 100
332 96.3 77.0 115.4
141 23.1 21.3 31.9

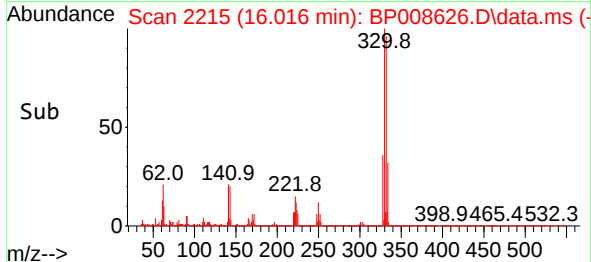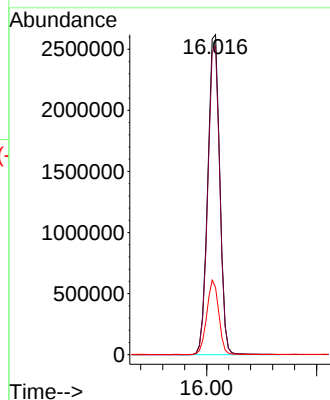

#45
2-Fluorobiphenyl
Concen: 56.914 ng
RT: 13.151 min Scan# 1728
Delta R.T. -0.006 min
Lab File: BP008626.D
Acq: 31 Dec 2021 01:32

Tgt Ion:172 Resp:11170891
Ion Ratio Lower Upper
172 100
171 37.2 29.3 43.9
170 24.6 19.5 29.3


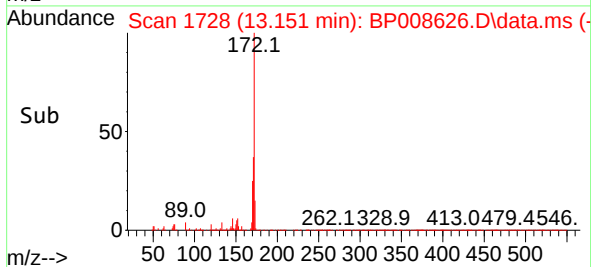
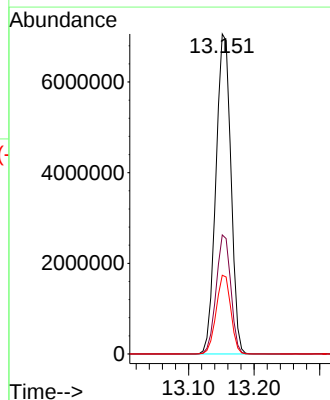
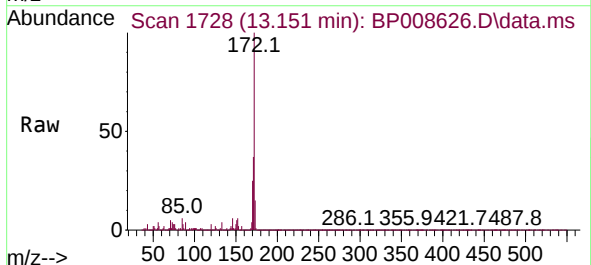




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.269 min Scan# 2429
Delta R.T. -0.006 min
Lab File: BP008626.D
Acq: 31 Dec 2021 01:32




Instrument :
BNA_P
ClientSampleId :
CONC-11E


Tgt Ion:188 Resp: 5887155
Ion Ratio Lower Upper
188 100
94 8.0 6.8 10.2
80 8.4 7.2 10.8

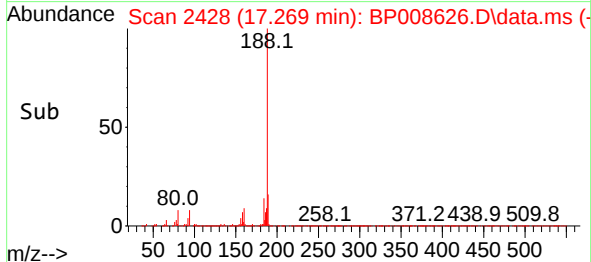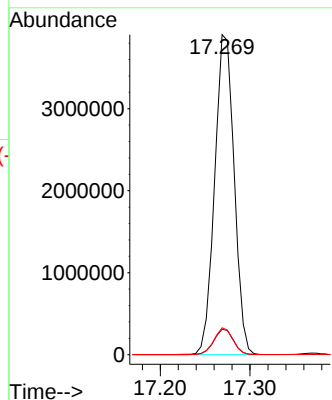

#74
Di-n-butylphthalate
Concen: 3.808 ng
RT: 18.234 min Scan# 2592
Delta R.T. -0.006 min
Lab File: BP008626.D
Acq: 31 Dec 2021 01:32

Tgt Ion:149 Resp: 1264576
Ion Ratio Lower Upper
149 100
150 9.0 7.9 11.9
104 4.3 3.7 5.5


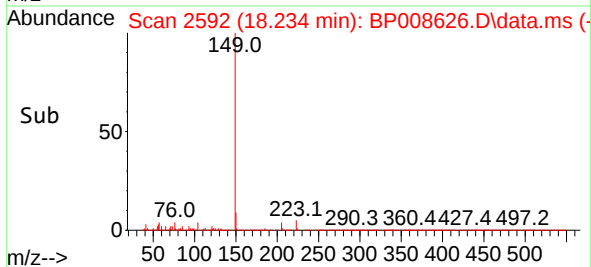
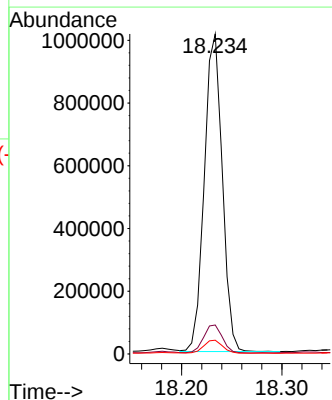
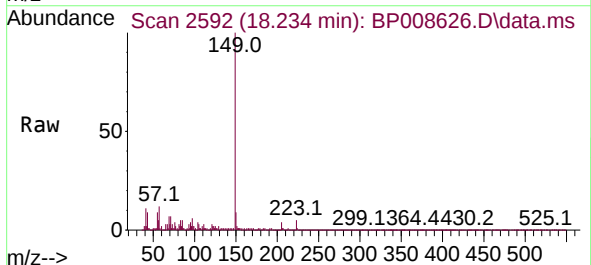




#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.357 min Scan# 31
Delta R.T. -0.006 min
Lab File: BP008626.D
Acq: 31 Dec 2021 01:32




Instrument :
BNA_P
ClientSampleId :
CONC-11E


Tgt Ion:240 Resp: 4760676
Ion Ratio Lower Upper
240 100
120 9.0 7.7 11.5
236 26.4 21.2 31.8

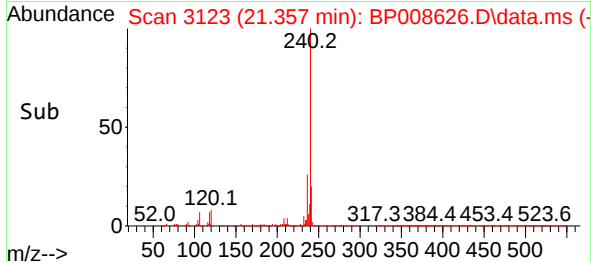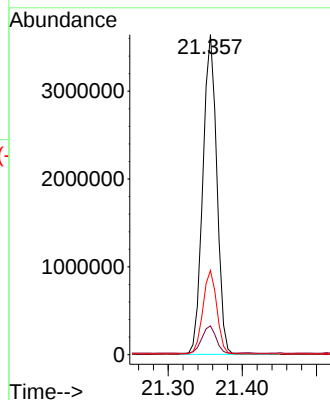

#79
Terphenyl-d14
Concen: 56.568 ng
RT: 19.828 min Scan# 2863
Delta R.T. 0.001 min
Lab File: BP008626.D
Acq: 31 Dec 2021 01:32

Tgt Ion:244 Resp:13189470
Ion Ratio Lower Upper
244 100
212 9.4 6.5 9.7
122 11.7 9.2 13.8


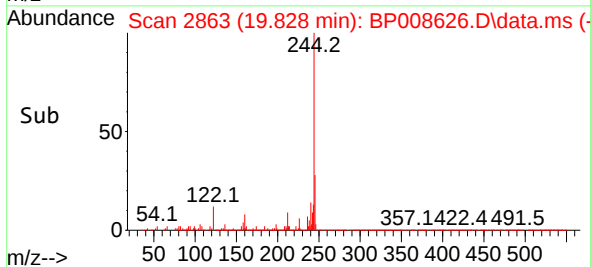
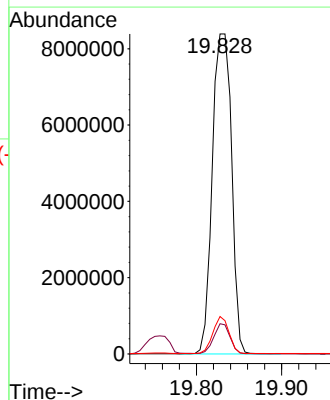
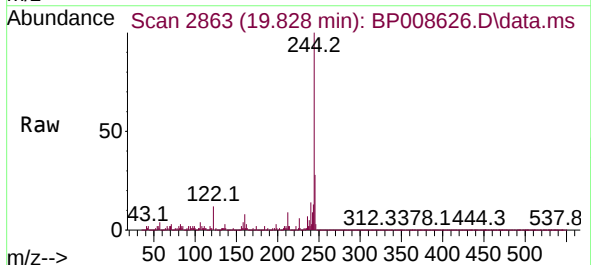




#80
Butylbenzylphthalate
Concen: 17.452 ng
RT: 20.510 min Scan# 2979
Delta R.T. 0.000 min
Lab File: BP008626.D
Acq: 31 Dec 2021 01:32




Instrument :
BNA_P
ClientSampleId :
CONC-11E


Tgt Ion:149 Resp: 2155883
Ion Ratio Lower Upper
149 100
91 56.5 50.6 76.0
206 26.2 19.7 29.5

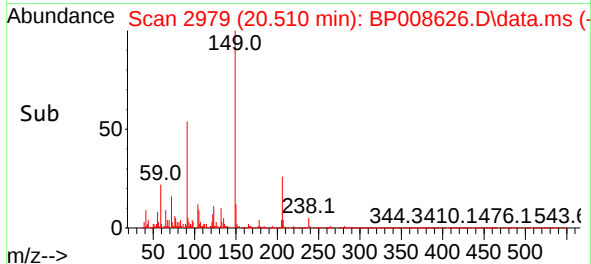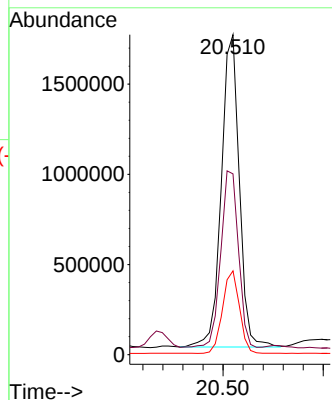

#84
Bis(2-ethylhexyl)phthalate
Concen: 28.877 ng
RT: 21.275 min Scan# 3109
Delta R.T. -0.006 min
Lab File: BP008626.D
Acq: 31 Dec 2021 01:32

Tgt Ion:149 Resp: 5388717
Ion Ratio Lower Upper
149 100
167 30.5 25.0 37.4
279 6.6 4.8 7.2


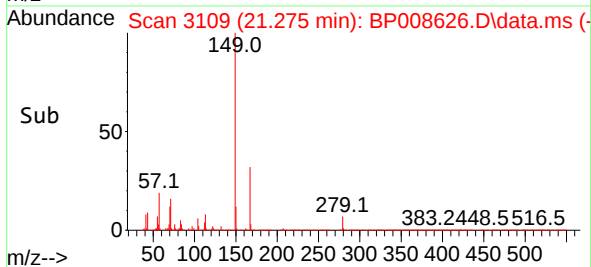
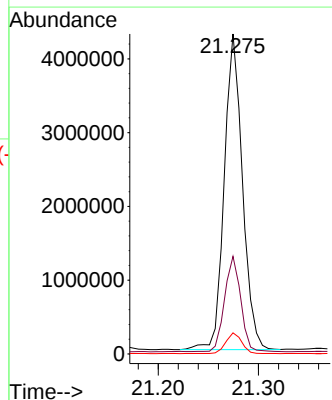
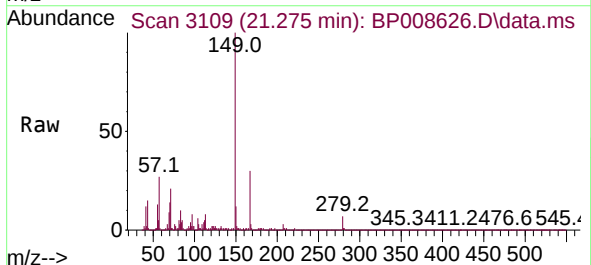




#85
Di-n-octyl phthalate
Concen: 4.065 ng
RT: 22.210 min Scan# 31
Delta R.T. -0.006 min
Lab File: BP008626.D
Acq: 31 Dec 2021 01:32

Instrument :
BNA_P
ClientSampleId :
CONC-11E

Tgt Ion:149 Resp: 1174231
Ion Ratio Lower Upper
149 100
167 0.0 1.4 2.0#
43 3.7 5.4 8.2#

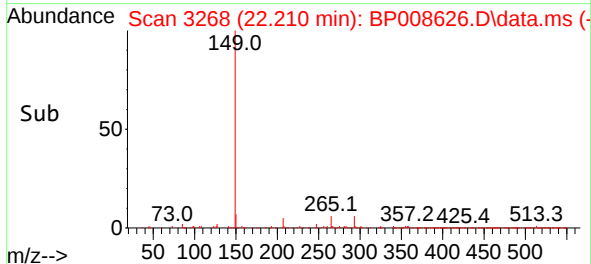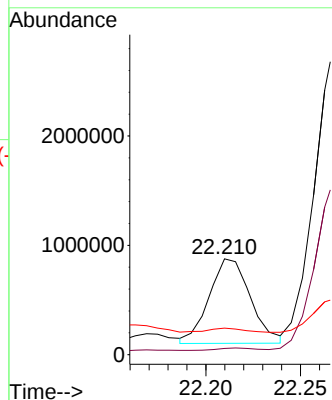

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.780 min Scan# 3535
Delta R.T. -0.006 min
Lab File: BP008626.D
Acq: 31 Dec 2021 01:32

Tgt Ion:264 Resp: 4600016
Ion Ratio Lower Upper
264 100
260 24.2 19.1 28.7
265 22.2 17.1 25.7

