

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123021\
 Data File : BP008602.D
 Acq On : 30 Dec 2021 10:17
 Operator : CG/JU
 Sample : PB141727BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB141727BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008602.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.469	415	422	436	rBV	10488093	15911135	36.59%	8.974%
2	7.058	684	692	708	rBV	9622446	16299942	37.48%	9.193%
3	7.893	827	834	843	rBV	2092788	3340072	7.68%	1.884%
4	9.052	1021	1031	1041	rBV	6335613	10658958	24.51%	6.012%
5	10.693	1302	1310	1319	rBV	2688921	4769845	10.97%	2.690%
6	13.157	1721	1729	1740	rBV	18573716	28914996	66.49%	16.308%
7	14.528	1953	1962	1972	rBV	4489867	6877596	15.81%	3.879%
8	16.010	2207	2214	2233	rBV	14335144	20627863	47.43%	11.634%
9	17.275	2421	2429	2436	rBV	5863556	8467376	19.47%	4.776%
10	19.833	2858	2864	2869	rBV	33049685	43490386	100.00%	24.529%
11	21.351	3117	3122	3133	rVB	7121373	9075559	20.87%	5.119%
12	23.780	3527	3535	3547	rVB	4344538	8866491	20.39%	5.001%




Sum of corrected areas: 177300219

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123021\
Data File : BP008602.D
Acq On : 30 Dec 2021 10:17
Operator : CG/JU
Sample : PB141727BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141727BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

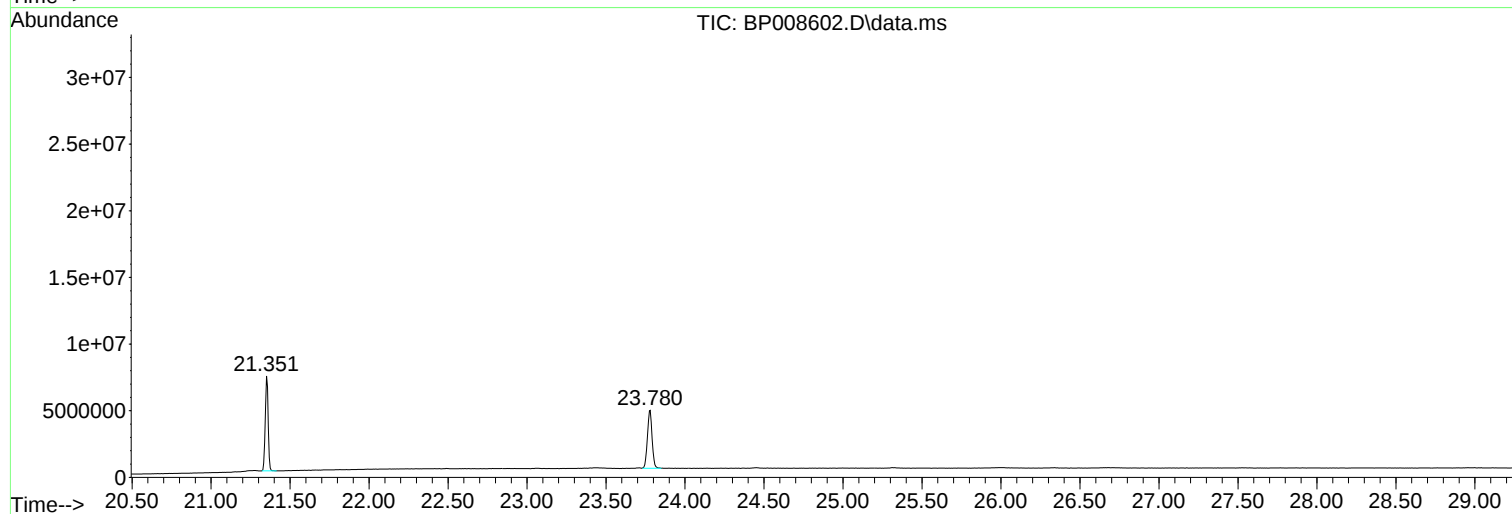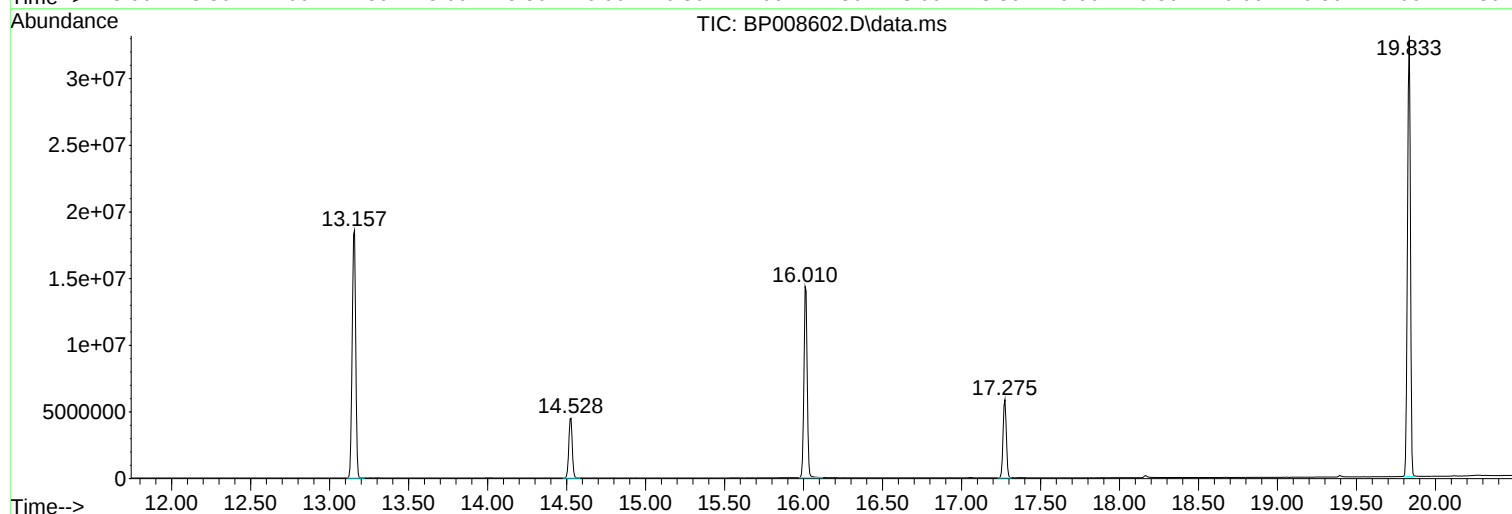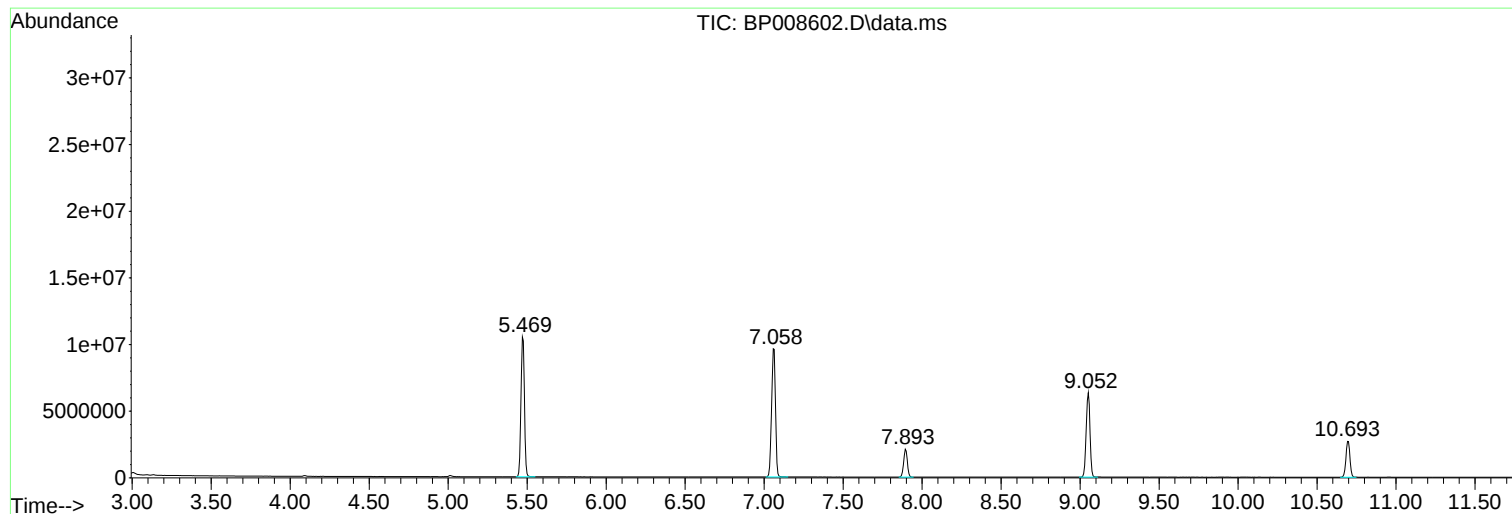

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123021\
Data File : BP008602.D
Acq On : 30 Dec 2021 10:17
Operator : CG/JU
Sample : PB141727BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141727BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123021\
Data File : BP008602.D
Acq On : 30 Dec 2021 10:17
Operator : CG/JU
Sample : PB141727BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141727BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------