

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP123021\  
 Data File : BP008614.D  
 Acq On : 30 Dec 2021 18:35  
 Operator : CG/JU  
 Sample : PB141733BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 PB141733BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP122821.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008614.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.469       | 415           | 422         | 437          | rBV      | 5561060        | 8638701       | 25.56%          | 7.224%        |
| 2         | 7.057       | 683           | 692         | 701          | rBV      | 5761813        | 9248546       | 27.36%          | 7.734%        |
| 3         | 7.893       | 827           | 834         | 842          | rBV      | 1055065        | 1725928       | 5.11%           | 1.443%        |
| 4         | 9.046       | 1022          | 1030        | 1042         | rBV      | 3479173        | 5778182       | 17.10%          | 4.832%        |
| 5         | 10.693      | 1301          | 1310        | 1323         | rBV      | 1541965        | 2667142       | 7.89%           | 2.230%        |
| 6         | 13.151      | 1718          | 1728        | 1737         | rBV      | 11513841       | 17005443      | 50.31%          | 14.220%       |
| 7         | 14.522      | 1954          | 1961        | 1970         | rBV      | 2895471        | 4226294       | 12.50%          | 3.534%        |
| 8         | 16.010      | 2207          | 2214        | 2235         | rBV      | 9539823        | 13578128      | 40.17%          | 11.354%       |
| 9         | 17.269      | 2421          | 2428        | 2438         | rBV      | 4098615        | 5890876       | 17.43%          | 4.926%        |
| 10        | 19.827      | 2857          | 2863        | 2869         | rBV      | 26891172       | 33800316      | 100.00%         | 28.264%       |
| 11        | 21.351      | 3116          | 3122        | 3128         | rBV      | 6236723        | 7952831       | 23.53%          | 6.650%        |
| 12        | 23.774      | 3526          | 3534        | 3546         | rVB2     | 4404320        | 9076842       | 26.85%          | 7.590%        |




Sum of corrected areas: 119589229

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP123021\  
Data File : BP008614.D  
Acq On : 30 Dec 2021 18:35  
Operator : CG/JU  
Sample : PB141733BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB141733BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP122821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

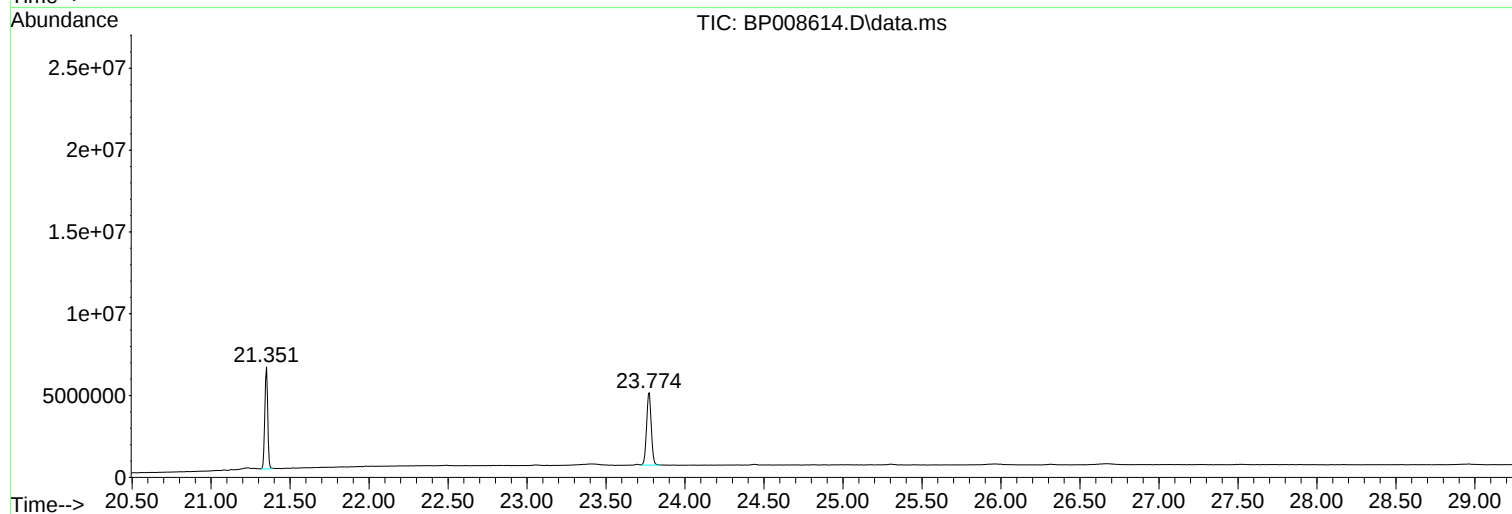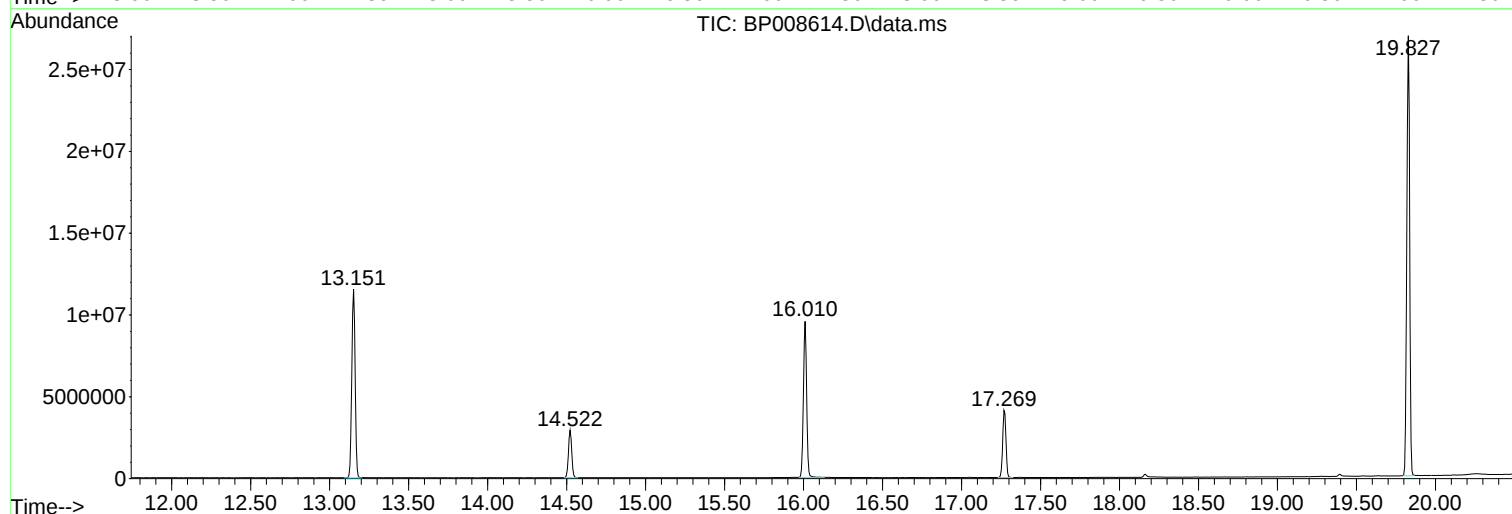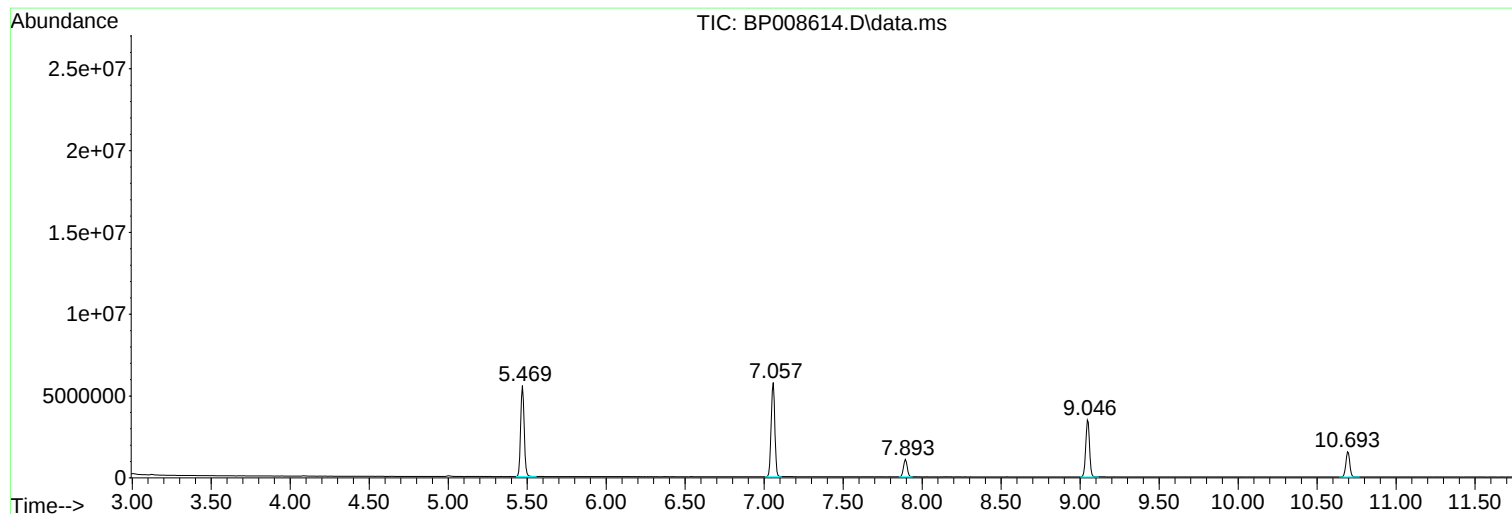

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP123021\  
Data File : BP008614.D  
Acq On : 30 Dec 2021 18:35  
Operator : CG/JU  
Sample : PB141733BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB141733BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP122821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP123021\  
Data File : BP008614.D  
Acq On : 30 Dec 2021 18:35  
Operator : CG/JU  
Sample : PB141733BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB141733BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP122821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|