


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123021\
 Data File : BP008600.D
 Acq On : 30 Dec 2021 09:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 30 08:44:33 2021

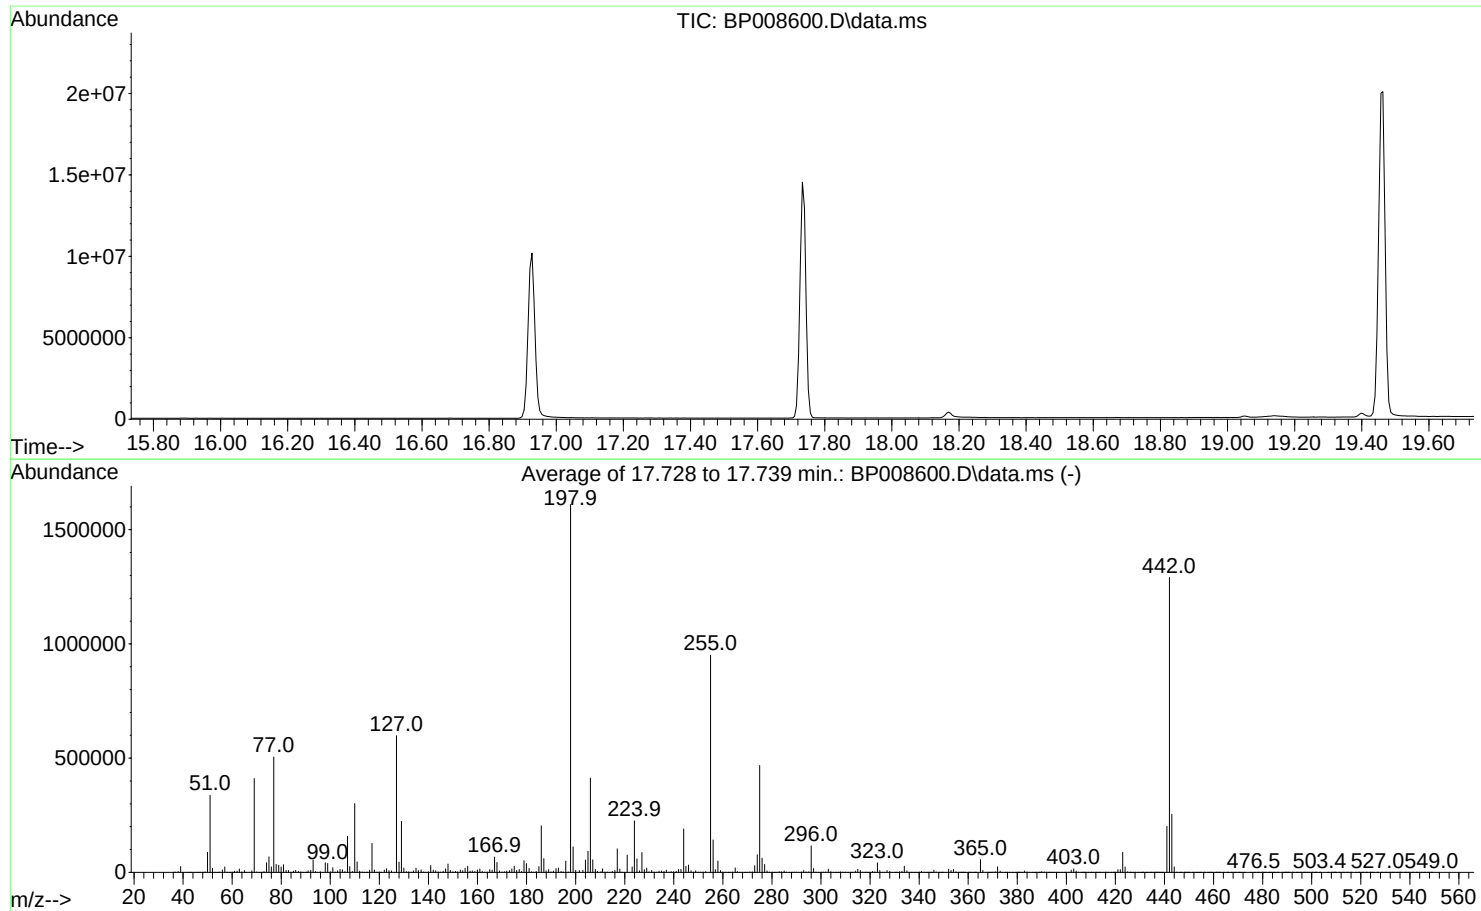

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.0	337931	PASS
68	69	0.00	2	1.8	7373	PASS
69	198	0.00	100	25.5	410317	PASS
70	69	0.00	2	0.6	2263	PASS
127	198	10	80	37.1	598187	PASS
197	198	0.00	2	0.1	2089	PASS
198	198	100	100	100.0	1610240	PASS
199	198	5	9	6.9	111291	PASS
275	198	10	60	29.1	467840	PASS
365	198	1	100	3.5	55819	PASS
441	198	0.01	100	12.5	201852	PASS
442	442	100	100	100.0	1290709	PASS
443	442	15	24	19.7	254229	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/30/2021	BNA_P	<u>BP008600.D</u>
Compound Name	Response	Retention Time
DDT	5767012	20.669
DDD	55832	20.233
DDE	3500	19.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
59332	5826344	1.02

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123021\
 Data File : BP008600.D
 Acq On : 30 Dec 2021 09:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 31 06:51:17 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 08:44:33 2021
 Response via : Initial Calibration

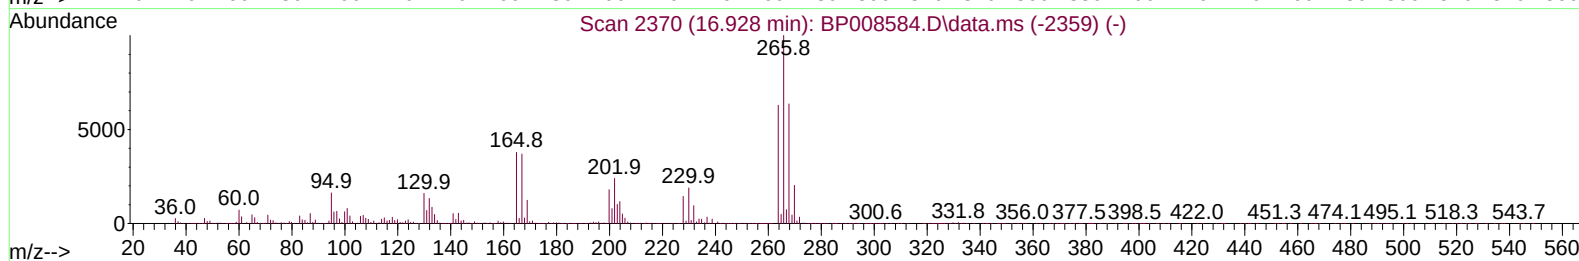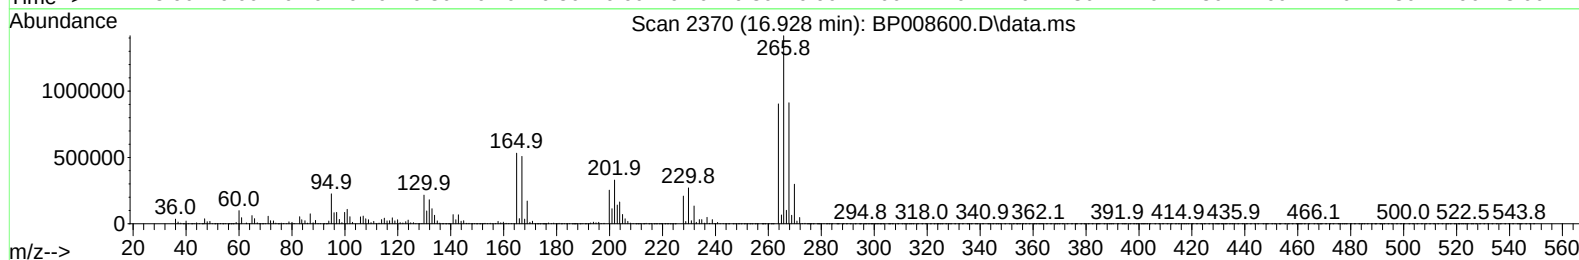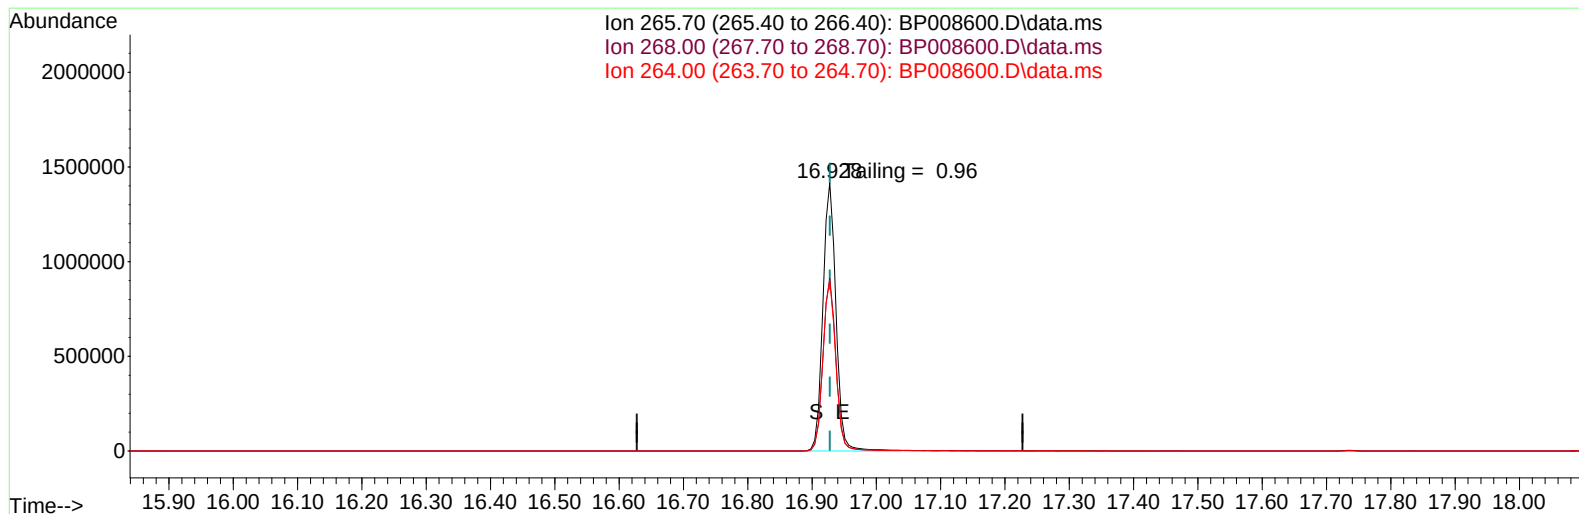

TIC: BP008600.D\data.ms

(70) Pentachlorophenol (C)

16.928min (+ 0.000) 252481.25 ng




response 2004097

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.32
264.00	62.90	63.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123021\
 Data File : BP008600.D
 Acq On : 30 Dec 2021 09:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 31 06:51:17 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 08:44:33 2021
 Response via : Initial Calibration

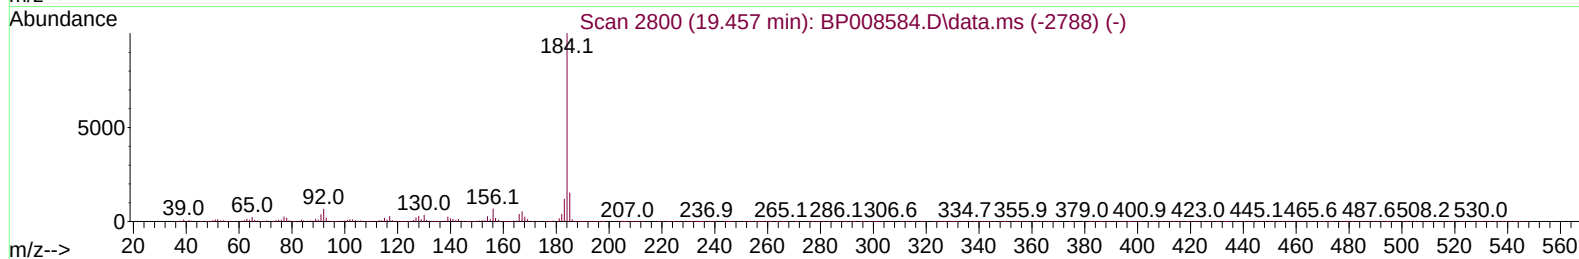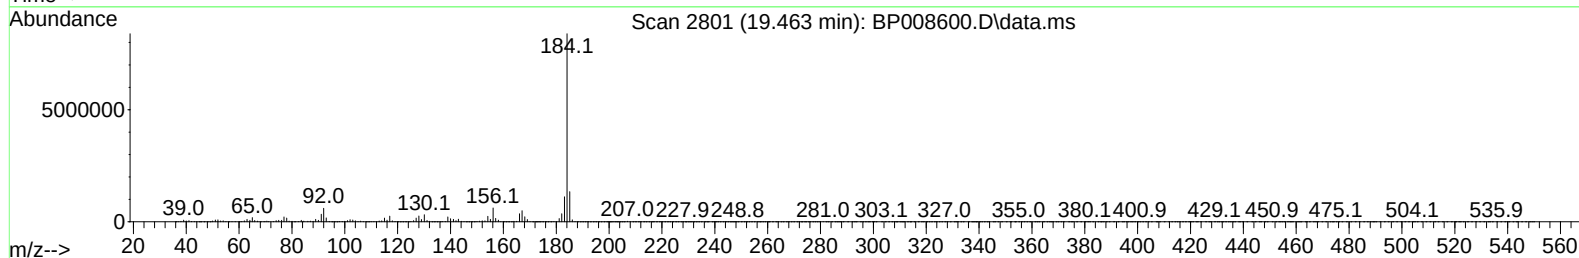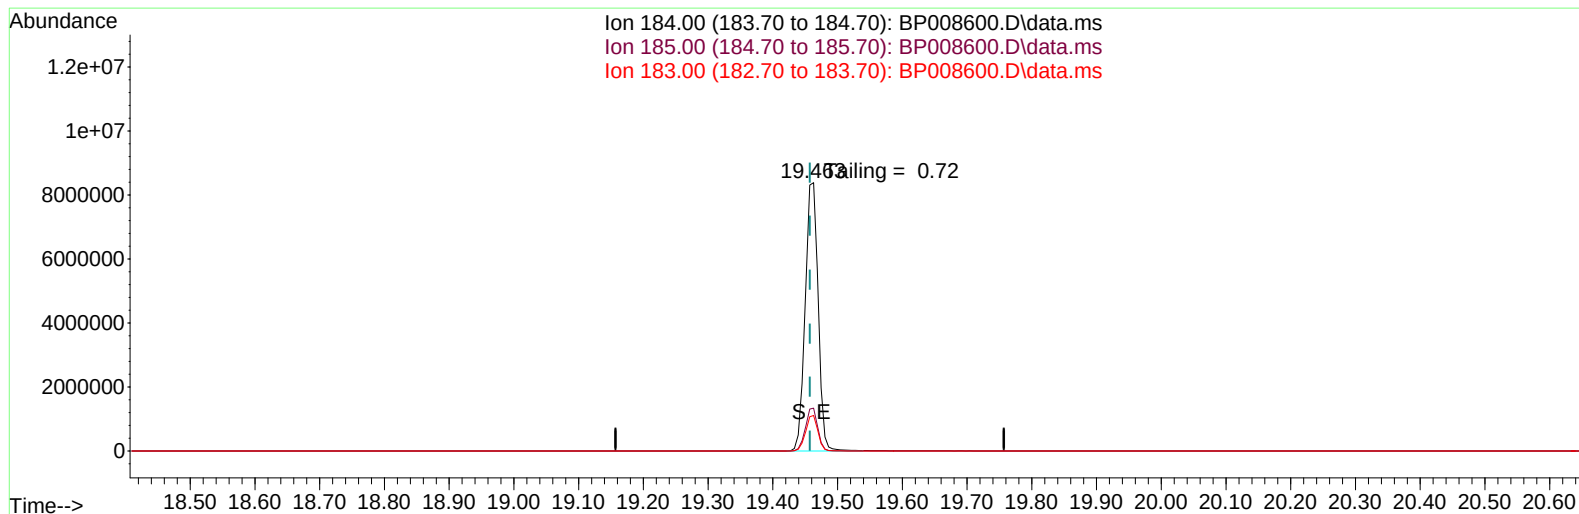

TIC: BP008600.D\data.ms

(77) Benzidine**19.463min (+ 0.006) 208075.99 ng****response 11739987**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.97
183.00	11.90	13.27
0.00	0.00	0.00