
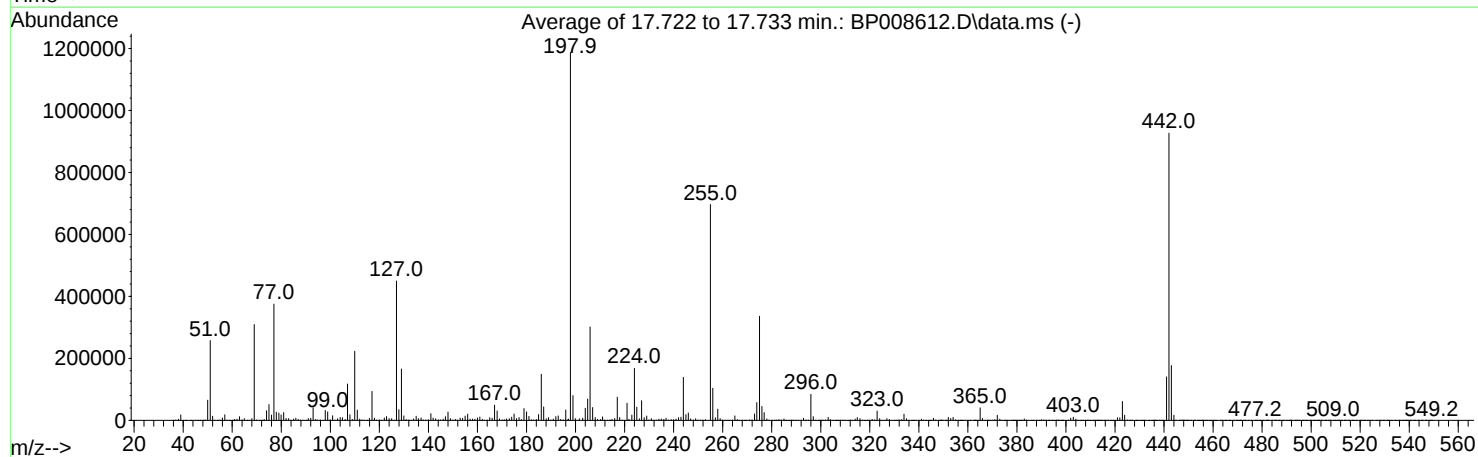


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123021\
 Data File : BP008612.D
 Acq On : 30 Dec 2021 16:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 30 08:44:33 2021

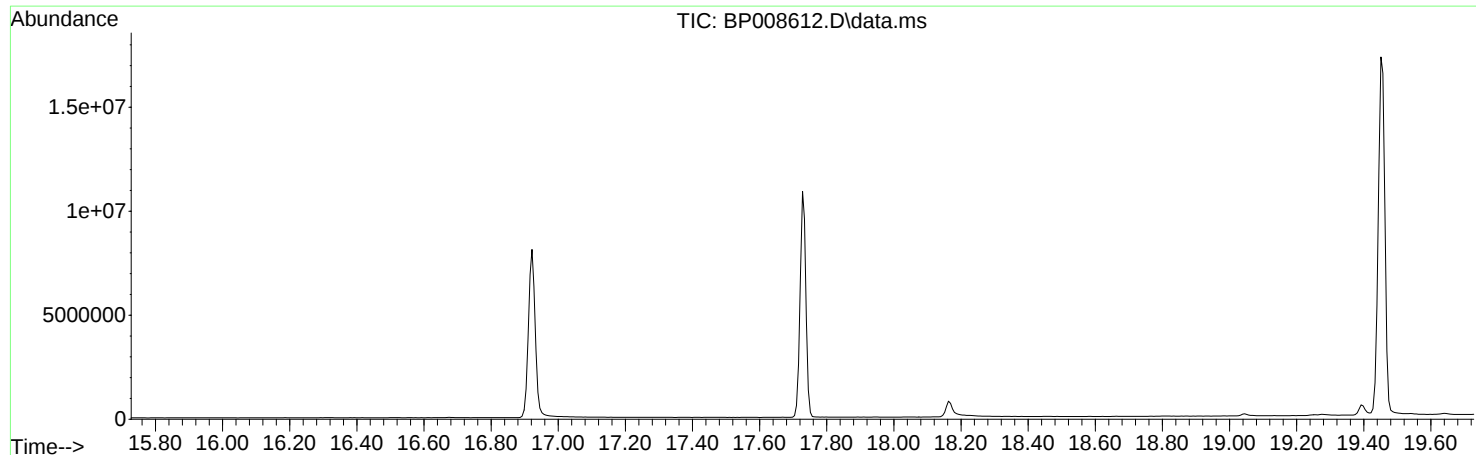

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.7	257734	PASS
68	69	0.00	2	1.8	5440	PASS
69	198	0.00	100	26.0	309260	PASS
70	69	0.00	2	0.6	1764	PASS
127	198	10	80	37.9	449727	PASS
197	198	0.00	2	0.3	3943	PASS
198	198	100	100	100.0	1187188	PASS
199	198	5	9	6.7	80015	PASS
275	198	10	60	28.3	336000	PASS
365	198	1	100	3.4	40322	PASS
441	198	0.01	100	11.8	140445	PASS
442	442	100	100	100.0	926775	PASS
443	442	15	24	19.1	176936	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/30/2021	BNA_P	<u>BP008612.D</u>
Compound Name	Response	Retention Time
DDT	4561759	20.663
DDD	93531	20.233
DDE	4796	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
98327	4660086	2.11

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123021\
 Data File : BP008612.D
 Acq On : 30 Dec 2021 16:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 31 07:02:54 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 08:44:33 2021
 Response via : Initial Calibration

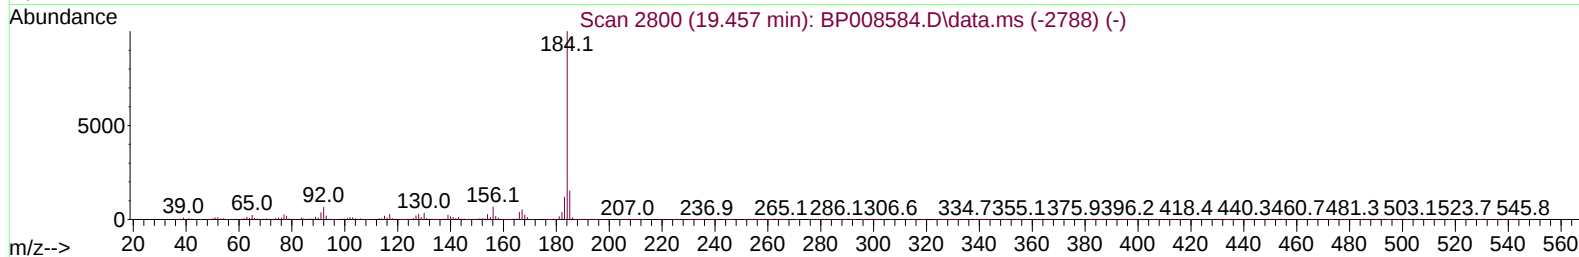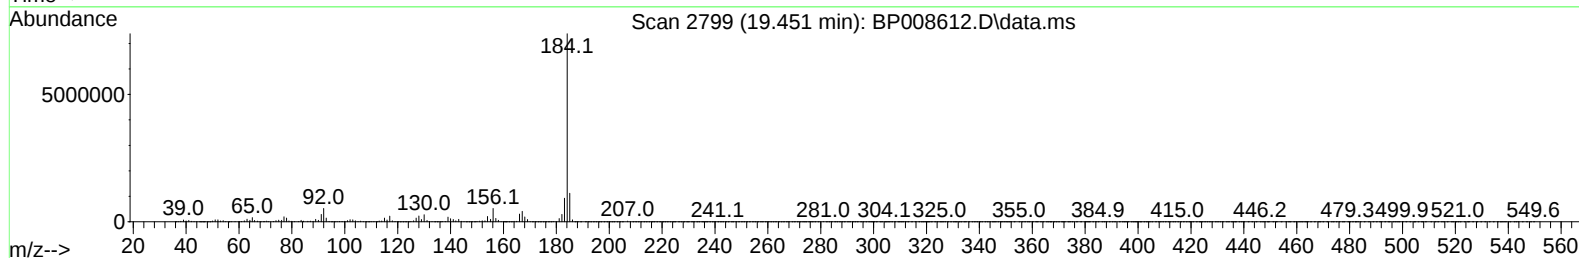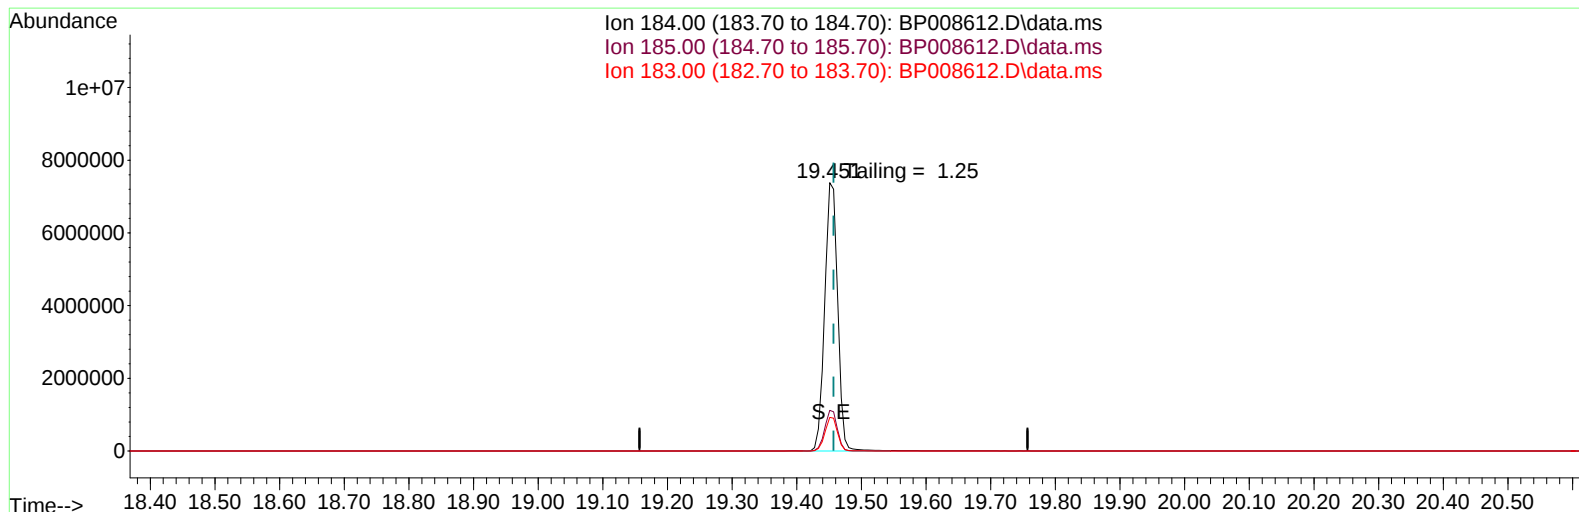

TIC: BP008612.D\data.ms

(77) Benzidine

19.451min (-0.006) 45209.96 ng




response 10325523

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.14
183.00	11.90	12.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123021\
 Data File : BP008612.D
 Acq On : 30 Dec 2021 16:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 31 07:02:54 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 08:44:33 2021
 Response via : Initial Calibration

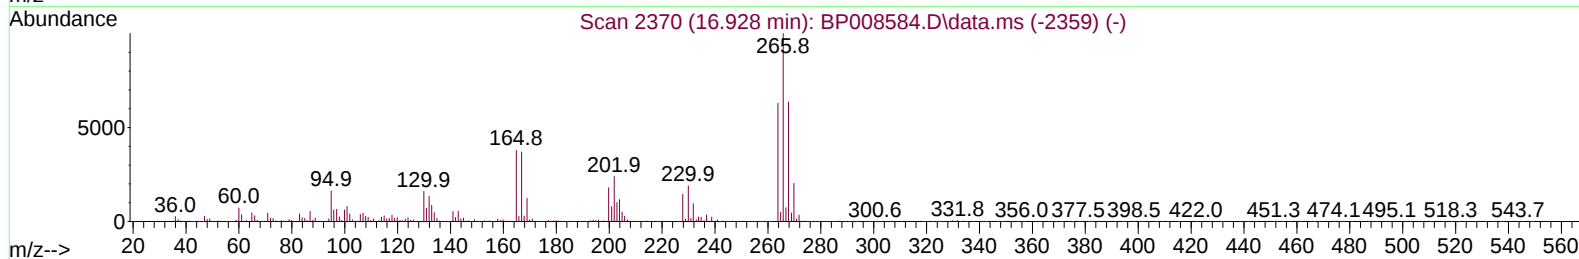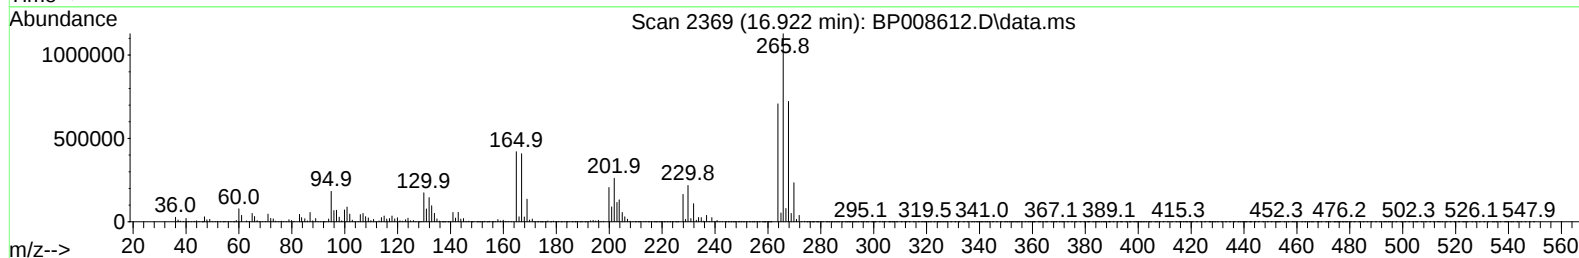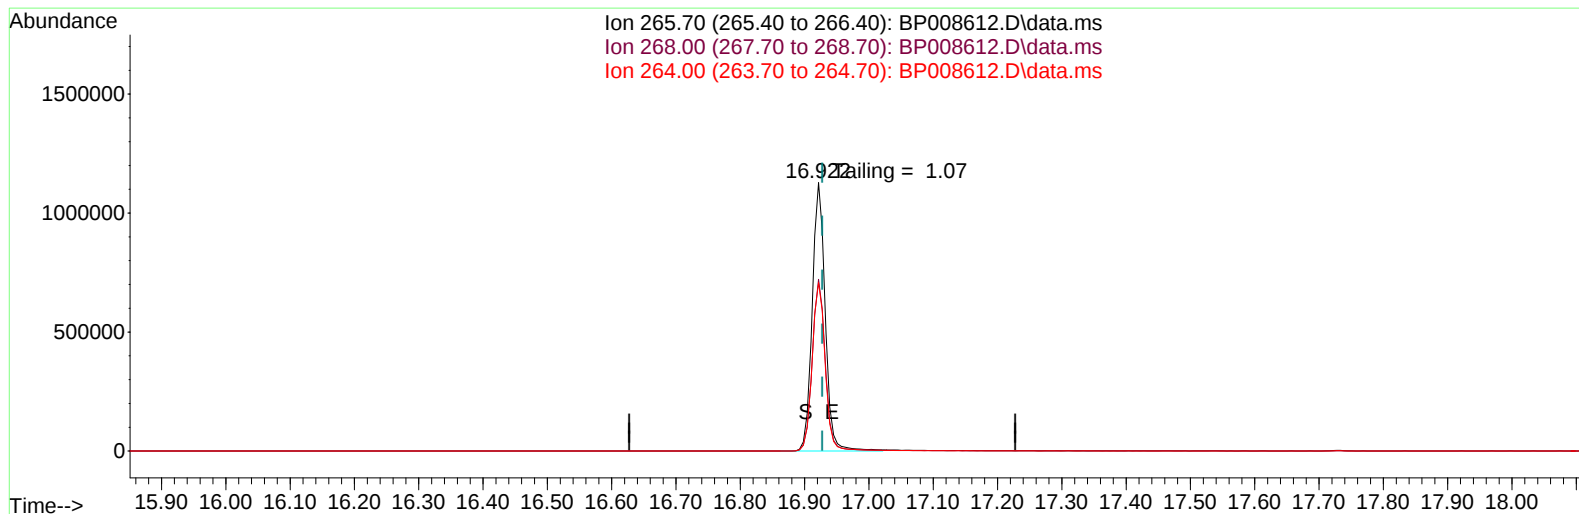

TIC: BP008612.D\data.ms

(70) Pentachlorophenol (C)

16.922min (-0.006) 108059.57 ng

response 1607165

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.96
264.00	62.90	62.71
0.00	0.00	0.00