
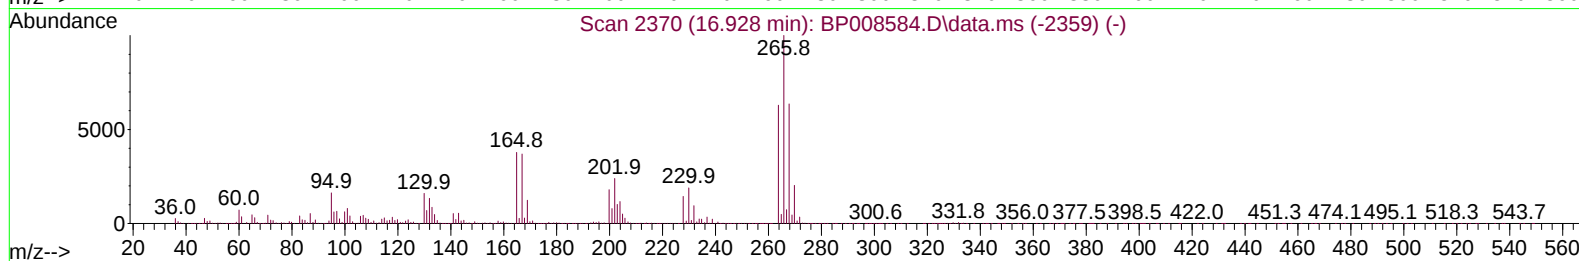
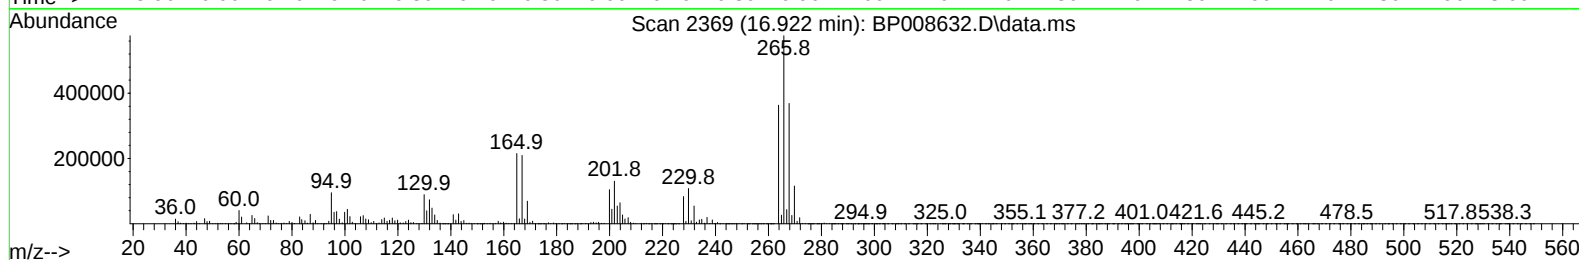


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010322\
Data File : BP008632.D
Acq On : 03 Jan 2022 11:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 14:13:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 08:44:33 2021
Response via : Initial Calibration

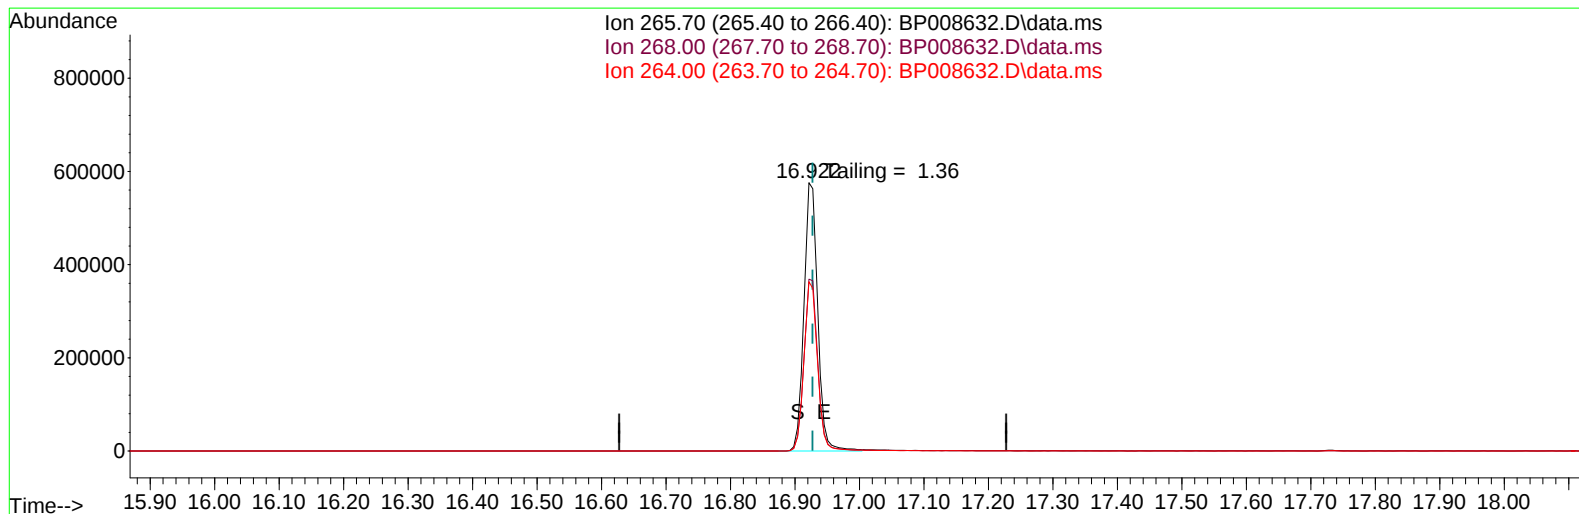

TIC: BP008632.D\data.ms

(70) Pentachlorophenol (C)

16.922min (-0.006) 601172.90 ng

response **862016**

Ion	Exp%	Act%
-----	------	------

265.70	100.00	100.00
--------	--------	--------




268.00	63.60	64.02
--------	-------	-------

264.00	62.90	63.10
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010322\
 Data File : BP008632.D
 Acq On : 03 Jan 2022 11:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 14:13:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 08:44:33 2021
 Response via : Initial Calibration

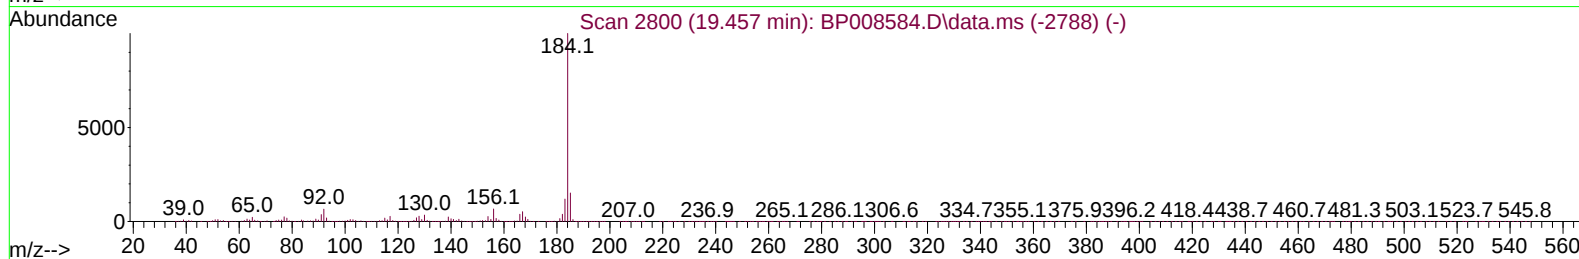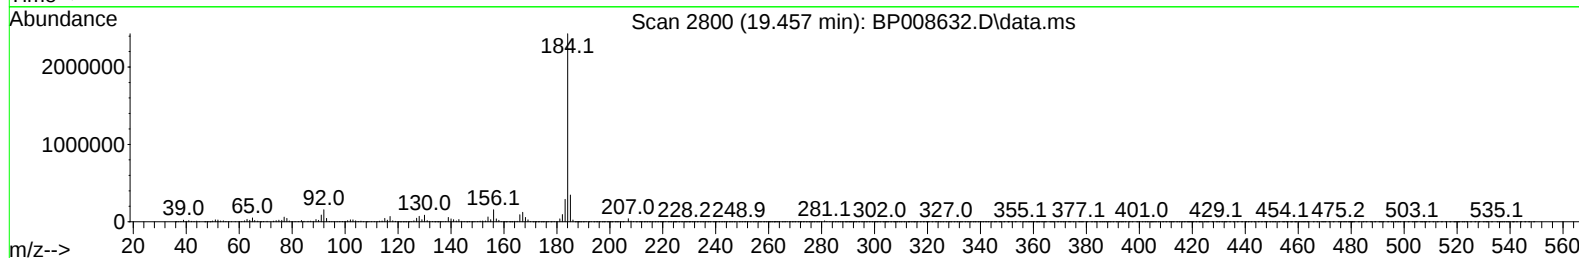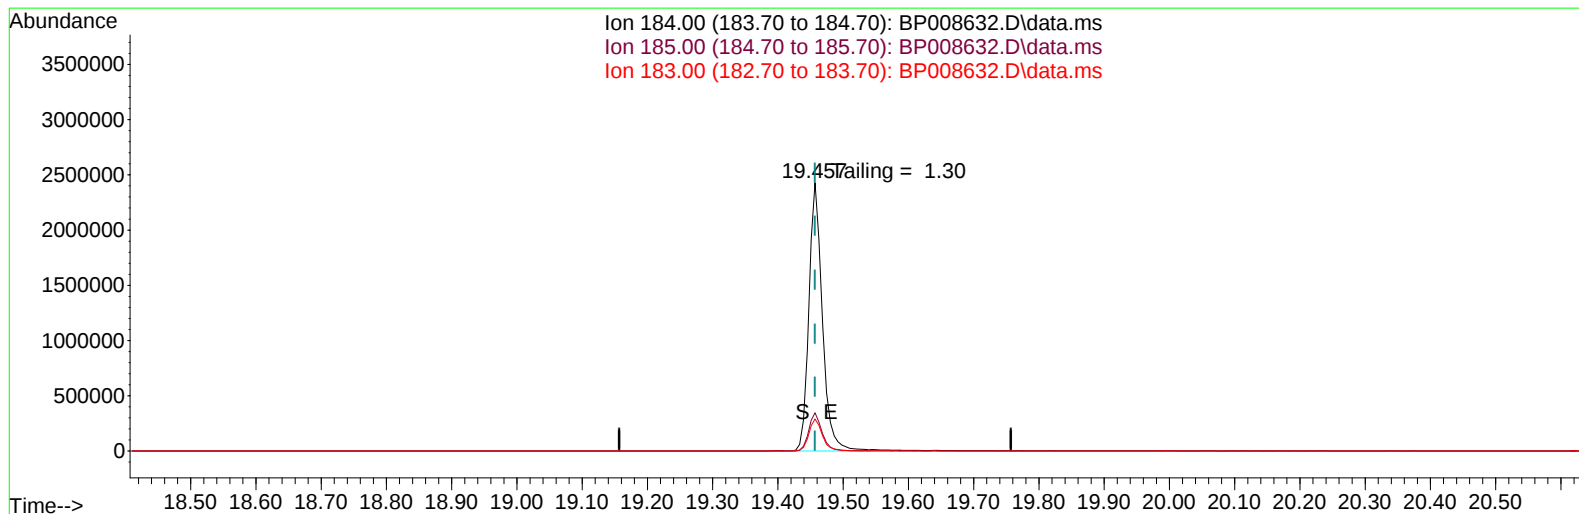

TIC: BP008632.D\data.ms

(77) Benzidine**19.457min (-0.000) 321509.22 ng****response 3525627**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.26
183.00	11.90	11.96
0.00	0.00	0.00