
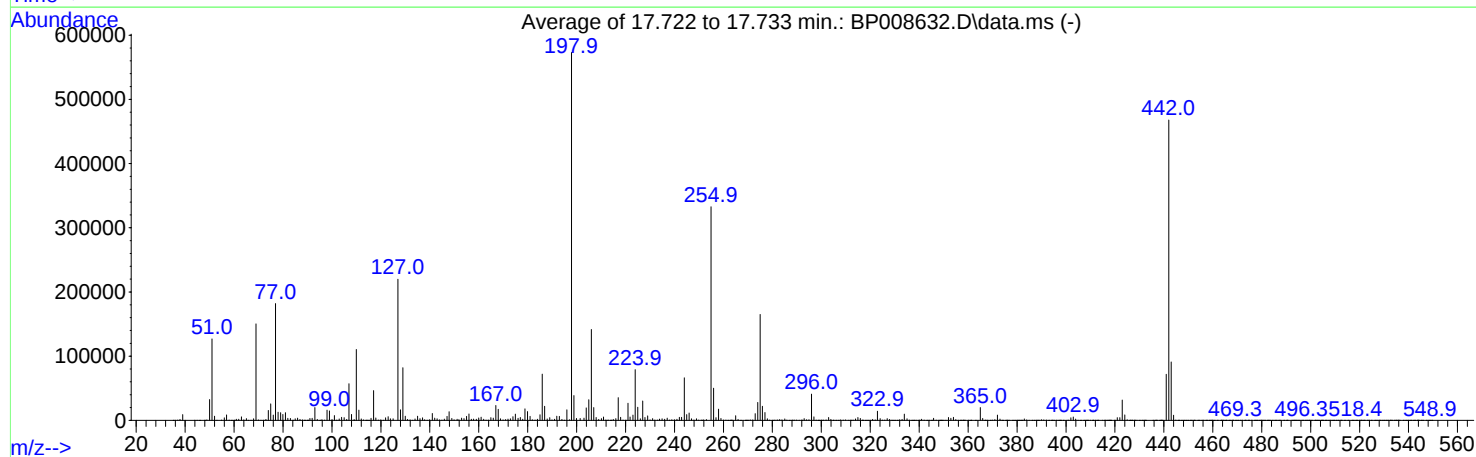


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010322\
 Data File : BP008632.D
 Acq On : 03 Jan 2022 11:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 30 08:44:33 2021

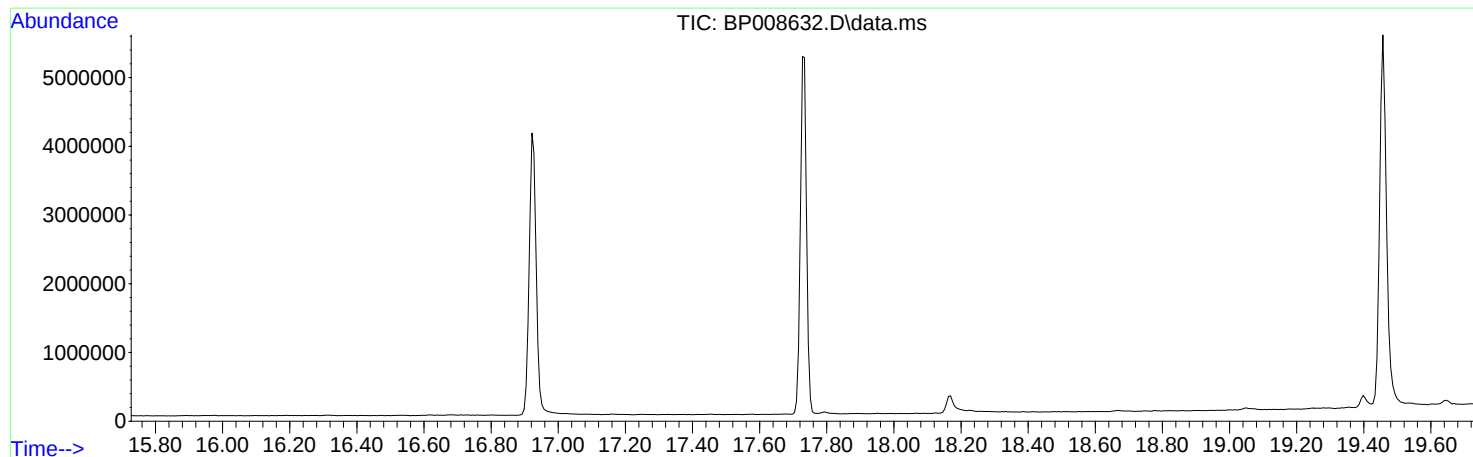




AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.2	126957	PASS
68	69	0.00	2	1.6	2432	PASS
69	198	0.00	100	26.2	150329	PASS
70	69	0.00	2	0.6	850	PASS
127	198	10	80	38.4	219800	PASS
197	198	0.00	2	0.2	1089	PASS
198	198	100	100	100.0	573039	PASS
199	198	5	9	6.7	38666	PASS
275	198	10	60	28.8	164975	PASS
365	198	1	100	3.5	20008	PASS
441	198	0.01	100	12.5	71786	PASS
442	442	100	100	100.0	467883	PASS
443	442	15	24	19.4	90941	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010322\
 Data File : BP008632.D
 Acq On : 03 Jan 2022 11:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 03 14:13:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 08:44:33 2021
 Response via : Initial Calibration

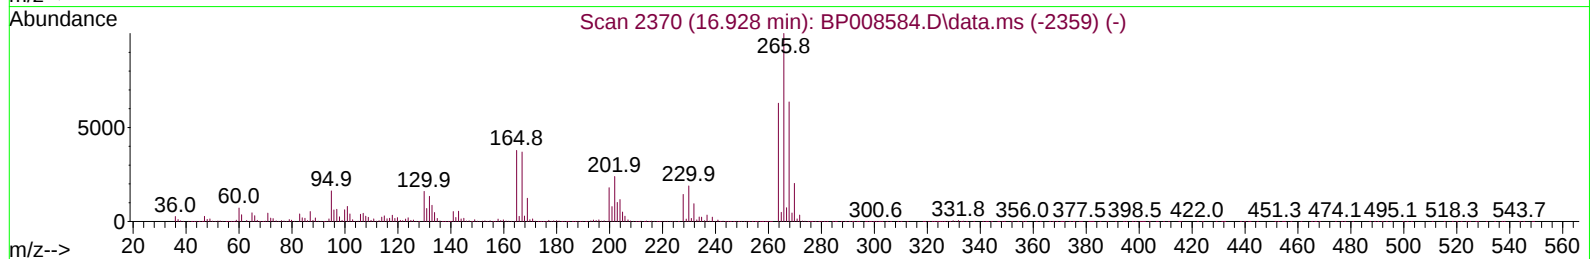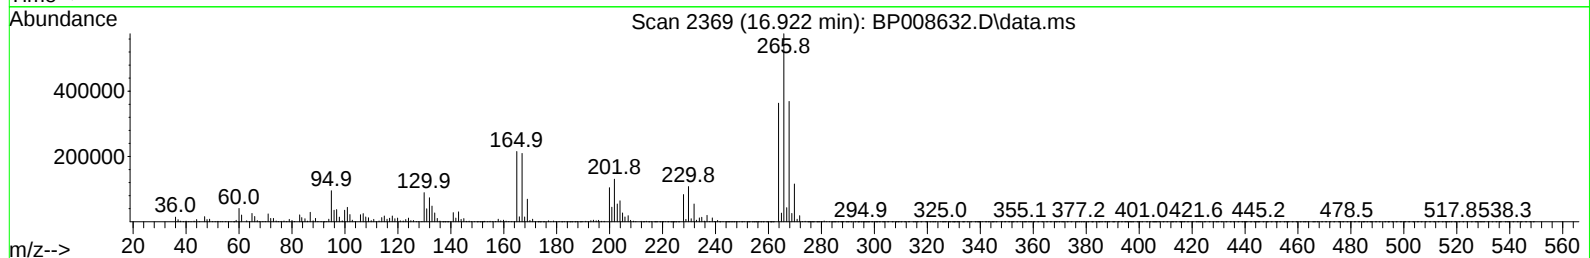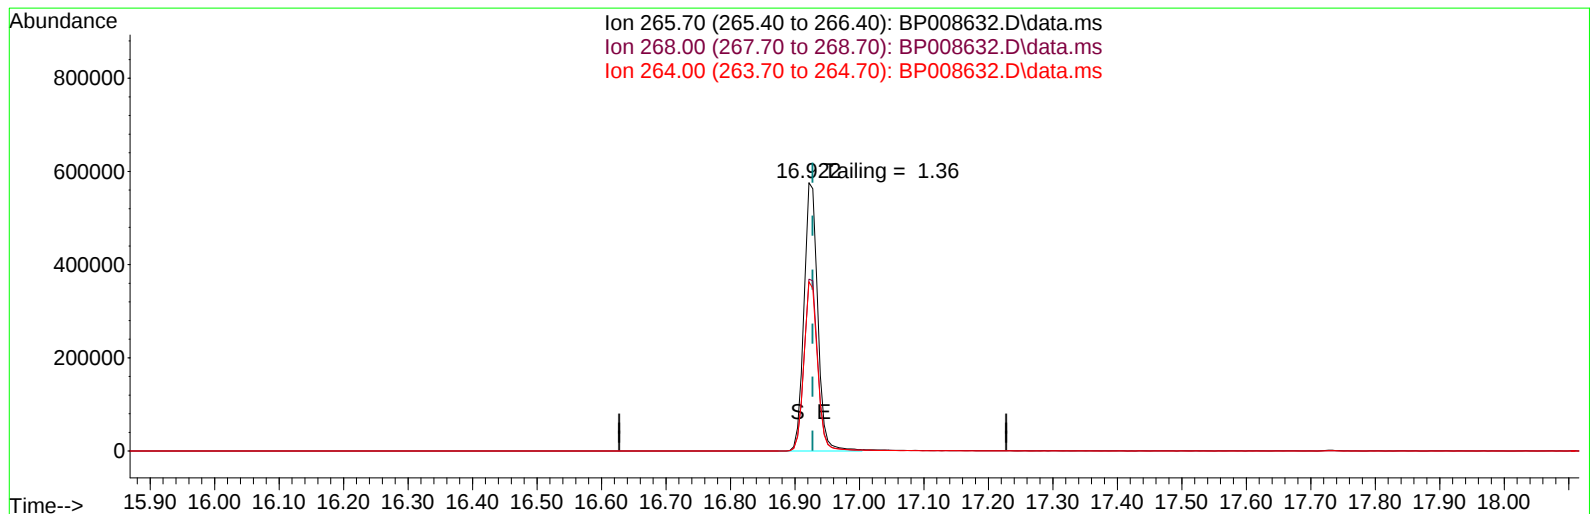

TIC: BP008632.D\data.ms

(70) Pentachlorophenol (C)

16.922min (-0.006) 601172.90 ng




response 862016

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.02
264.00	62.90	63.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010322\
Data File : BP008632.D
Acq On : 03 Jan 2022 11:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 03 14:13:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 08:44:33 2021
Response via : Initial Calibration

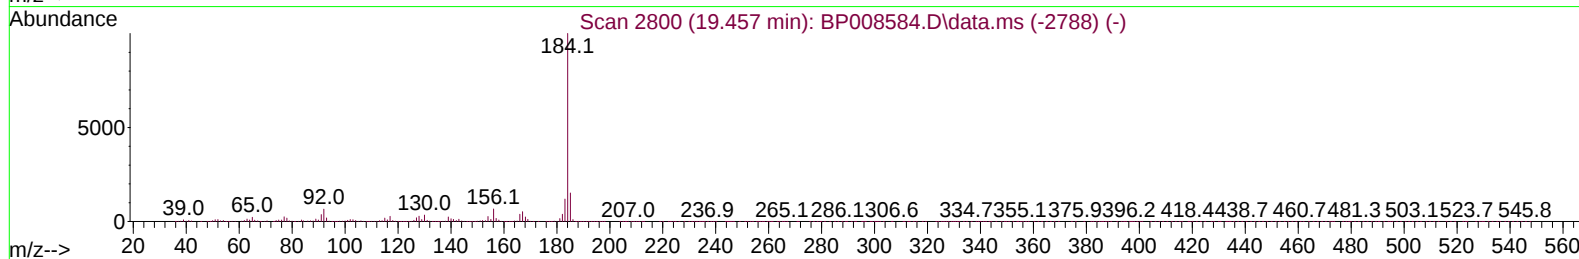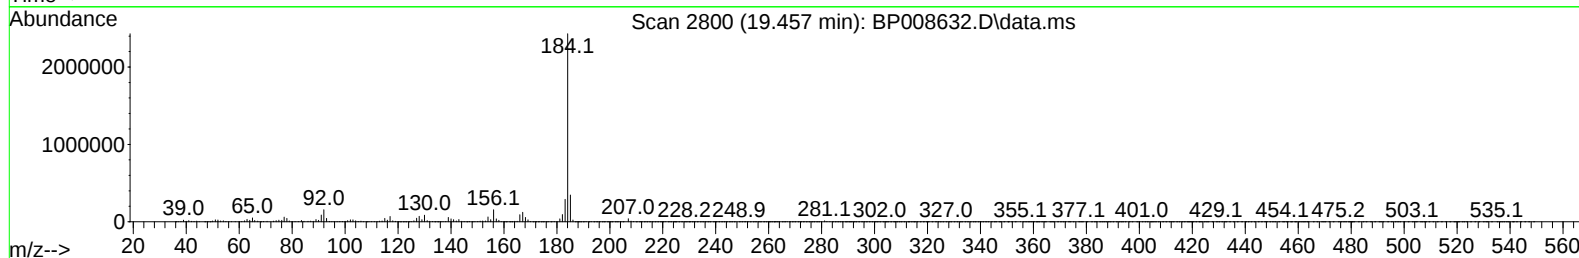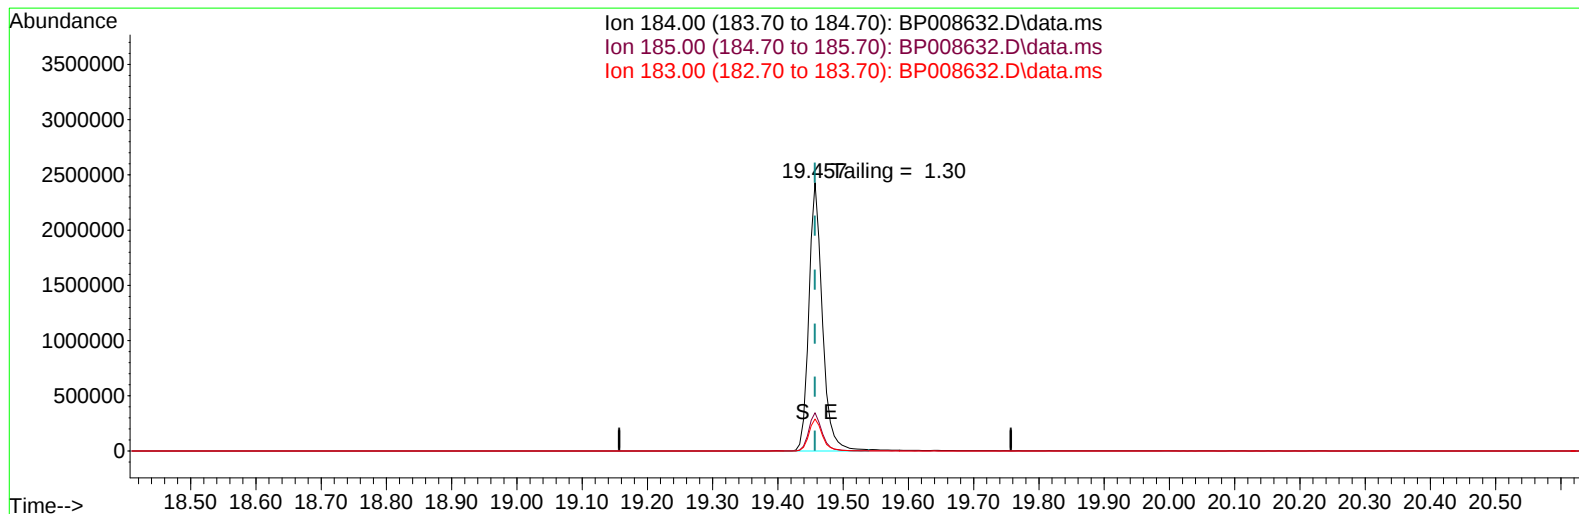

TIC: BP008632.D\data.ms

(77) Benzidine

19.457min (-0.000) 321509.22 ng

response 3525627

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.26
183.00	11.90	11.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/3/2022	BNA_P	<u>BP008632.D</u>
Compound Name	Response	Retention Time
DDT	1281916	20.66
DDD	402371	20.23
DDE	3135	19.74
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
405506	1687422	24.03

Instrument :
BNA_P
ClientSampleId :
DFTPP