

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010623\
 Data File : BP013403.D
 Acq On : 06 Jan 2023 10:27
 Operator : CG/JU
 Sample : PB150058BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK058

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013403.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.311	17	21	28	rVB	119902	145733	1.44%	0.147%
2	3.740	90	94	115	rBV	1440044	2151063	21.21%	2.168%
3	4.064	146	149	155	rVB	28650	41211	0.41%	0.042%
4	7.081	655	662	679	rBV	1581254	2452493	24.18%	2.472%
5	7.252	682	691	701	rBV	1346061	2069716	20.41%	2.086%
6	7.452	718	725	734	rBV	1636361	2521292	24.86%	2.541%
7	7.922	798	805	815	rVB	1446275	2214391	21.83%	2.232%
8	8.634	919	926	941	rBV	1847035	2919341	28.78%	2.942%
9	9.093	994	1004	1013	rBV	1491187	2400545	23.67%	2.419%
10	9.816	1119	1127	1136	rBV	1210975	1969221	19.42%	1.985%
11	10.352	1211	1218	1233	rBV	1848037	3054328	30.12%	3.078%
12	10.734	1275	1283	1292	rBV	1898052	3132773	30.89%	3.157%
13	10.875	1298	1307	1325	rBV	1773592	3083401	30.40%	3.108%
14	12.322	1546	1553	1563	rBV2	30953	59012	0.58%	0.059%
15	12.557	1586	1593	1597	rBV	12820	22615	0.22%	0.023%
16	13.975	1827	1834	1847	rBV	3473353	4804701	47.37%	4.842%
17	14.263	1875	1883	1900	rBV	3727787	5332628	52.58%	5.374%
18	14.569	1929	1935	1945	rBV	2948492	4228956	41.70%	4.262%
19	14.769	1962	1969	1990	rBV	1211991	1955458	19.28%	1.971%
20	15.563	2097	2104	2118	rBV	5101056	7113066	70.13%	7.169%
21	15.687	2118	2125	2136	rVV	1552377	2194343	21.64%	2.212%
22	15.804	2141	2145	2155	rVB4	25353	49611	0.49%	0.050%
23	16.351	2233	2238	2243	rBV8	7640	14954	0.15%	0.015%
24	16.992	2345	2347	2355	rVB8	8423	13262	0.13%	0.013%
25	17.328	2396	2404	2414	rBV	3600785	5253670	51.80%	5.295%
26	17.428	2414	2421	2440	rVV	5452771	7823267	77.14%	7.885%
27	19.239	2725	2729	2733	rVB3	68623	82336	0.81%	0.083%
28	19.304	2736	2740	2744	rBV2	63522	95884	0.95%	0.097%
29	19.657	2795	2800	2813	rBV	7433499	9715694	95.79%	9.792%
30	21.416	3094	3099	3112	rBV	4381139	5933830	58.51%	5.980%
31	23.716	3483	3490	3503	rBV2	4973365	10142199	100.00%	10.222%
32	23.874	3511	3517	3528	rVB2	3037194	6231138	61.44%	6.280%




Sum of corrected areas: 99222132

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010623\
Data File : BP013403.D
Acq On : 06 Jan 2023 10:27
Operator : CG/JU
Sample : PB150058BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

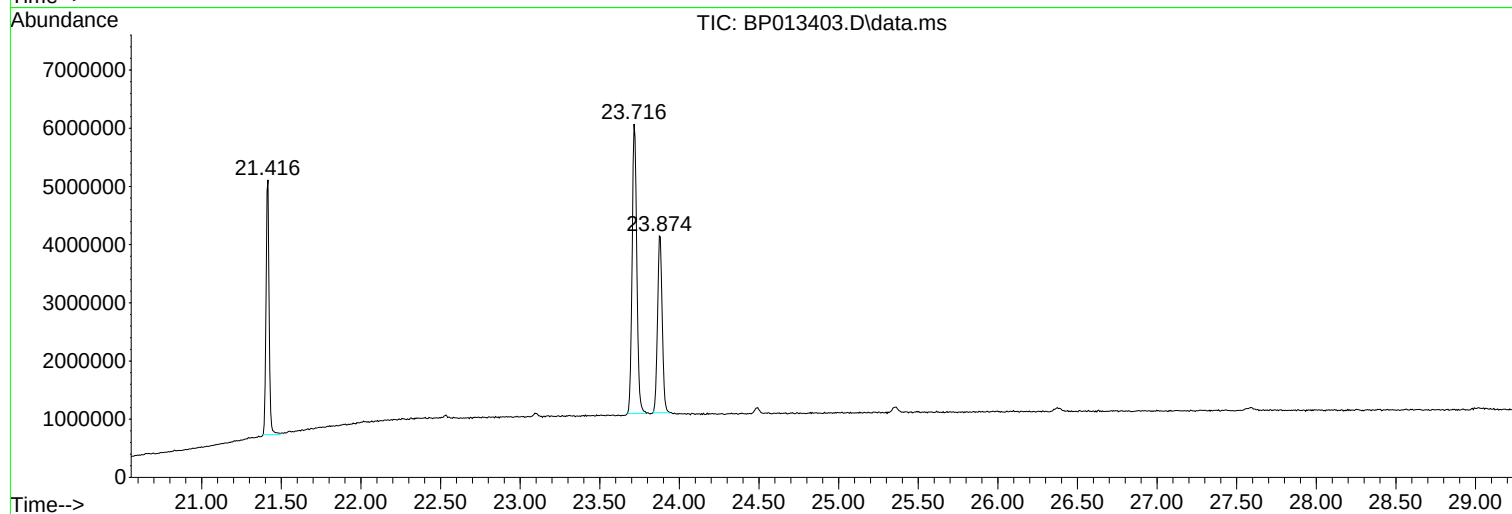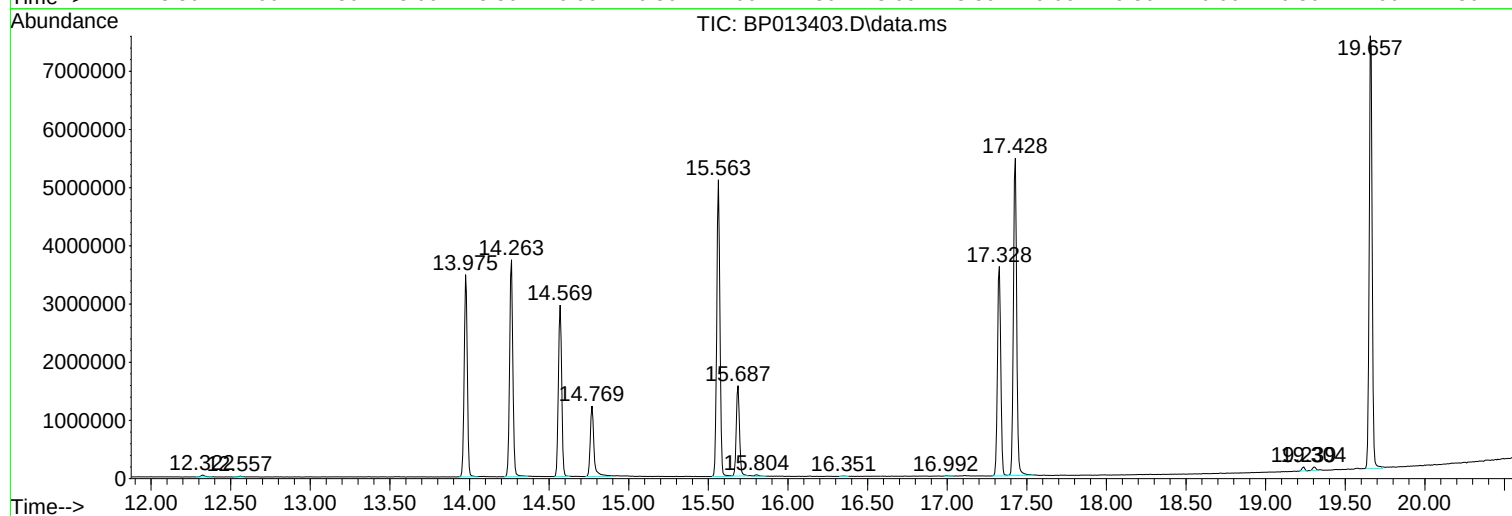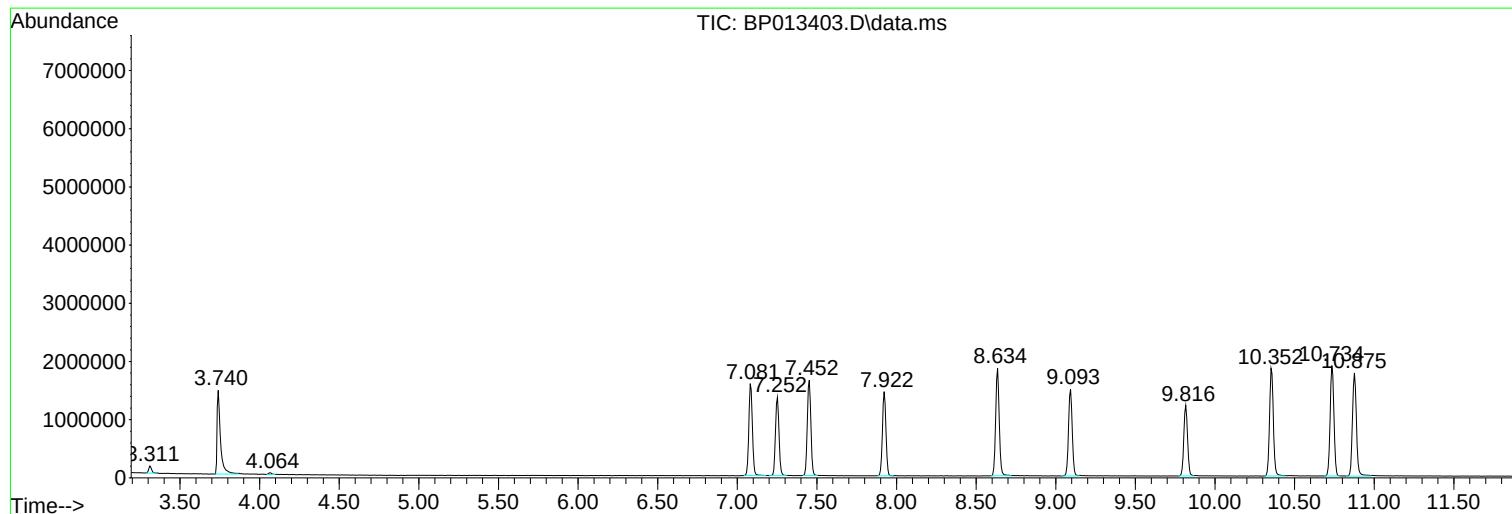

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010623\
Data File : BP013403.D
Acq On : 06 Jan 2023 10:27
Operator : CG/JU
Sample : PB150058BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010623\
Data File : BP013403.D
Acq On : 06 Jan 2023 10:27
Operator : CG/JU
Sample : PB150058BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc