

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010623\
 Data File : BP013405.D
 Acq On : 06 Jan 2023 12:01
 Operator : CG/JU
 Sample : PB150061BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK061

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013405.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.311	17	21	28	rVB	128586	158651	1.57%	0.160%
2	3.740	91	94	120	rBV	1540035	2309983	22.91%	2.323%
3	4.069	145	150	154	rBV	32532	48324	0.48%	0.049%
4	7.081	654	662	677	rBV	1675795	2599698	25.79%	2.614%
5	7.252	684	691	703	rVB	1379615	2136593	21.19%	2.148%
6	7.452	718	725	738	rVB	1729821	2663604	26.42%	2.678%
7	7.922	797	805	813	rBV	1562024	2372466	23.53%	2.386%
8	8.634	918	926	944	rBV	1922223	3077454	30.53%	3.094%
9	9.093	996	1004	1021	rBV	1523195	2453528	24.34%	2.467%
10	9.816	1118	1127	1136	rBV	1273699	2007145	19.91%	2.018%
11	10.357	1209	1219	1233	rBV	1859111	3131902	31.07%	3.149%
12	10.734	1276	1283	1291	rBV	1981634	3273030	32.47%	3.291%
13	10.875	1299	1307	1320	rBV	1831687	3119489	30.94%	3.137%
14	12.328	1547	1554	1561	rBV2	29247	52918	0.52%	0.053%
15	12.557	1587	1593	1599	rBV	14286	25730	0.26%	0.026%
16	13.975	1826	1834	1847	rBV	3428180	4709616	46.72%	4.736%
17	14.263	1876	1883	1893	rBV	3757973	5275888	52.33%	5.305%
18	14.569	1927	1935	1945	rBV	2970540	4313818	42.79%	4.338%
19	14.769	1962	1969	1988	rBV	1184727	1906969	18.92%	1.918%
20	15.563	2098	2104	2116	rBV	5053900	6982882	69.27%	7.021%
21	15.686	2119	2125	2140	rVV	1569125	2131084	21.14%	2.143%
22	15.804	2142	2145	2150	rVB	25757	33848	0.34%	0.034%
23	15.933	2162	2167	2171	rVB8	5476	10555	0.10%	0.011%
24	16.998	2346	2348	2353	rVB5	8241	10845	0.11%	0.011%
25	17.110	2364	2367	2375	rVB5	9184	15379	0.15%	0.015%
26	17.328	2396	2404	2411	rBV	3807983	5234663	51.93%	5.264%
27	17.428	2414	2421	2446	rVV2	5327735	7628285	75.67%	7.670%
28	19.239	2725	2729	2736	rVB3	60509	87224	0.87%	0.088%
29	19.304	2737	2740	2745	rVV	56275	75325	0.75%	0.076%
30	19.663	2795	2801	2810	rBV	7125258	9318136	92.43%	9.370%
31	21.416	3094	3099	3110	rBV	4418218	5927454	58.80%	5.960%
32	23.721	3484	3491	3506	rVB2	4985293	10081073	100.00%	10.137%
33	23.880	3512	3518	3529	rVB	3146387	6276712	62.26%	6.311%




Sum of corrected areas: 99450271

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010623\
Data File : BP013405.D
Acq On : 06 Jan 2023 12:01
Operator : CG/JU
Sample : PB150061BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK061

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

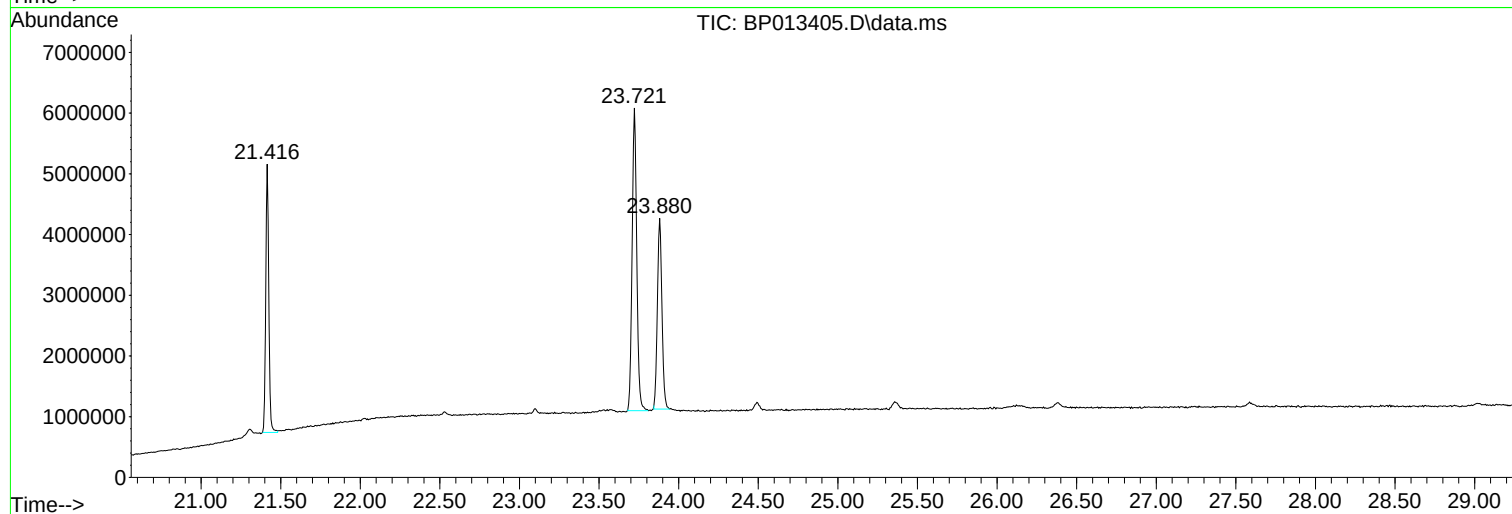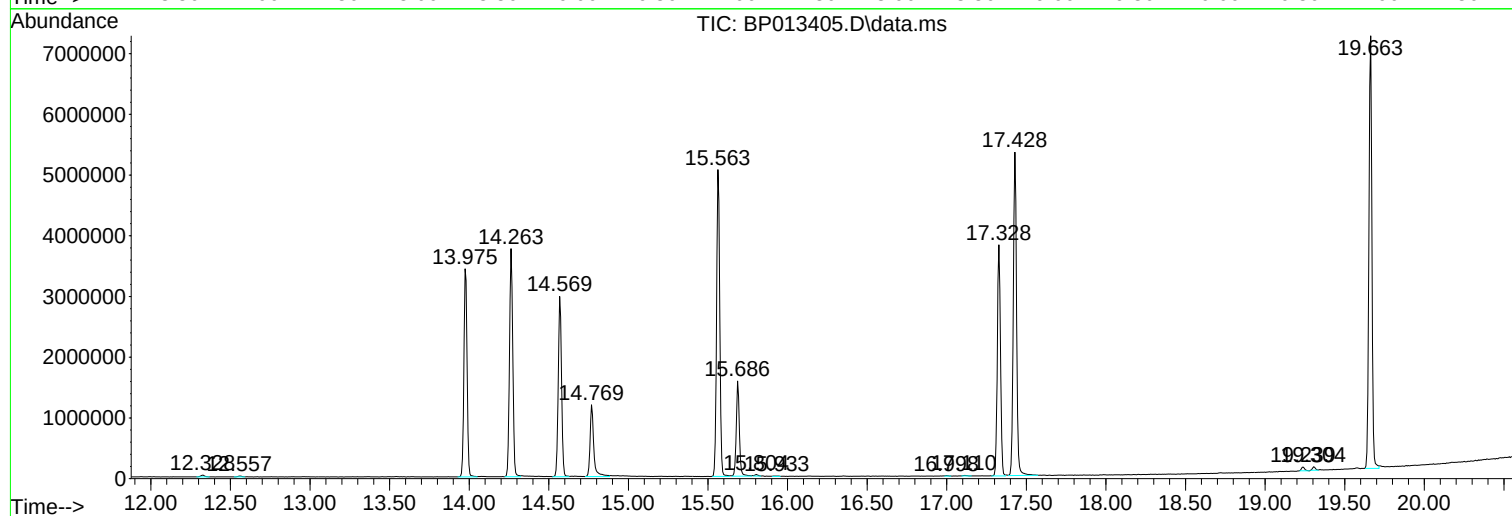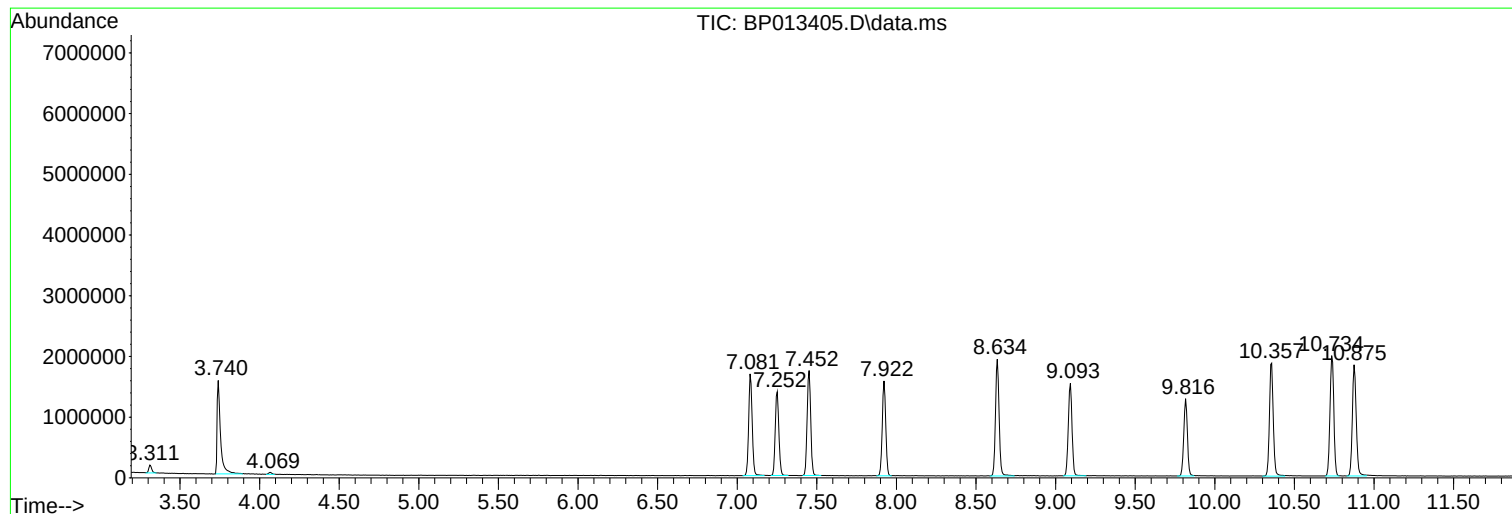

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010623\
Data File : BP013405.D
Acq On : 06 Jan 2023 12:01
Operator : CG/JU
Sample : PB150061BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK061

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010623\
Data File : BP013405.D
Acq On : 06 Jan 2023 12:01
Operator : CG/JU
Sample : PB150061BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK061

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------