
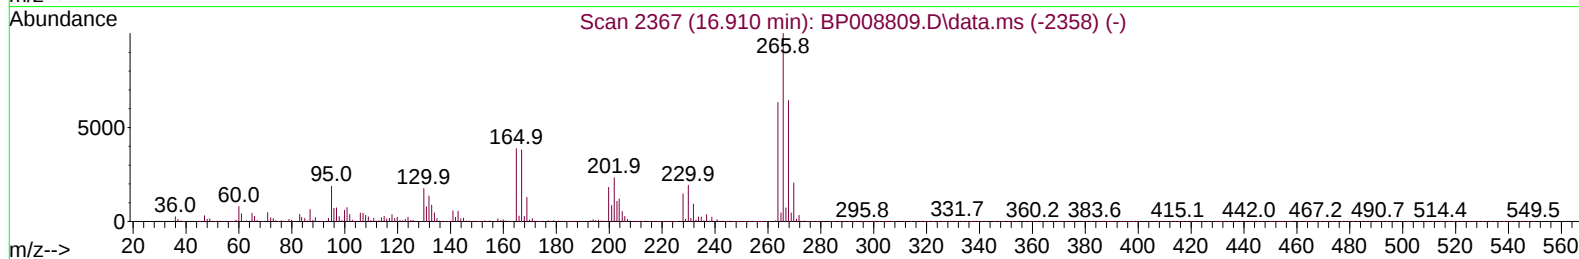
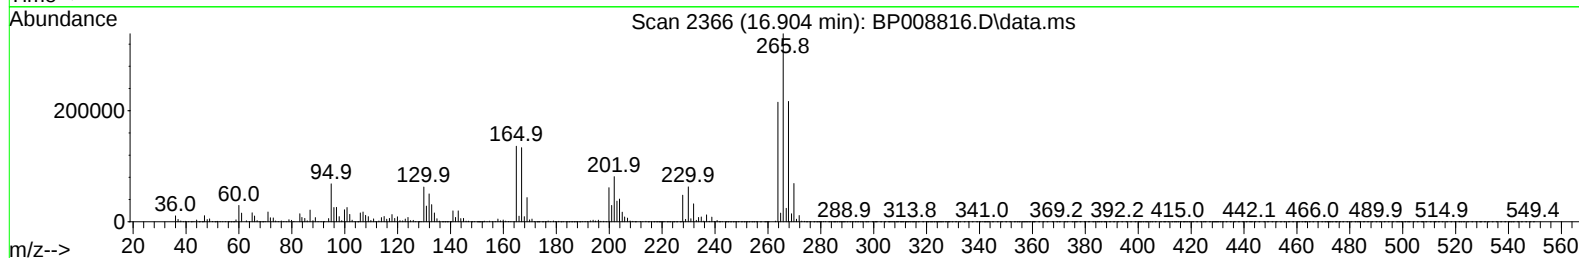


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011722\
 Data File : BP008816.D
 Acq On : 17 Jan 2022 09:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 14:28:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 14 18:05:00 2022
 Response via : Initial Calibration

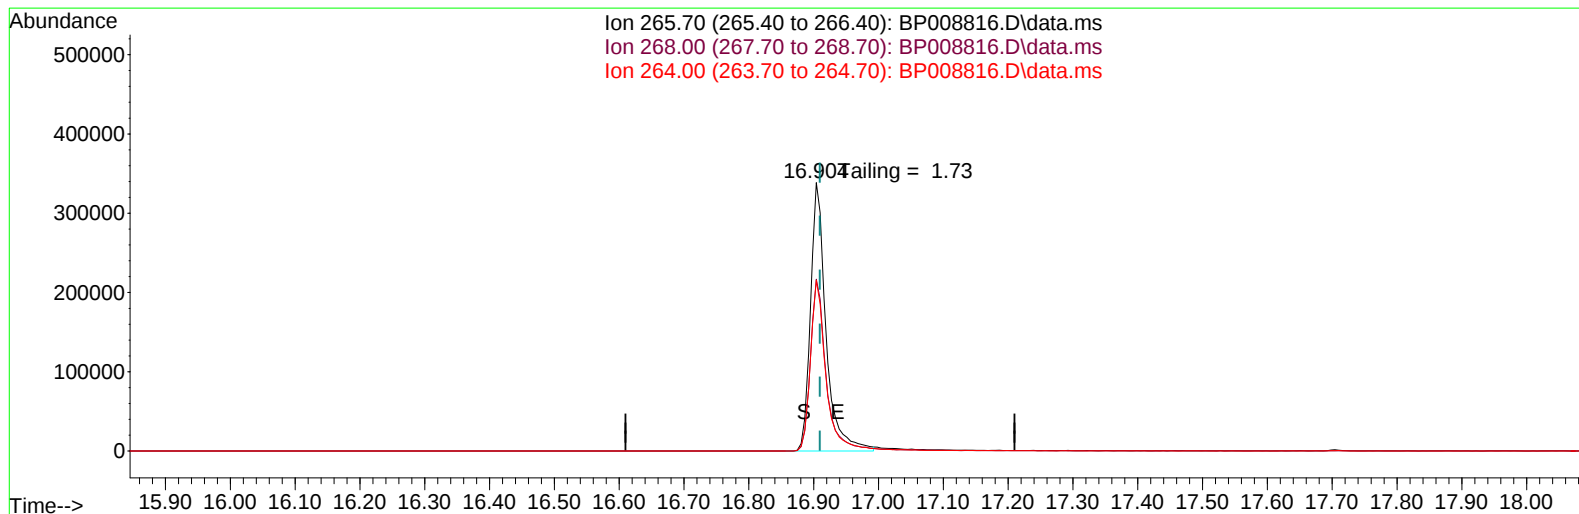




TIC: BP008816.D\data.ms

(70) Pentachlorophenol (C)**16.904min (-0.006) 3994483.44 ng****response 578463**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.01
264.00	62.90	63.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011722\
 Data File : BP008816.D
 Acq On : 17 Jan 2022 09:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 14:28:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 14 18:05:00 2022
 Response via : Initial Calibration

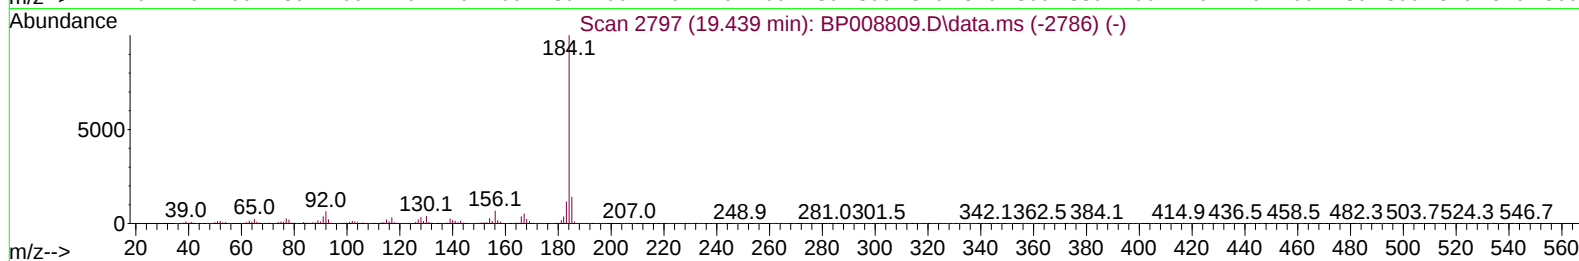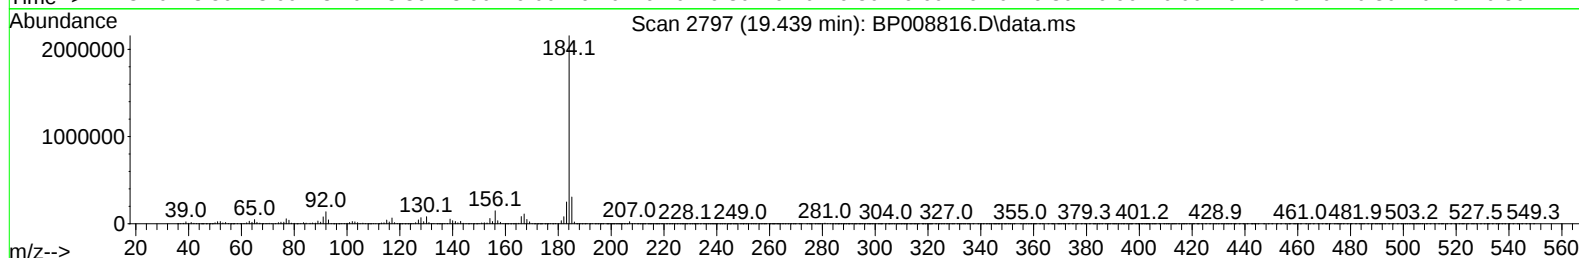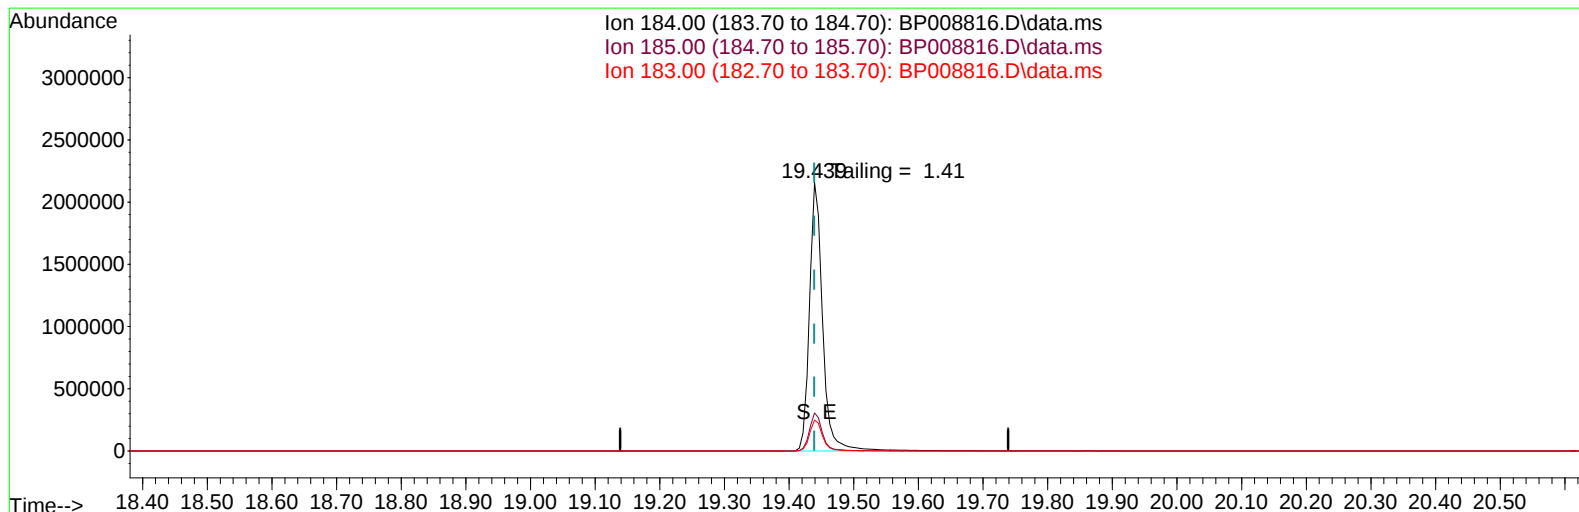

TIC: BP008816.D\data.ms

(77) Benzidine**19.439min (+ 0.000) 960249.74 ng****response 3053115**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.22
183.00	11.90	11.54
0.00	0.00	0.00