
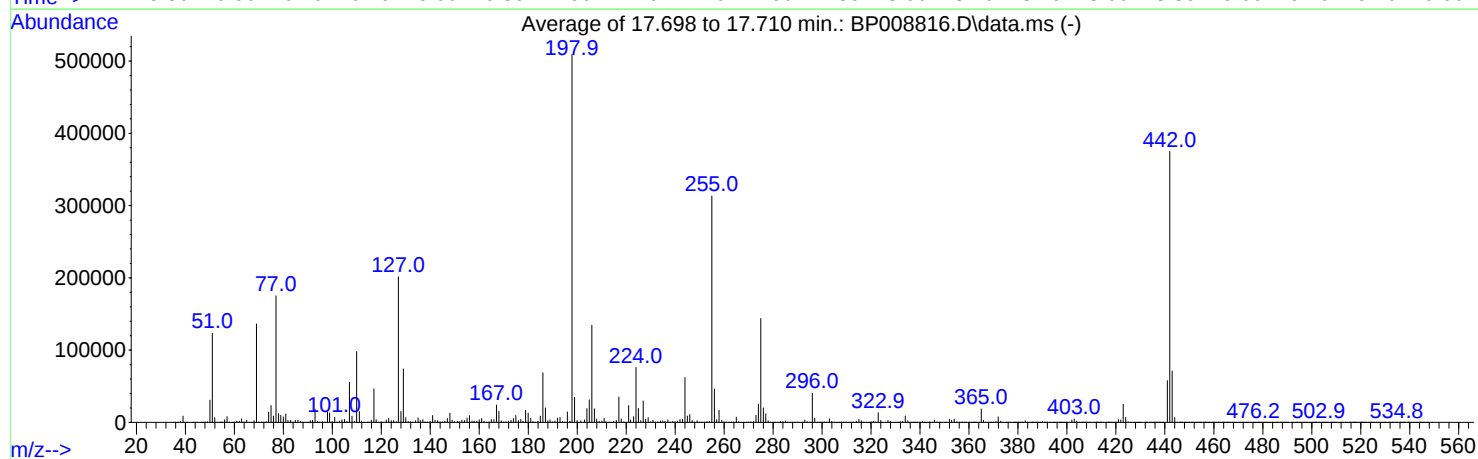


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011722\
 Data File : BP008816.D
 Acq On : 17 Jan 2022 09:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 14 18:05:00 2022

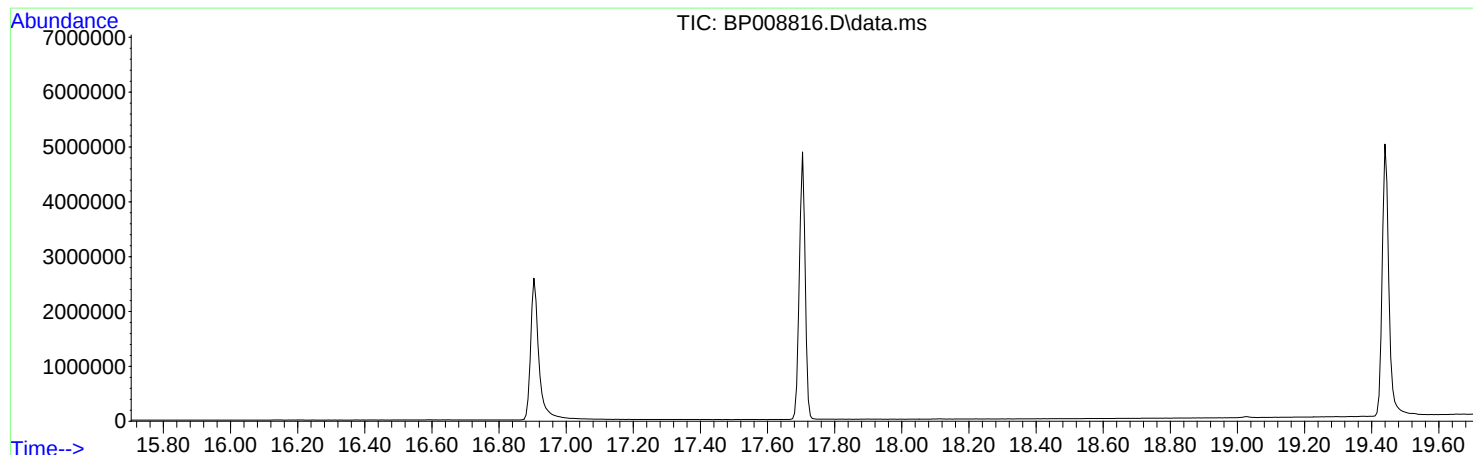




AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.2	123400	PASS
68	69	0.00	2	1.6	2124	PASS
69	198	0.00	100	26.7	136161	PASS
70	69	0.00	2	0.5	722	PASS
127	198	10	80	39.6	201515	PASS
197	198	0.00	2	0.3	1282	PASS
198	198	100	100	100.0	509139	PASS
199	198	5	9	6.8	34629	PASS
275	198	10	60	28.2	143749	PASS
365	198	1	100	3.7	18712	PASS
441	198	0.01	100	11.3	57714	PASS
442	442	100	100	100.0	374912	PASS
443	442	15	24	19.0	71075	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011722\
Data File : BP008816.D
Acq On : 17 Jan 2022 09:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 17 14:28:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 14 18:05:00 2022
Response via : Initial Calibration

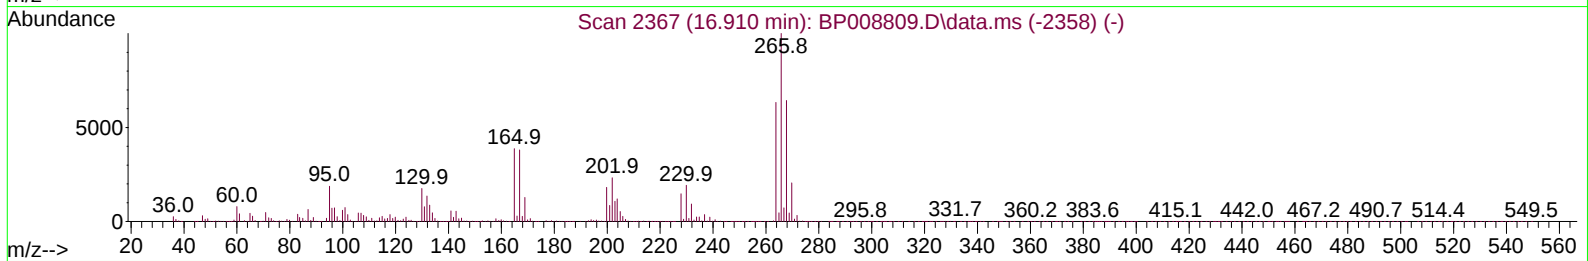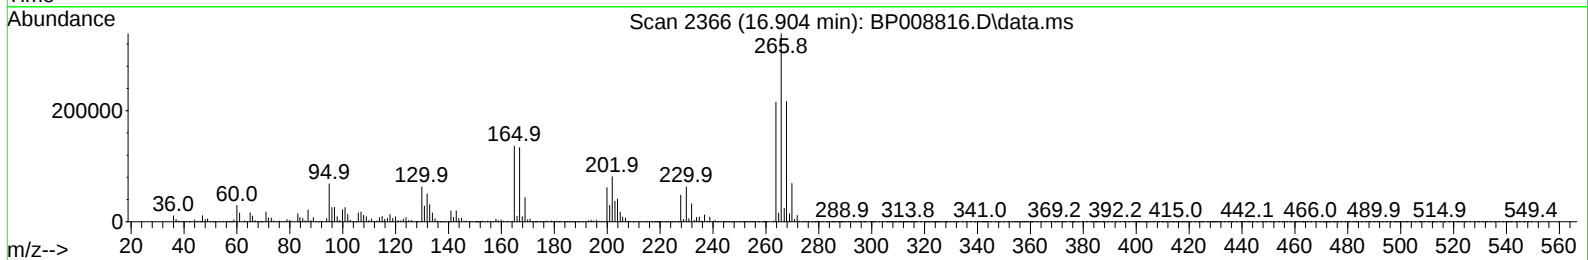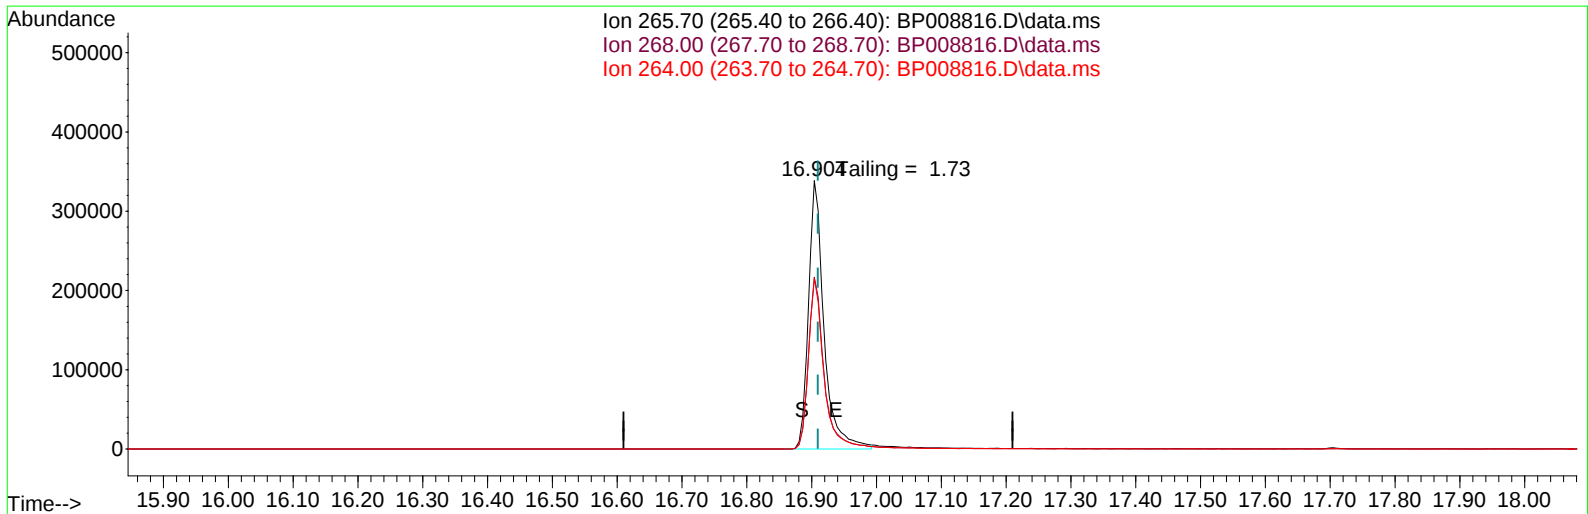

TIC: BP008816.D\data.ms

(70) Pentachlorophenol (C)

16.904min (-0.006) 3994483.44 ng




response 578463

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.01
264.00	62.90	63.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011722\
Data File : BP008816.D
Acq On : 17 Jan 2022 09:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 17 14:28:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 14 18:05:00 2022
Response via : Initial Calibration

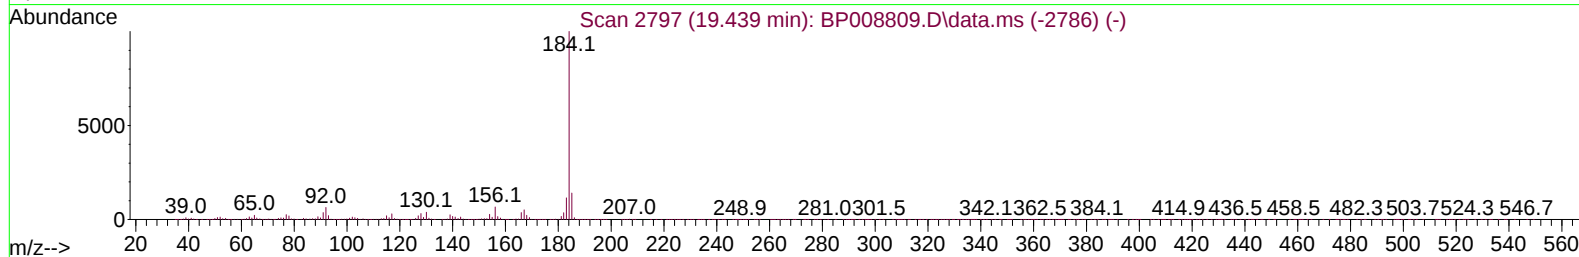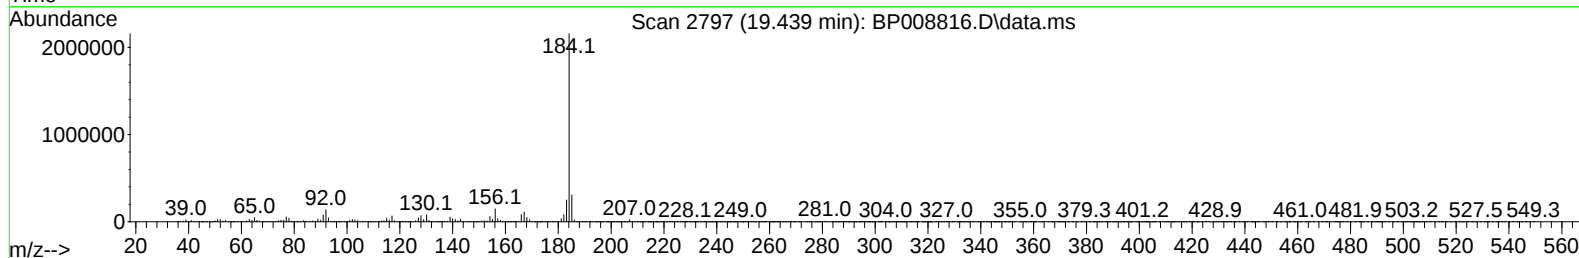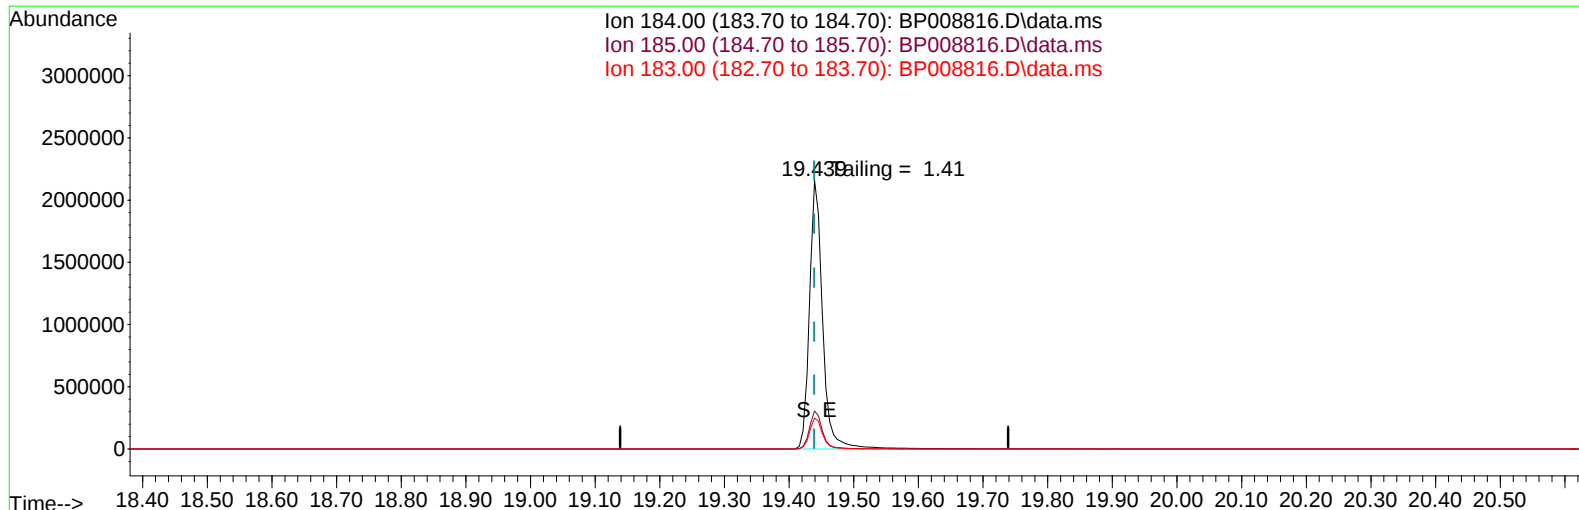

TIC: BP008816.D\data.ms

(77) Benzidine

19.439min (+ 0.000) 960249.74 ng

response 3053115

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.22
183.00	11.90	11.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/17/2022	BNA_P	BP008816.D
Compound Name	Response	Retention Time
DDT	1669003	20.65
DDD	20071	20.22
DDE	4645	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24716	1693719	1.46

Instrument :
BNA_P
ClientSampleId :
DFTPP