
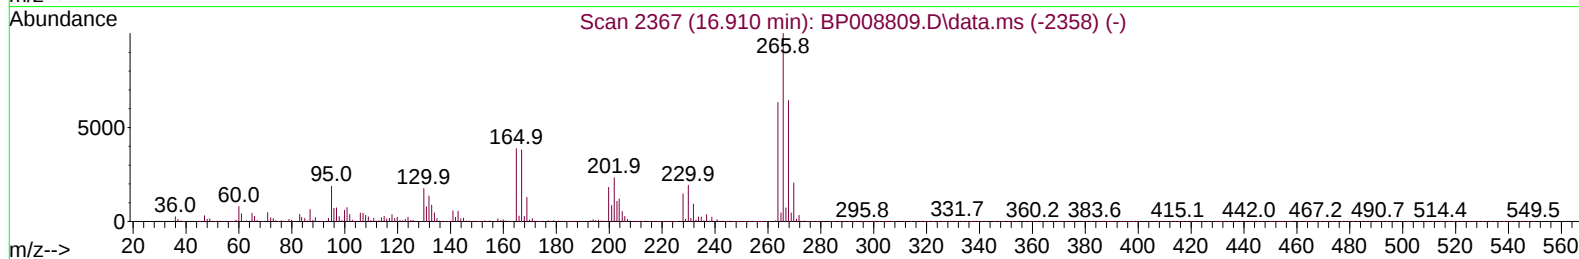
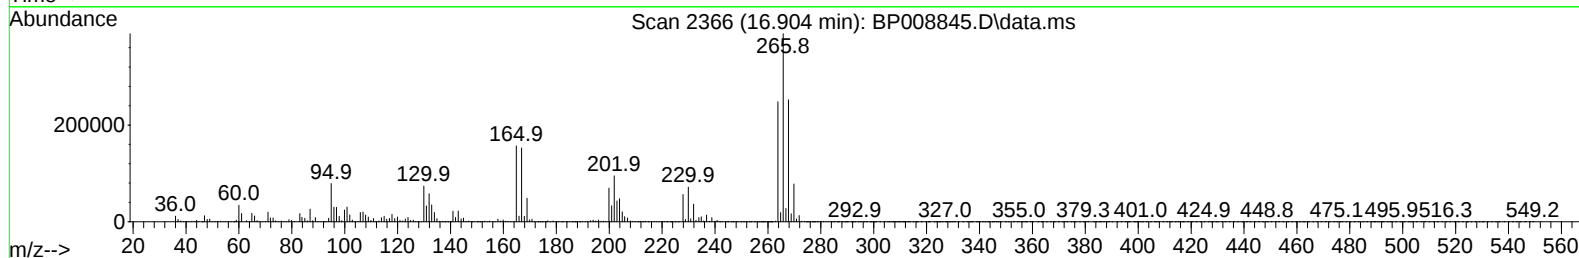


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011922\
Data File : BP008845.D
Acq On : 19 Jan 2022 10:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 12:57:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 14 18:05:00 2022
Response via : Initial Calibration

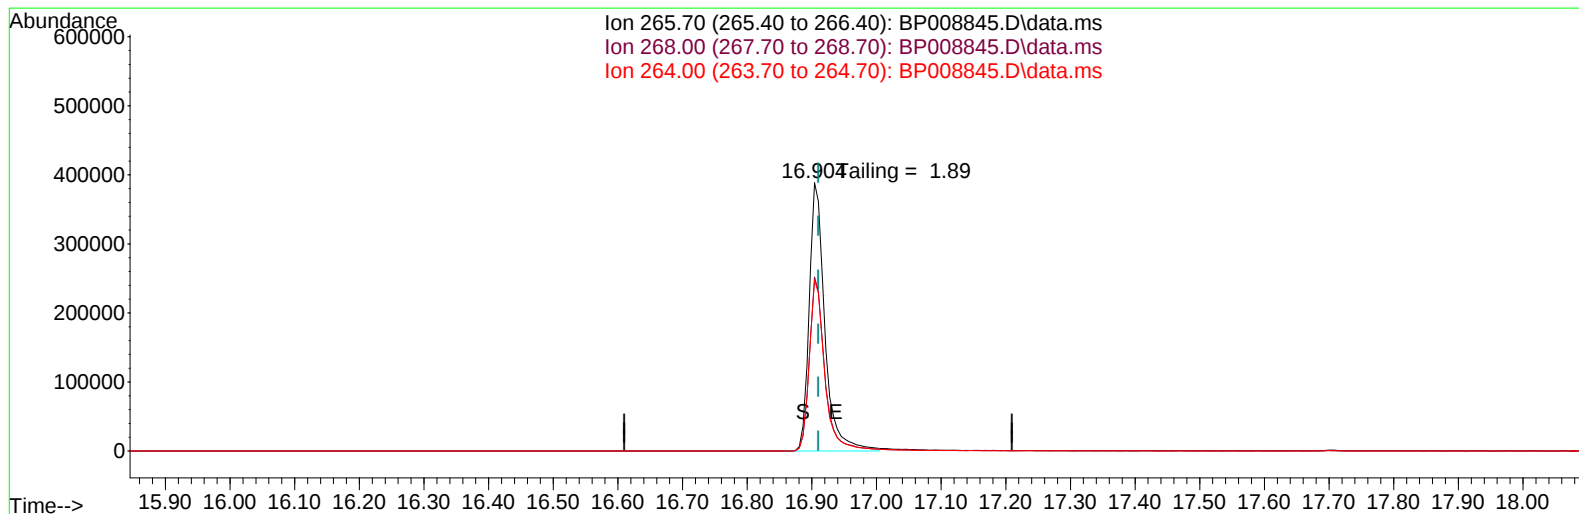

TIC: BP008845.D\data.ms

(70) Pentachlorophenol (C)




16.904min (-0.006) 1268864.45 ng

response 667307

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.83
264.00	62.90	63.81
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP01192\  
Data File : BP008845.D  
Acq On    : 19 Jan 2022  10:08  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jan 19 12:57:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 14 18:05:00 2022
Response via : Initial Calibration

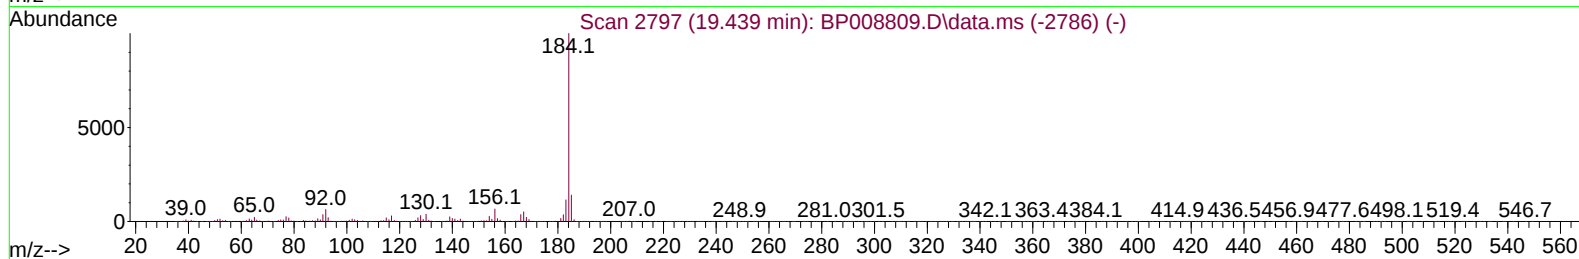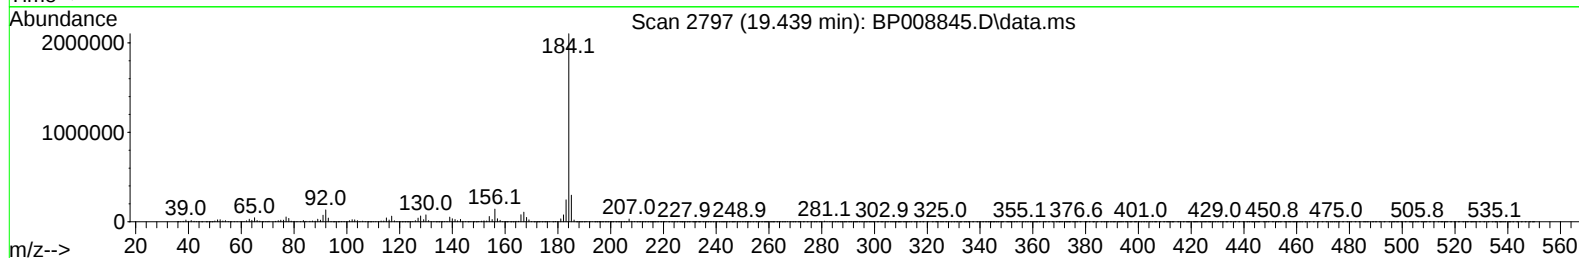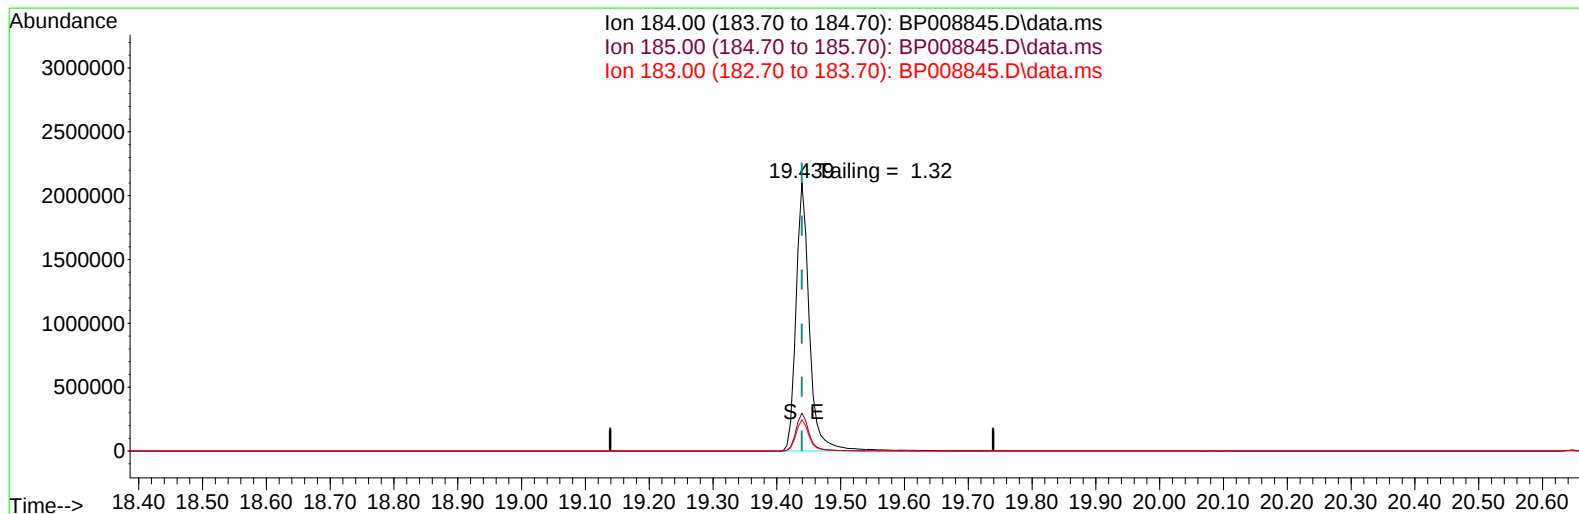

TIC: BP008845.D\data.ms

(77) Benzidine

19.439min (+ 0.000) 1062688.27 ng

response 3078479

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.14
183.00	11.90	11.69
0.00	0.00	0.00