

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011922\
 Data File : BP008856.D
 Acq On : 19 Jan 2022 16:29
 Operator : CG/JU
 Sample : N1154-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 20220032-KEANSBURG-3-MODIFIED-ELUTRIATE

Quant Time: Jan 20 05:29:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 14 18:05:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	267920	20.000	ng	-0.01
21) Naphthalene-d8	10.646	136	1028977	20.000	ng	-0.01
39) Acenaphthene-d10	14.487	164	662041	20.000	ng	-0.01
64) Phenanthrene-d10	17.239	188	1318734	20.000	ng	-0.01
76) Chrysene-d12	21.333	240	1300794	20.000	ng	-0.01
86) Perylene-d12	23.751	264	1458406	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.428	112	1048856	60.539	ng	-0.01
7) Phenol-d6	7.022	99	851754	40.599	ng	-0.01
23) Nitrobenzene-d5	9.005	82	1746626	96.370	ng	-0.01
42) 2,4,6-Tribromophenol	15.981	330	1340528	139.107	ng	-0.01
45) 2-Fluorobiphenyl	13.110	172	4616156	91.951	ng	-0.01
79) Terphenyl-d14	19.804	244	5169911	67.086	ng	-0.01


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011922\
Data File : BP008856.D
Acq On : 19 Jan 2022 16:29
Operator : CG/JU
Sample : N1154-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20220032-KEANSBURG-3-MODIFIED-ELUTRIATE

Quant Time: Jan 20 05:29:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 14 18:05:00 2022
Response via : Initial Calibration



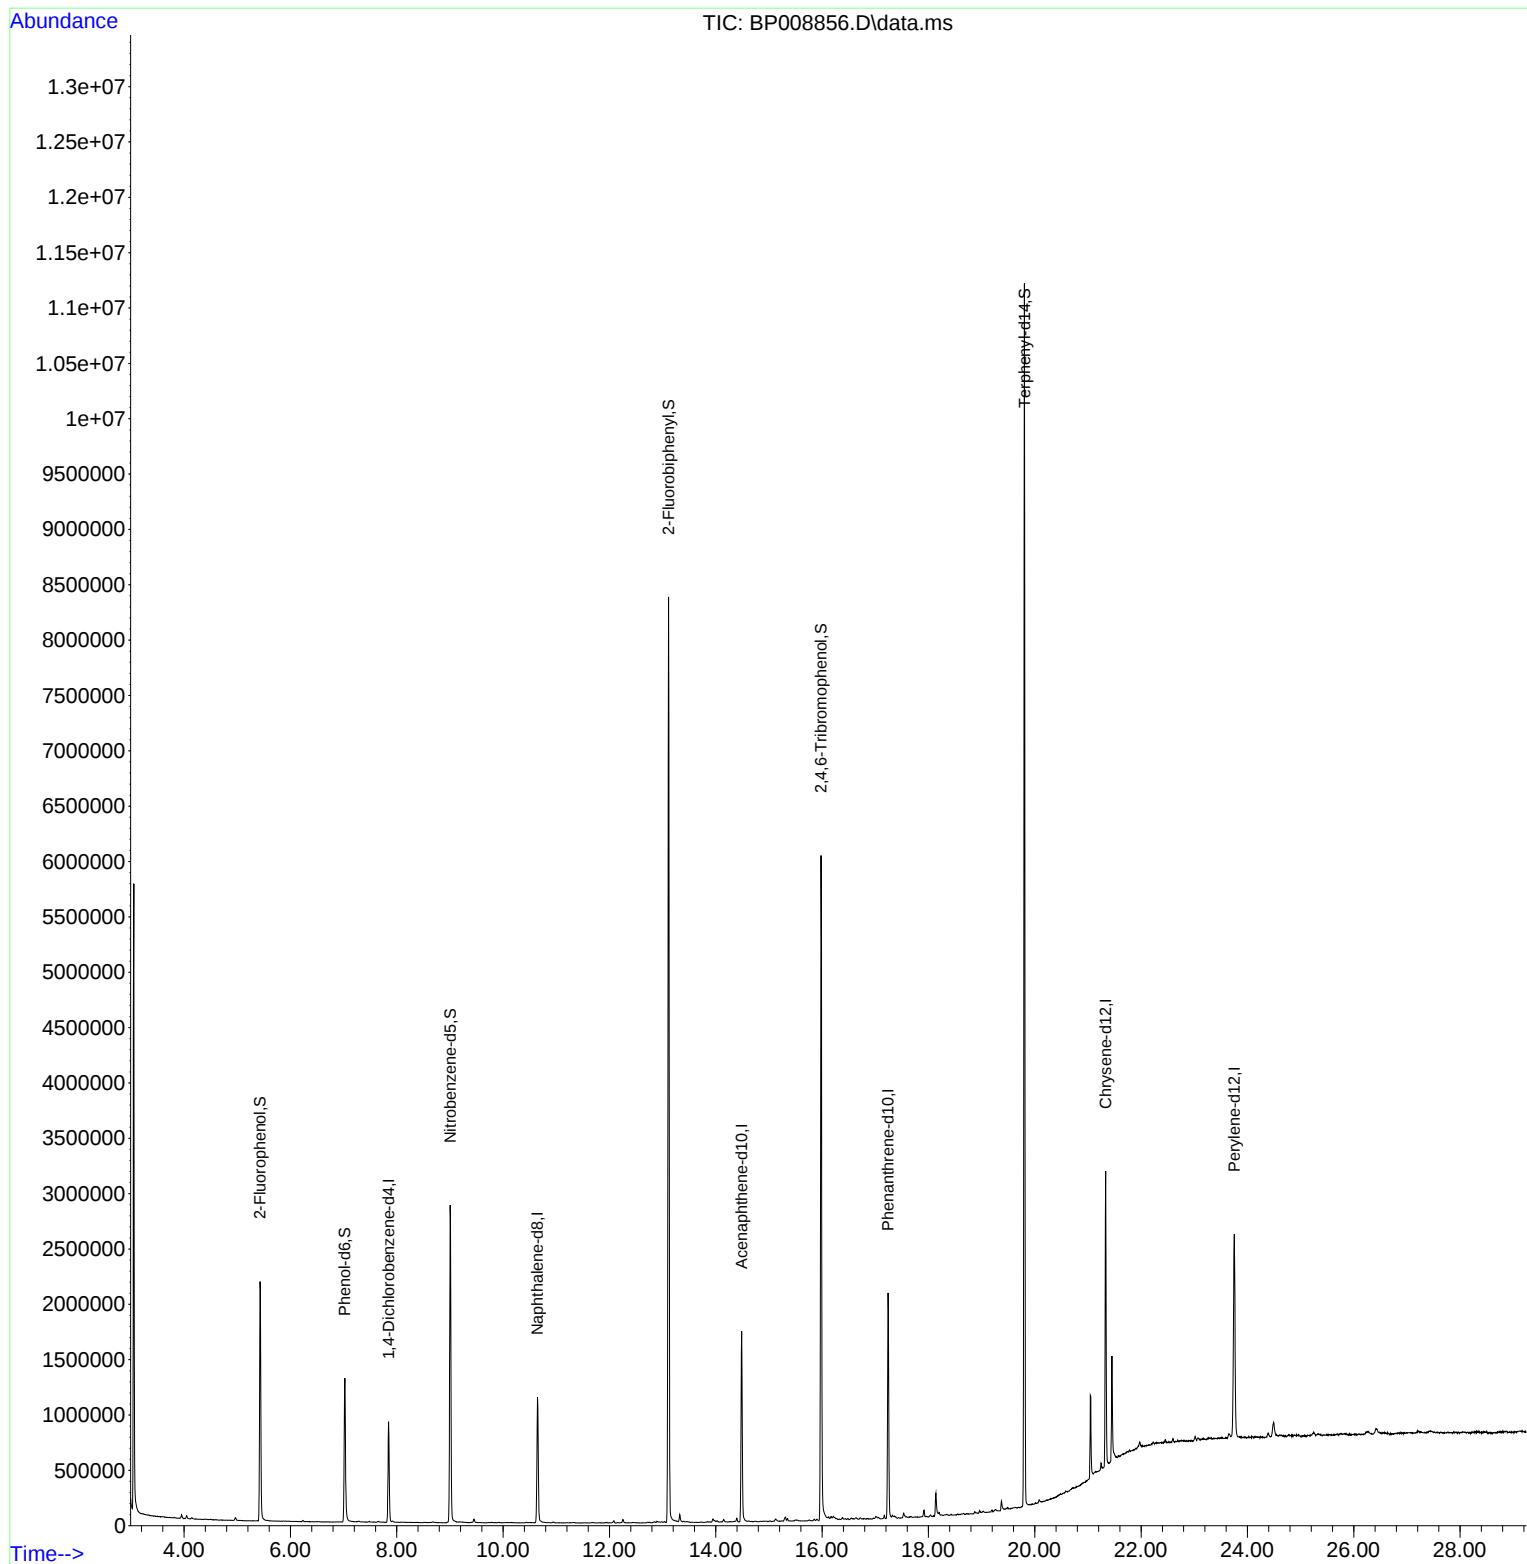




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.846 min Scan# 81
Delta R.T. -0.011 min
Lab File: BP008856.D
Acq: 19 Jan 2022 16:29




Instrument :
BNA_P
ClientSampleId :
20220032-KEANSBURG-3-MODIFIED-ELUTRIATE


Tgt Ion:152 Resp: 267920
Ion Ratio Lower Upper
152 100
150 154.8 127.0 190.6
115 55.5 43.7 65.5

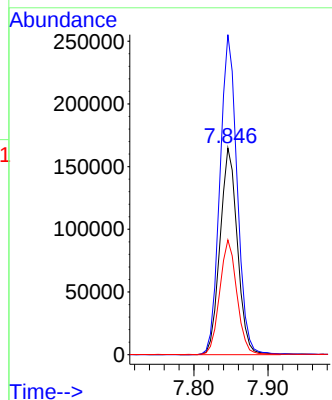

#5
2-Fluorophenol
Concen: 60.539 ng
RT: 5.428 min Scan# 415
Delta R.T. -0.011 min
Lab File: BP008856.D
Acq: 19 Jan 2022 16:29

Tgt Ion:112 Resp: 1048856
Ion Ratio Lower Upper
112 100
64 51.9 39.7 59.5
63 27.5 20.0 30.0


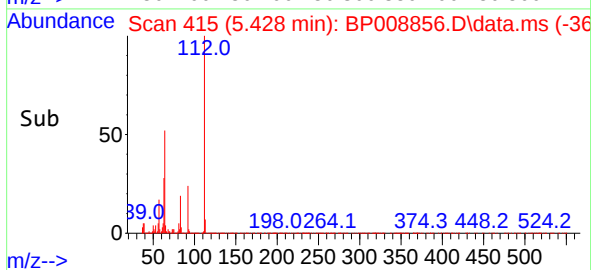
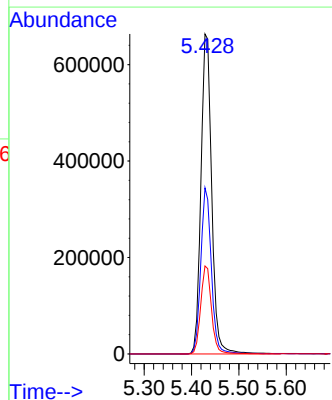





#7
Phenol-d6
Concen: 40.599 ng
RT: 7.022 min Scan# 61
Delta R.T. -0.011 min
Lab File: BP008856.D
Acq: 19 Jan 2022 16:29




Instrument : BNA_P
ClientSampleId : 20220032-KEANSBURG-3-MODIFIED-ELUTRIATE

Tgt Ion: 99 Resp: 851754
Ion Ratio Lower Upper
99 100
42 16.3 10.8 16.2#
71 31.9 23.8 35.6

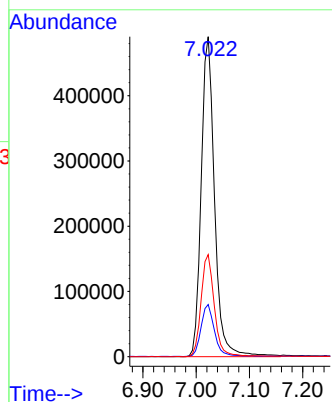

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.646 min Scan# 1302
Delta R.T. -0.011 min
Lab File: BP008856.D
Acq: 19 Jan 2022 16:29

Tgt Ion: 136 Resp: 1028977
Ion Ratio Lower Upper
136 100
137 11.5 9.0 13.4
54 6.3 4.9 7.3
68 5.4 4.3 6.5


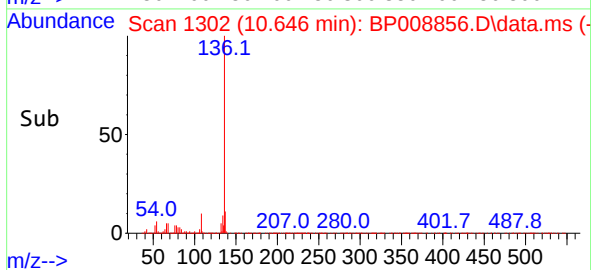
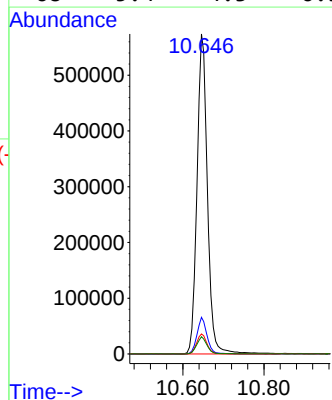





#23
Nitrobenzene-d5
Concen: 96.370 ng
RT: 9.005 min Scan# 10
Delta R.T. -0.011 min
Lab File: BP008856.D
Acq: 19 Jan 2022 16:29




Instrument :
BNA_P
ClientSampleId :
20220032-KEANSBURG-3-MODIFIED-ELUTRIATE


Tgt Ion: 82 Resp: 1746626
Ion Ratio Lower Upper
82 100
128 46.4 39.4 59.2
54 43.5 32.6 48.8

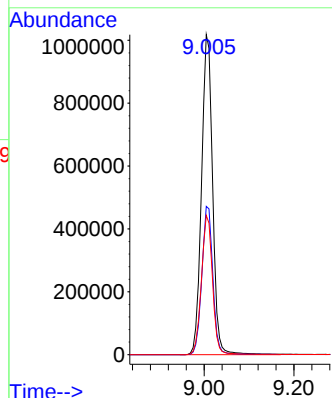

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.487 min Scan# 1955
Delta R.T. -0.011 min
Lab File: BP008856.D
Acq: 19 Jan 2022 16:29

Tgt Ion:164 Resp: 662041
Ion Ratio Lower Upper
164 100
162 98.7 79.9 119.9
160 44.9 35.5 53.3


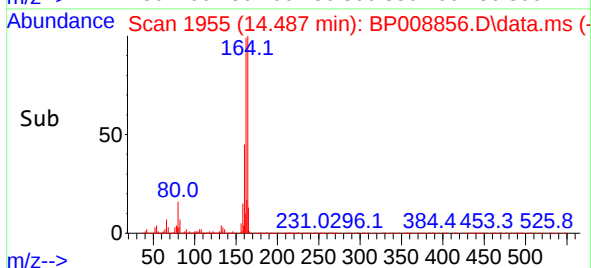
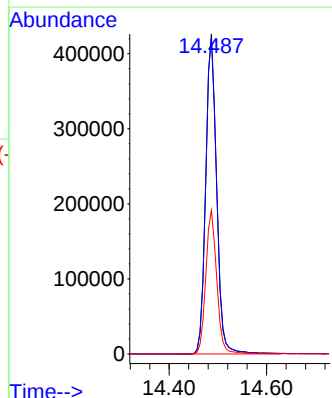





#42
2,4,6-Tribromophenol
Concen: 139.107 ng
RT: 15.981 min Scan# 21
Delta R.T. -0.011 min
Lab File: BP008856.D
Acq: 19 Jan 2022 16:29




Instrument : BNA_P
ClientSampleId : 20220032-KEANSBURG-3-MODIFIED-ELUTRIATE


Tgt Ion:330 Resp: 1340528
Ion Ratio Lower Upper
330 100
332 96.5 77.0 115.4
141 29.9 21.3 31.9

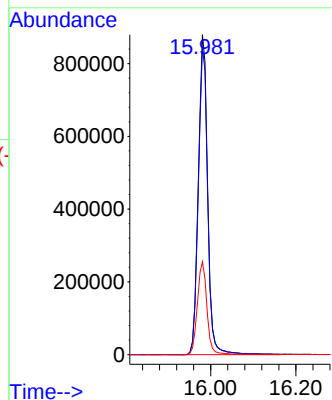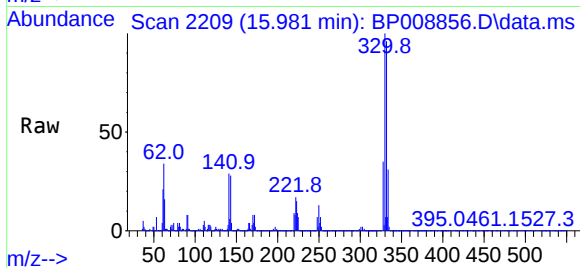

#45
2-Fluorobiphenyl
Concen: 91.951 ng
RT: 13.110 min Scan# 1721
Delta R.T. -0.011 min
Lab File: BP008856.D
Acq: 19 Jan 2022 16:29

Tgt Ion:172 Resp: 4616156
Ion Ratio Lower Upper
172 100
171 36.0 29.3 43.9
170 24.1 19.5 29.3


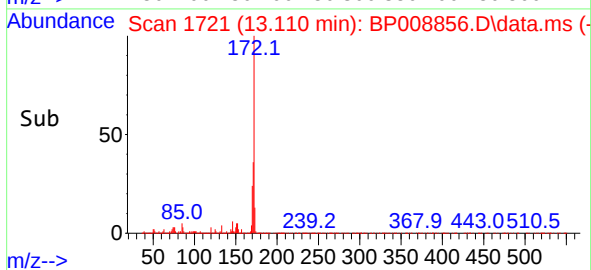
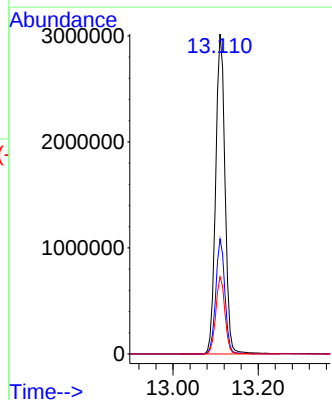
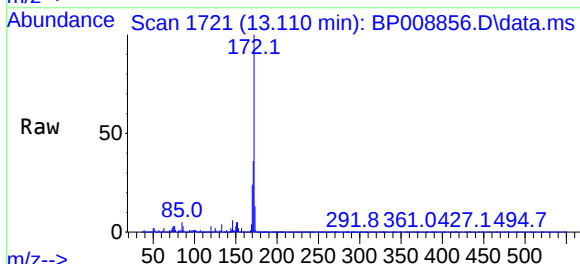




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.239 min Scan# 2425
Delta R.T. -0.011 min
Lab File: BP008856.D
Acq: 19 Jan 2022 16:29




Instrument : BNA_P
ClientSampleId : 20220032-KEANSBURG-3-MODIFIED-ELUTRIATE


Tgt Ion:188 Resp: 1318734
Ion Ratio Lower Upper
188 100
94 7.5 6.8 10.2
80 7.9 7.2 10.8

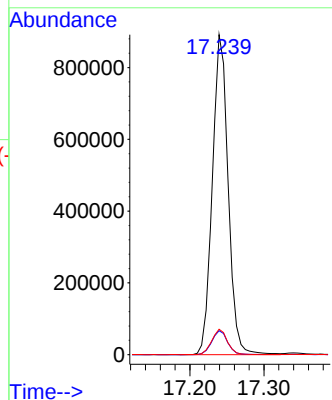

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.333 min Scan# 3119
Delta R.T. -0.011 min
Lab File: BP008856.D
Acq: 19 Jan 2022 16:29

Tgt Ion:240 Resp: 1300794
Ion Ratio Lower Upper
240 100
120 8.6 7.7 11.5
236 26.1 21.2 31.8


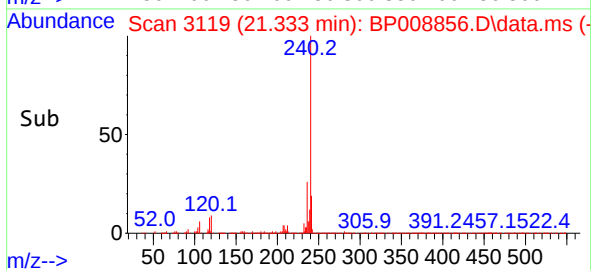
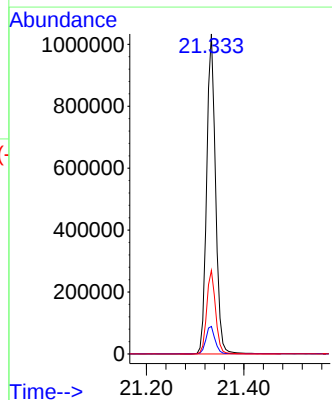





#79
 Terphenyl-d14
 Concen: 67.086 ng
 RT: 19.804 min Scan# 21
 Delta R.T. -0.011 min
 Lab File: BP008856.D
 Acq: 19 Jan 2022 16:29

Instrument : BNA_P
 ClientSampleId : 20220032-KEANSBURG-3-MODIFIED-ELUTRIATE

Tgt Ion:244 Resp: 5169911
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.5 9.7
 122 8.8 9.2 13.8#

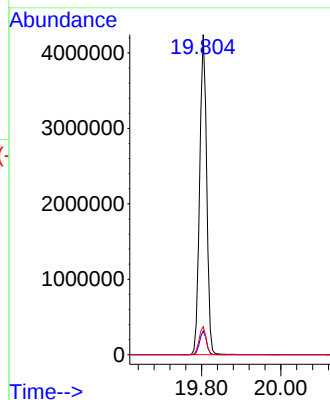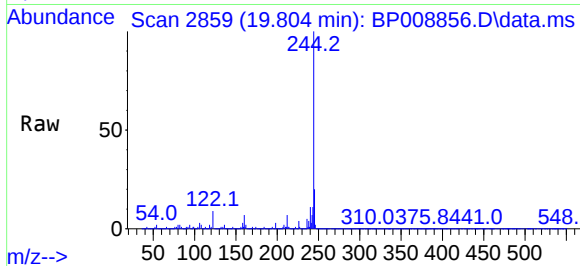

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.751 min Scan# 3530
 Delta R.T. -0.011 min
 Lab File: BP008856.D
 Acq: 19 Jan 2022 16:29

Tgt Ion:264 Resp: 1458406
 Ion Ratio Lower Upper
 264 100
 260 24.6 19.1 28.7
 265 21.6 17.1 25.7

