

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011922\
 Data File : BP008865.D
 Acq On : 19 Jan 2022 21:29
 Operator : CG/JU
 Sample : N1182-01 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OR-2-011822

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008865.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.046	6	10	32	rVB	208312	385983	7.26%	1.044%
2	5.434	410	416	429	rBV	343842	581291	10.93%	1.572%
3	7.022	679	686	705	rBV	322074	638424	12.01%	1.726%
4	7.846	818	826	835	rBV	1007923	1657720	31.18%	4.482%
5	9.005	1017	1023	1033	rBV	204970	404774	7.61%	1.094%
6	10.646	1291	1302	1320	rBV	1439021	2619065	49.27%	7.081%
7	12.081	1541	1546	1552	rBV2	34755	55145	1.04%	0.149%
8	13.110	1714	1721	1732	rBV	874026	1361544	25.61%	3.681%
9	13.322	1751	1757	1763	rBV	56648	87391	1.64%	0.236%
10	14.210	1902	1908	1914	rBV	36555	65706	1.24%	0.178%
11	14.398	1935	1940	1945	rVB	82738	106582	2.00%	0.288%
12	14.487	1948	1955	1963	rBV	2685602	4053388	76.25%	10.959%
13	15.351	2097	2102	2107	rVB2	88708	114846	2.16%	0.311%
14	15.540	2130	2134	2138	rBV	34469	54458	1.02%	0.147%
15	15.981	2203	2209	2227	rBV	669721	1150143	21.64%	3.110%
16	16.216	2244	2249	2252	rBV	116001	173909	3.27%	0.470%
17	17.010	2380	2384	2389	rBV2	111515	147834	2.78%	0.400%
18	17.063	2390	2393	2402	rVB2	68232	123025	2.31%	0.333%
19	17.245	2417	2424	2428	rBV	3545949	5315877	100.00%	14.373%
20	17.286	2428	2431	2436	rVB	299503	423138	7.96%	1.144%
21	17.375	2443	2446	2452	rVB	82124	124017	2.33%	0.335%
22	17.751	2506	2510	2515	rBV	118998	156473	2.94%	0.423%
23	17.922	2535	2539	2543	rBV	191397	219059	4.12%	0.592%
24	18.139	2573	2576	2586	rVB3	125907	273764	5.15%	0.740%
25	18.298	2599	2603	2607	rBV3	97702	160797	3.02%	0.435%
26	18.422	2621	2624	2633	rBV2	144669	178469	3.36%	0.483%
27	19.028	2720	2727	2729	rBV5	279245	536442	10.09%	1.450%
28	19.051	2729	2731	2735	rVB4	290736	319281	6.01%	0.863%
29	19.186	2751	2754	2760	rVB6	86395	127196	2.39%	0.344%
30	19.251	2761	2765	2773	rBV	665508	969693	18.24%	2.622%
31	19.604	2820	2825	2834	rVB2	602030	1082676	20.37%	2.927%
32	19.804	2854	2859	2863	rBV	1769180	2175631	40.93%	5.882%
33	20.598	2991	2994	2997	rBV	206223	233739	4.40%	0.632%
34	21.051	3069	3071	3074	rVB2	284496	254479	4.79%	0.688%
35	21.333	3114	3119	3124	rBV	3746304	4999339	94.05%	13.517%
36	21.451	3136	3139	3143	rBV	783234	976561	18.37%	2.640%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011922\
Data File : BP008865.D
Acq On : 19 Jan 2022 21:29
Operator : CG/JU
Sample : N1182-01 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OR-2-011822

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37 23.757 3525 3531 3545 rVB2 2201592 4677806 88.00% 12.648%




Sum of corrected areas: 36985665

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011922\
Data File : BP008865.D
Acq On : 19 Jan 2022 21:29
Operator : CG/JU
Sample : N1182-01 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OR-2-011822

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

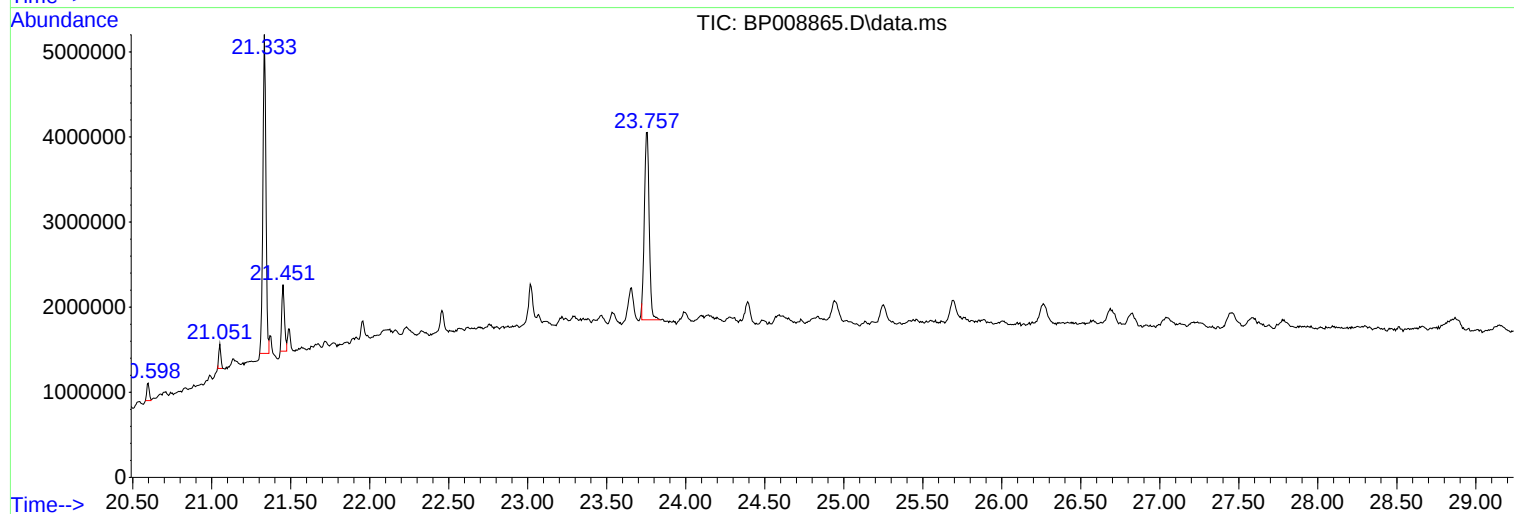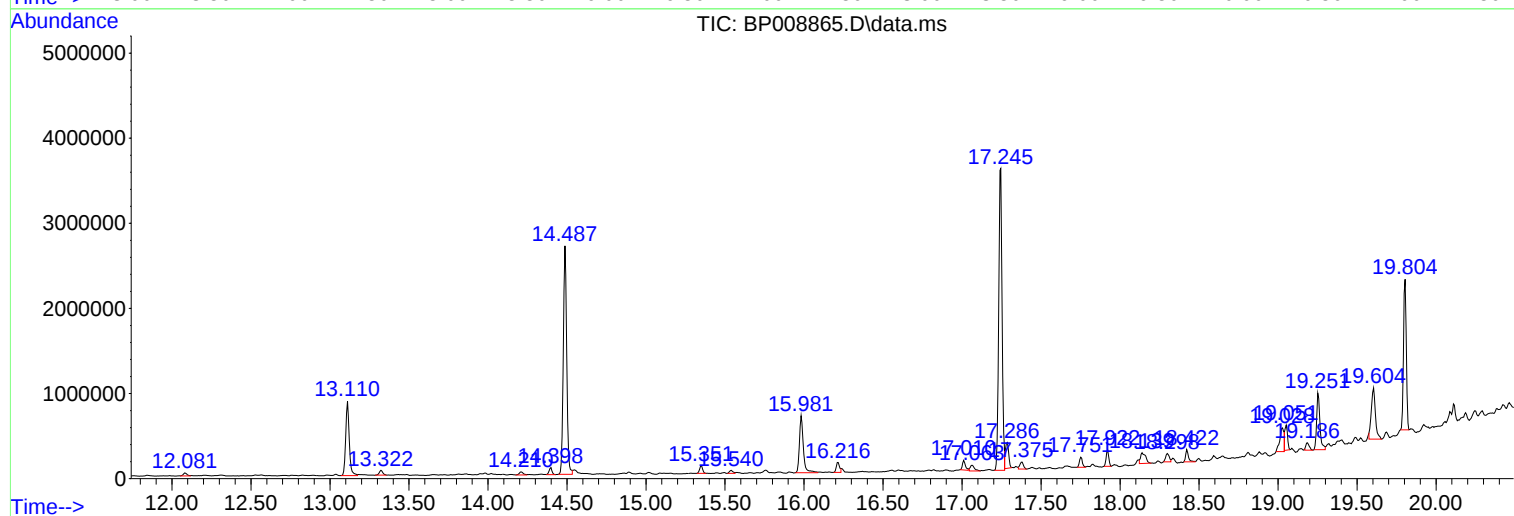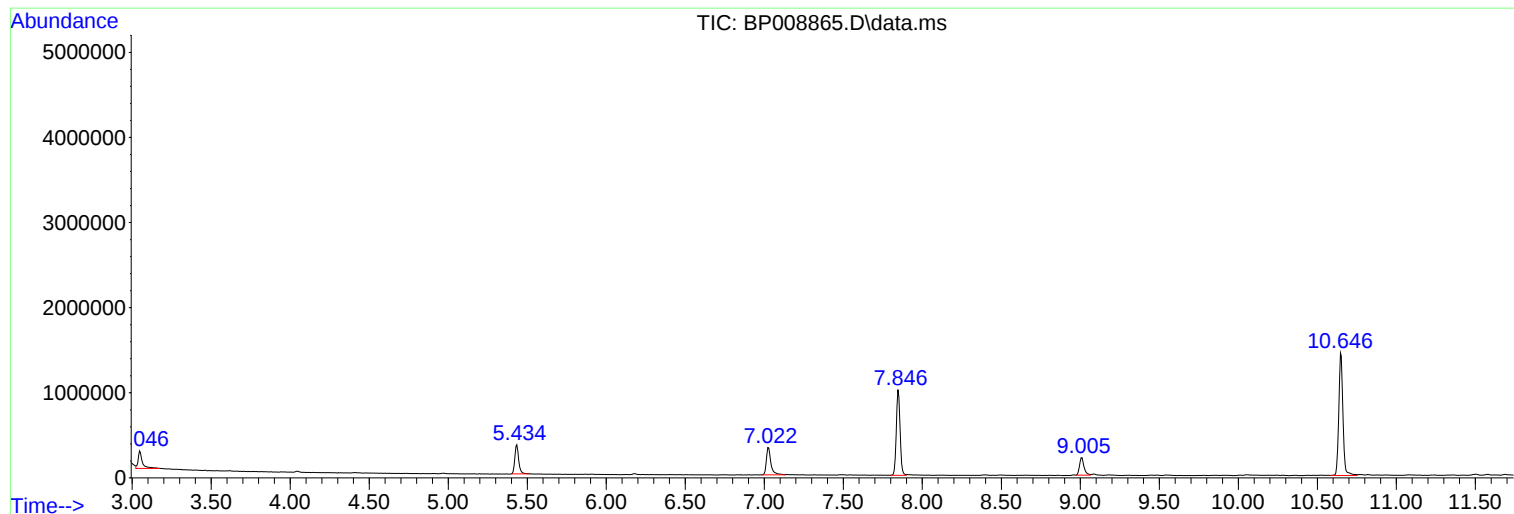

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011922\
Data File : BP008865.D
Acq On : 19 Jan 2022 21:29
Operator : CG/JU
Sample : N1182-01 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OR-2-011822

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011922\
Data File : BP008865.D
Acq On : 19 Jan 2022 21:29
Operator : CG/JU
Sample : N1182-01 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OR-2-011822

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------