
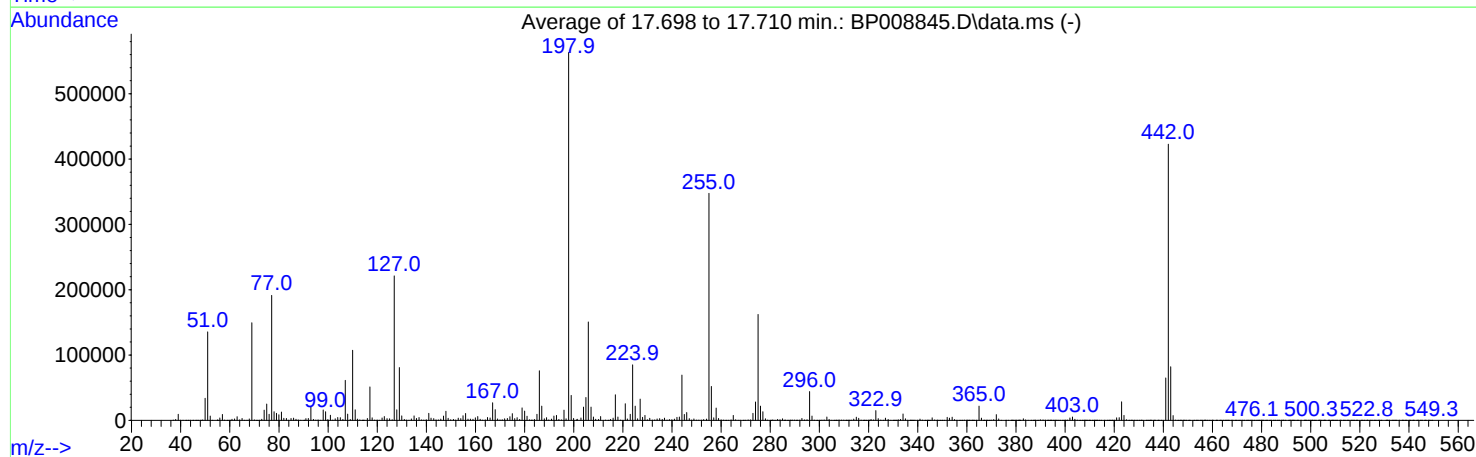


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011922\
 Data File : BP008845.D
 Acq On : 19 Jan 2022 10:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 14 18:05:00 2022

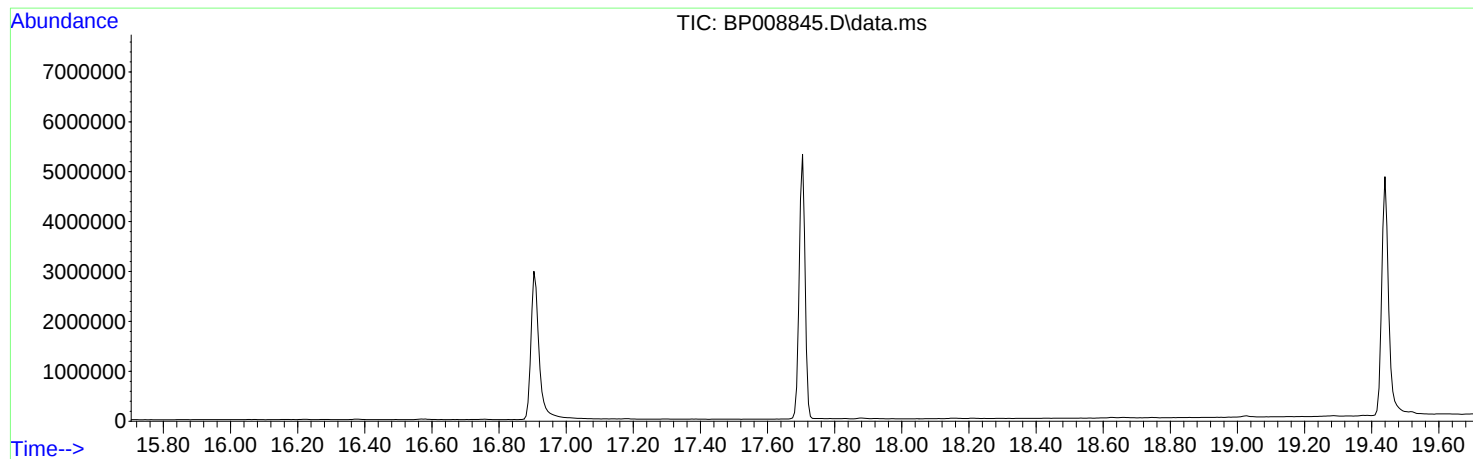




AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.0	135455	PASS
68	69	0.00	2	1.6	2320	PASS
69	198	0.00	100	26.5	149426	PASS
70	69	0.00	2	0.6	849	PASS
127	198	10	80	39.3	221141	PASS
197	198	0.00	2	0.4	2428	PASS
198	198	100	100	100.0	563241	PASS
199	198	5	9	6.8	38173	PASS
275	198	10	60	28.8	162317	PASS
365	198	1	100	3.9	21755	PASS
441	198	0.01	100	11.5	64926	PASS
442	442	100	100	100.0	422784	PASS
443	442	15	24	19.4	82016	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011922\
Data File : BP008845.D
Acq On : 19 Jan 2022 10:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 19 12:57:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 14 18:05:00 2022
Response via : Initial Calibration

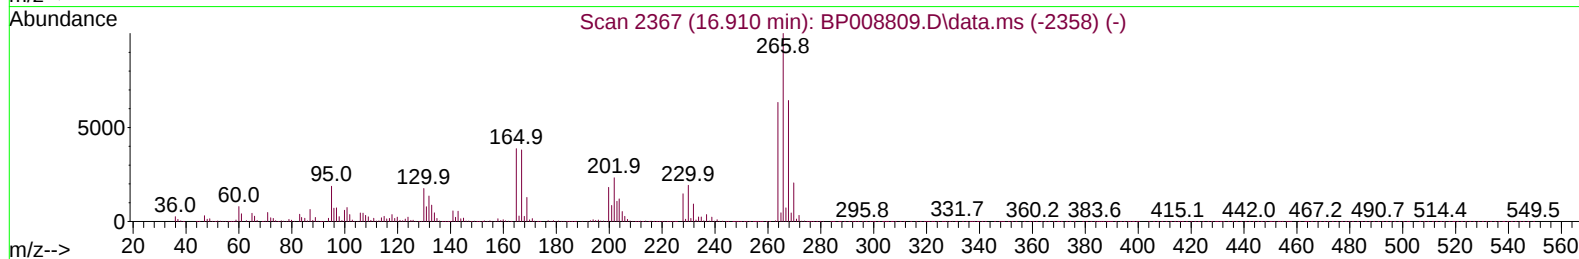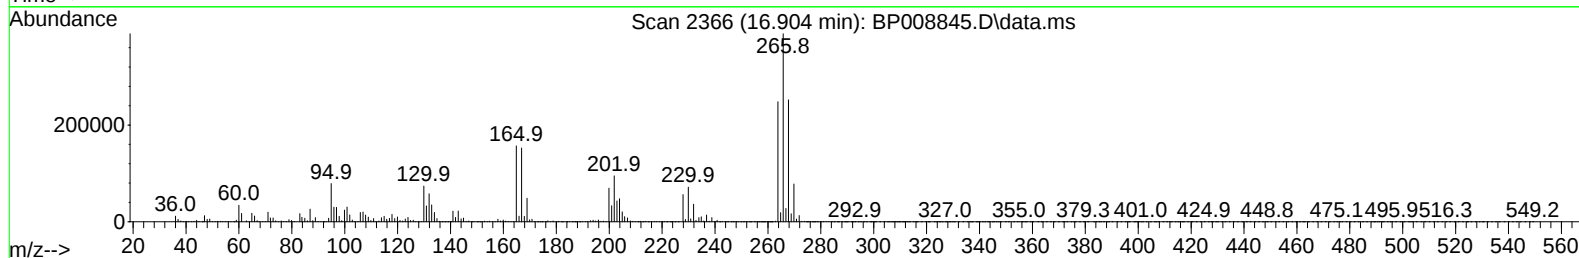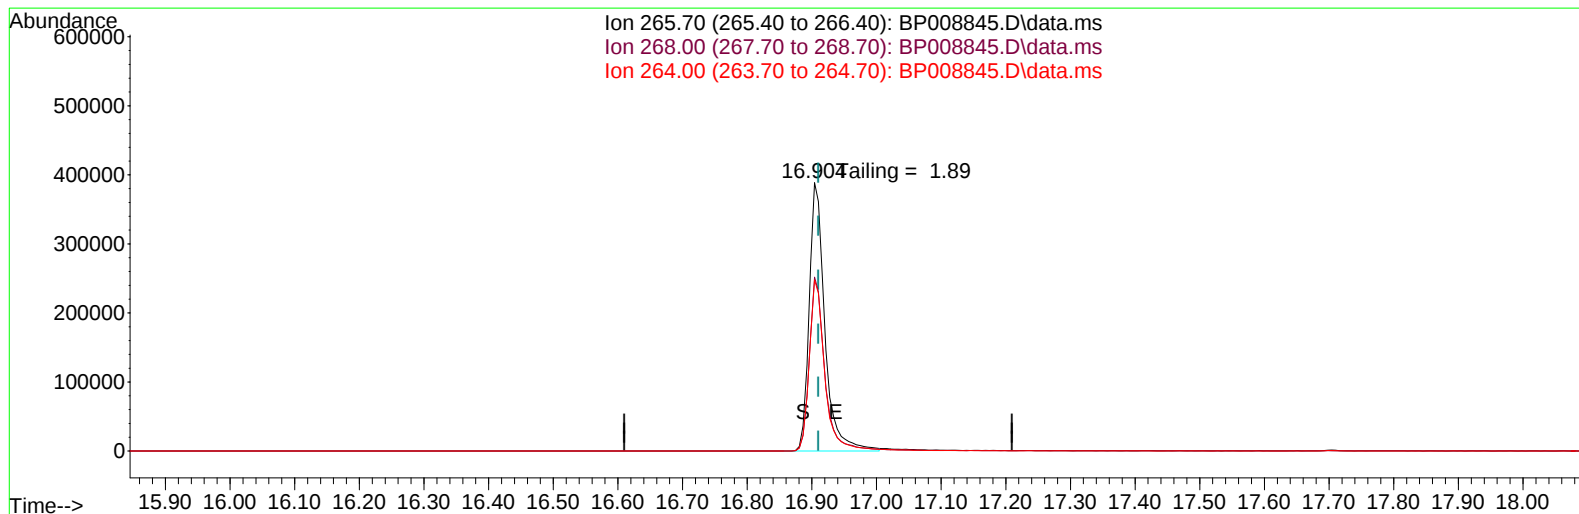

TIC: BP008845.D\data.ms

(70) Pentachlorophenol (C)

16.904min (-0.006) 1268864.45 ng




response 667307

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.83
264.00	62.90	63.81
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP01192\  
Data File : BP008845.D  
Acq On    : 19 Jan 2022  10:08  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 19 12:57:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 14 18:05:00 2022
Response via : Initial Calibration

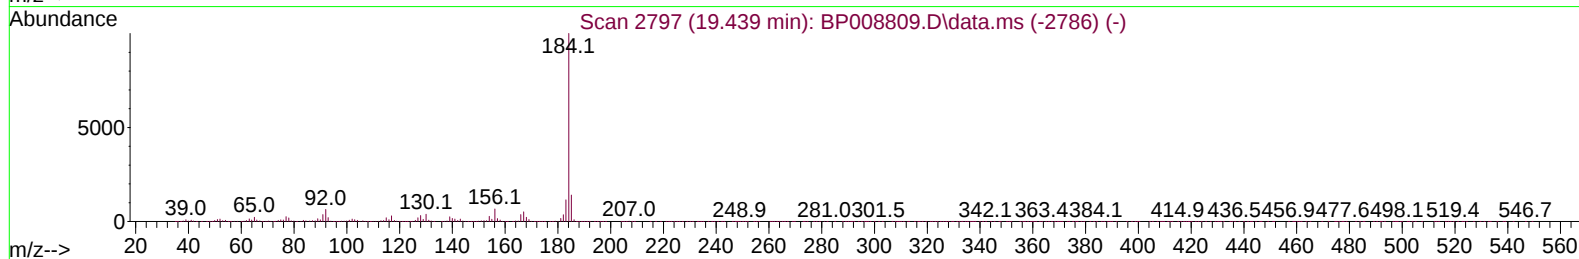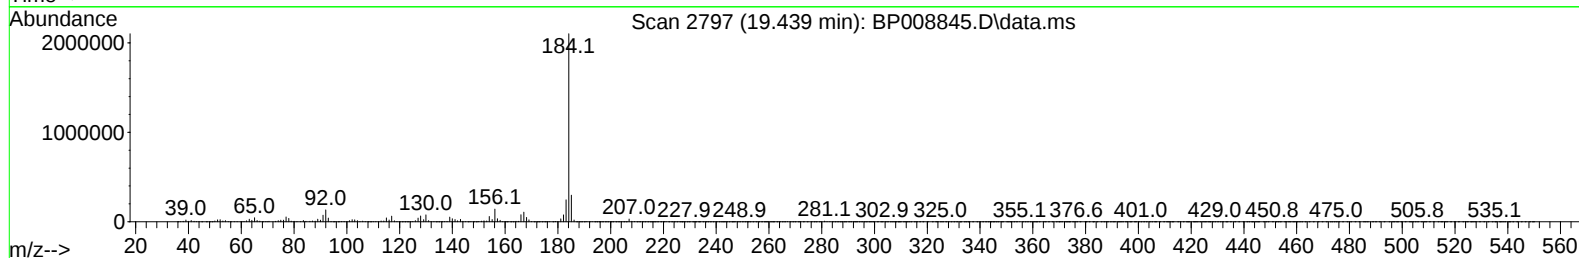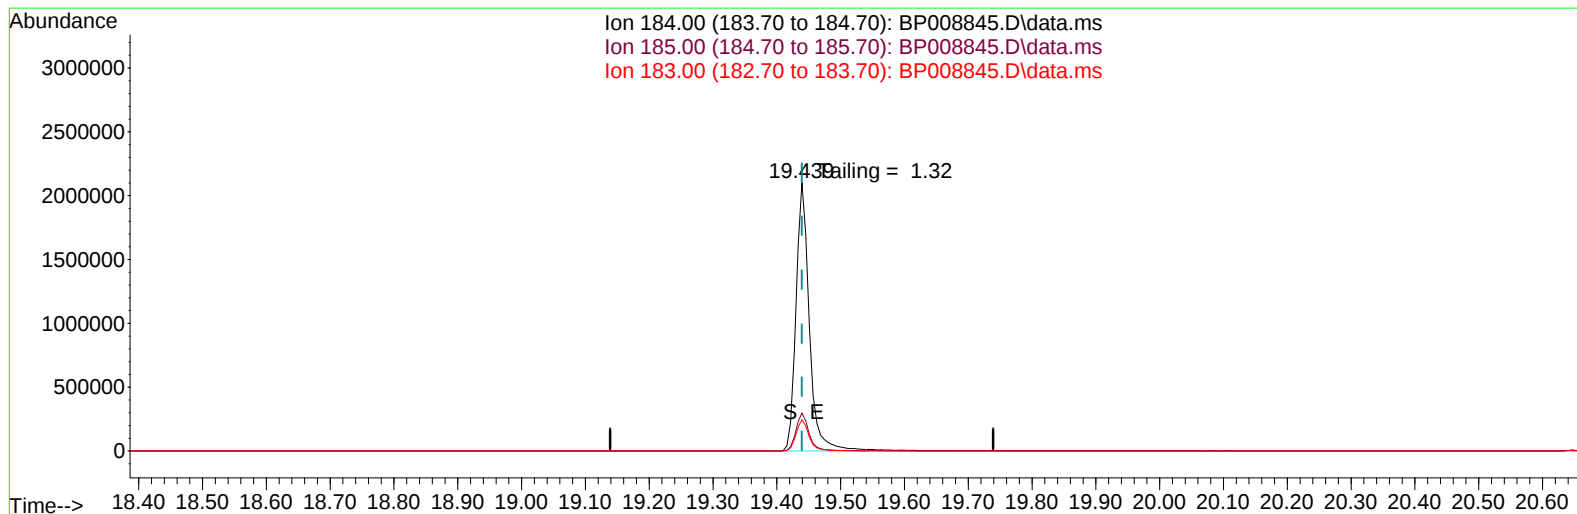

TIC: BP008845.D\data.ms

(77) Benzidine

19.439min (+ 0.000) 1062688.27 ng

response 3078479

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.14
183.00	11.90	11.69
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/19/2022	BNA_P	<u>BP008845.D</u>
Compound Name	Response	Retention Time
DDT	1738770	20.64
DDD	29832	20.21
DDE	3222	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33054	1771824	1.87

Instrument :
BNA_P
ClientSampleId :
DFTPP