
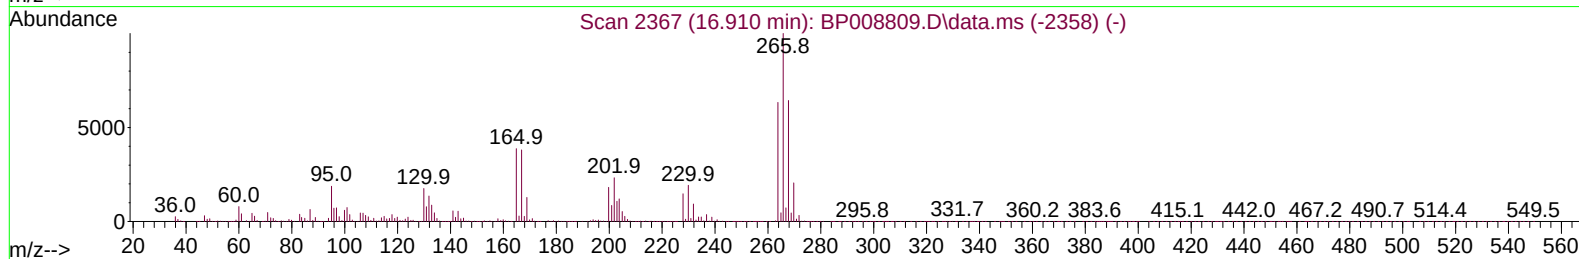
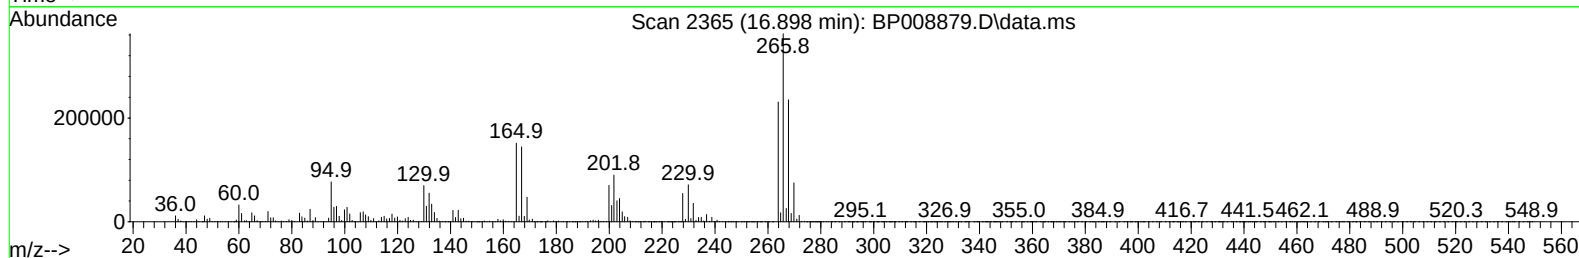


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012422\
Data File : BP008879.D
Acq On : 24 Jan 2022 10:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 17:10:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 14 18:05:00 2022
Response via : Initial Calibration

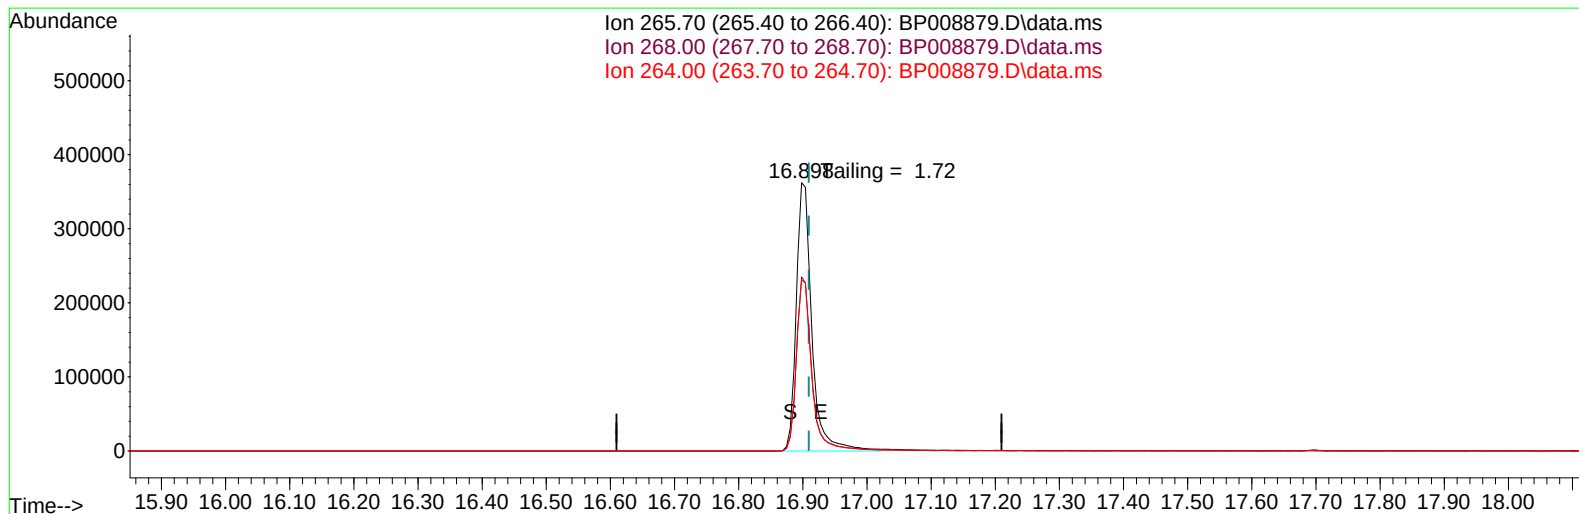

TIC: BP008879.D\data.ms

(70) Pentachlorophenol (C)




16.898min (-0.012) 272033.44 ng

response 617874

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.89
264.00	62.90	63.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012422\
 Data File : BP008879.D
 Acq On : 24 Jan 2022 10:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 17:10:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 14 18:05:00 2022
 Response via : Initial Calibration

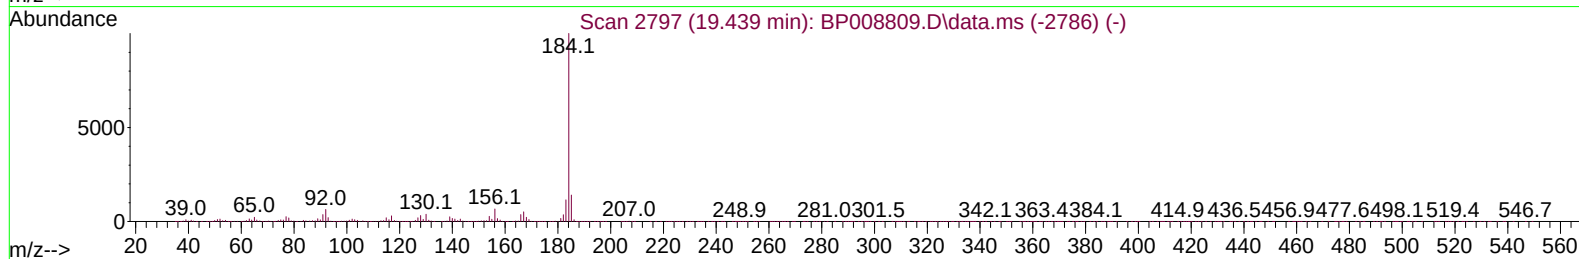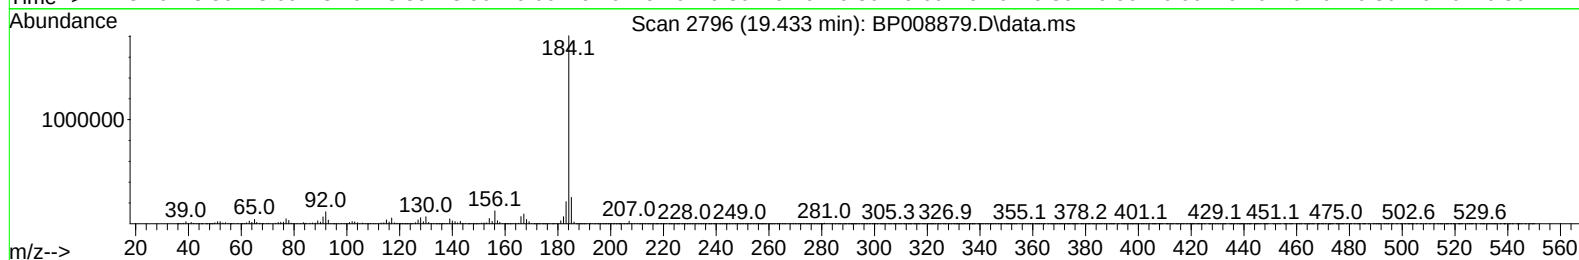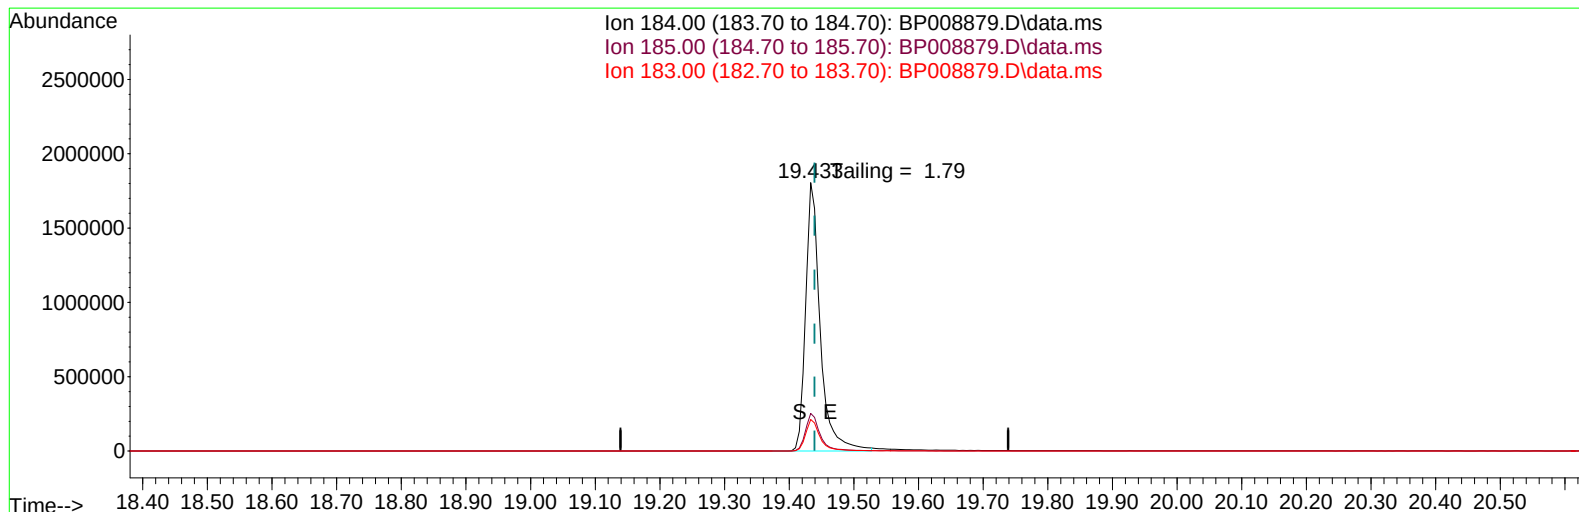

TIC: BP008879.D\data.ms

(77) Benzidine**19.433min (-0.006) 60654.00 ng****response 2890599**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.03
183.00	11.90	11.78
0.00	0.00	0.00